
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document


REVIEWER ACTIVITIES: ARMY - MD NAVY - AS, YD AIR FORCE - 82

USER ACTIVITIES:

FED. SUP CLASS
6640

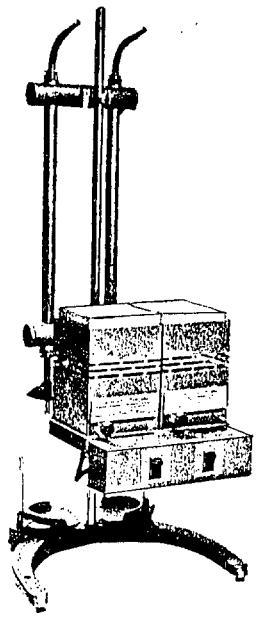

MS36199-1

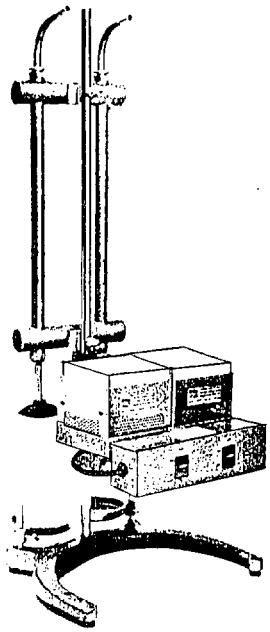

MS36199-2

PART NUMBER	W IN. (mm)	D IN. (mm)	H IN. (mm)	TYPE HEAT CONTROL
MS36199-1	12 (305)	14 (356)	36 (914)	Single Heat
MS36199-2	12 (305)	14 (356)	36 (914)	Rheostat
MS36199-3	Cancelled Without Replacement			

Ⓐ

MATERIAL: Frame, cast aluminum and formed steel; base, case iron; support rod, nickel plated steel; manifold, tubular copper; condenser, pure block tin; cooling tank, stainless steel; flask support, cast aluminum. Refractories shall be porcelain or other suitable material.

DESIGN: The apparatus shall accommodate two flasks, 500 and 800 mL capacity. The electrical heaters shall be nichrome wound type with 3-prong line cords. Part numbers MS36199-1 and MS36199-2 are 120V, AC/DC, 1.1 KW. The heater controls shall be as follows: Ⓐ

MS36199-1 Fixed, 550 watts
MS36199-2 Adjustable, 110 to 550 watts

FINISH: All metal parts shall have a baked enamel finish.

NOTES:
1. Furnish complete except glassware.
2. Items that vary in design but which otherwise conform to the requirements herein are considered one interchangeable Military Standard item.
Ⓐ 3. FSCMs: 22527 and 48619

APPROVED 07 FEB 1980 REVISED Ⓐ 27 MAR 1987

P. A.	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust EA MS, MB 99		DISTILLING APPARATUS, LABORATORY KJELDAHL, NITROGEN DETERMINATION twin-unit, electric	MS 36199
PROCUREMENT SPECIFICATION NONE	SUPERSEDES:		SHEET 1 OF 1

DD FORM 1 MAY 73 672-1 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE PROJECT NUMBER 6640-1415-4

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:36Z
Check the source to verify that this is the current version before use.