A-A-50805
April 17, 1981

COMMERCIAL ITEM DESCRIPTION

RACK, TEST TUBE, LABORATORY
Wintrobe, Enameled Steel, 10 Tube

This commercial item description shall be used in preference to Military Specification MIL-R-37624.

This commercial item description covers a laboratory test tube rack designed to accommodate ten Wintrobe hematocrit tubes in conjunction with determining sedimentation and hematocrit rates in blood samples.

Salient characteristics.

Design construction. The test tube rack shall consist of a steel base with three leveling screw legs, a spirit level, an aluminum frame with a plastic back plate and a chromium plated brass cross bar with spring activated pressure buttons. The top and bottom bar of the aluminum frame shall have 10 triangular notches to accommodate 10 hematocrit tubes in a perpendicular position. The notches in the bottom bar shall be numbered consecutively from 1 to 10. See Figure 1.

Workmanship. Workmanship shall be first class throughout. All metal parts shall be free of corrosion and shall be thoroughly cleaned of foreign particles (e.g., dirt, grease, and metal chips). The test tube rack shall be free of sharp edges, cracks, deformation, and other defects which detract from its appearance or impair its serviceability. The leveling screws and threaded members of the base shall perform properly. The finish on component parts shall be free of discontinuities and evidence of chipping and flaking.

Packaging and packing quantities. Unit. Each (EA.). Each rack as specified, constitutes one unit. Shipping containers shall contain six units.

Contractor certification. The contractor shall certify that product offered meets the salient characteristics of the description and conforms to the producers' own drawings, specifications, standards and quality assurance practices, and is the same product offered for sale in the commercial marketplace. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

FSC 6640

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:47Z
Check the source to verify that this is the current version before use.

Regulatory requirements. The offeror/contractor shall comply, and be responsible for compliance by their subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act and regulations promulgated thereunder, and the requirements of all other applicable Federal and State statutes and regulations.

Recovered materials. Offerors/contractors are encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging and packing. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and conforms to applicable carrier's rules and regulations.

NOTE: The following National Stock Number is covered by this document: 6640-00-010-8358.

Custodians:
Army - MD
Navy - MS
Air Force - 03


Preparing activity:
DoD - MB

Agent:
DLA - DM

54314

Project No. 6640-1094

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:47Z
Check the source to verify that this is the current version before use.

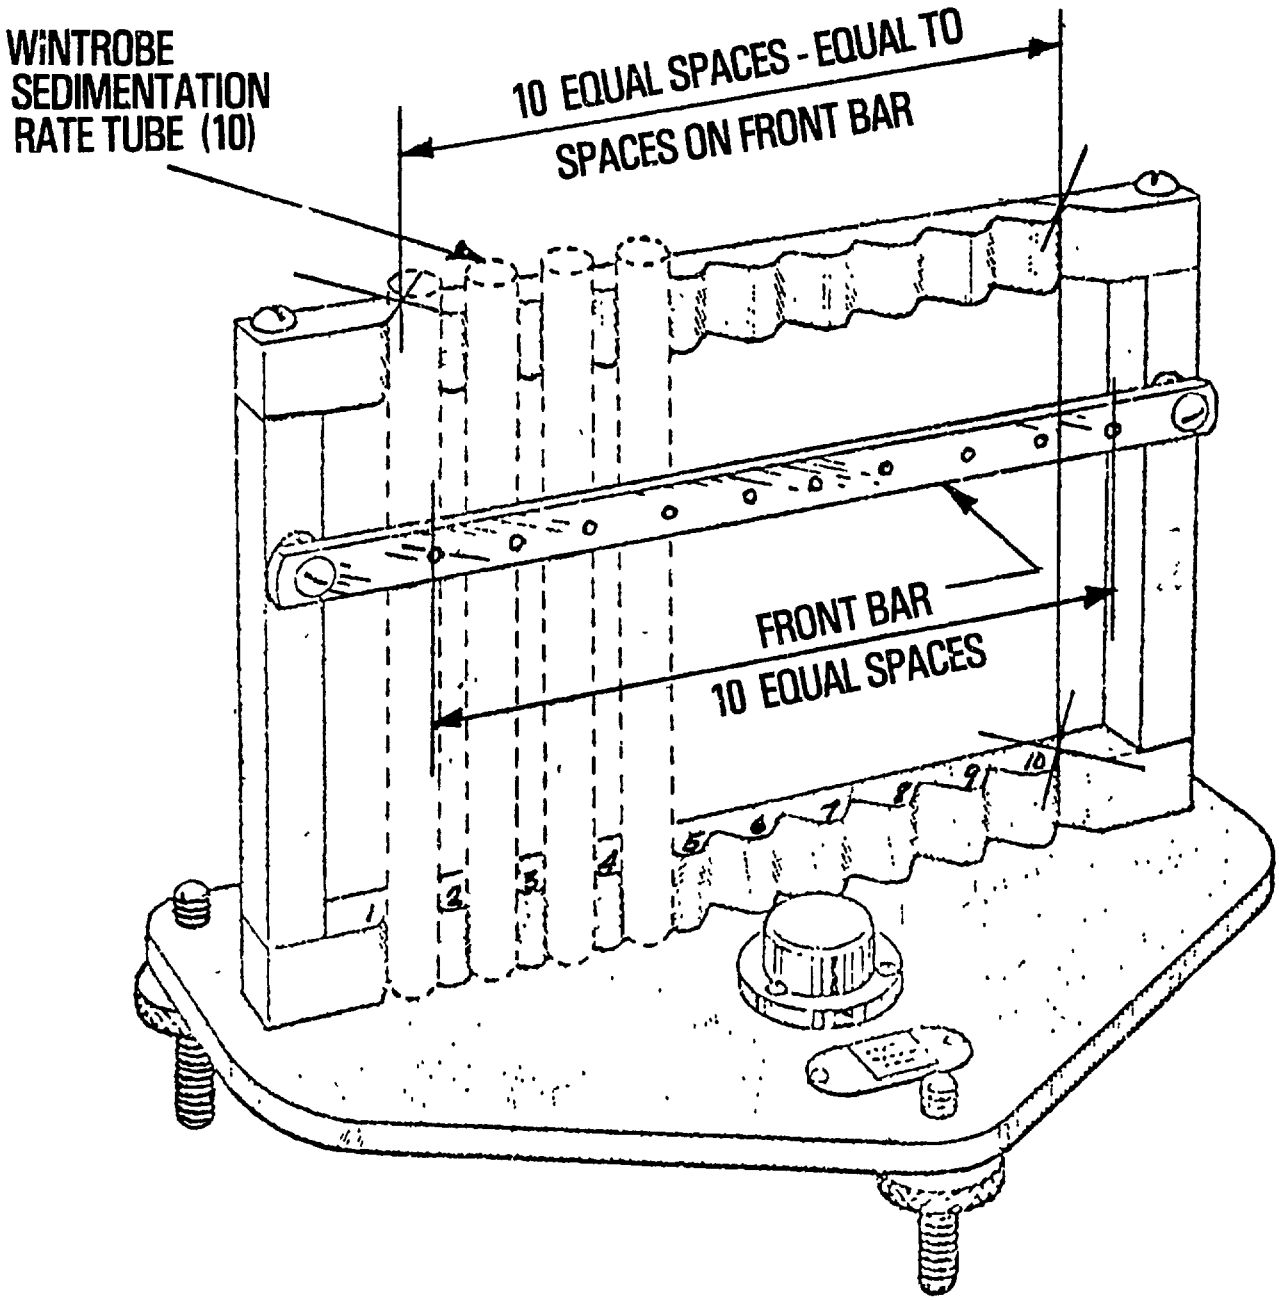

RACK, TEST TUBE, LABORATORY
Wintrobe, Enameled Steel, 10 Tube

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:47Z
Check the source to verify that this is the current version before use.