A-A-50826
30 July 1982

COMMERCIAL ITEM DESCRIPTION

TRAYS, INSERT, DENTAL INSTRUMENT AND SUPPLIES CABINET, Plastic

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-T-36754A.

This commercial item description covers plastic trays used as inserts in dental cabinets for containing various dental instruments and supplies.

The trays shall be furnished in the following style numbers, as specified:

16A, 17, 18, 19, 20.

Salient characteristics:

Style and design of trays shall be as shown in figure 1 for the style number specified. Trays shall be white and shall be fabricated of polypropylene or a polypropylene copolymer. Trays shall be shatter resistant, chip-proof, resistant to staining, odor-free, non-toxic, readily cleansable, and autoclavable at 270° F for 20 minutes. Trays shall have a smooth, glossy finish on all surfaces.

The No. 16A tray shall have two indented partitions with grooves running parallel with the length of the tray, separated by a minimum of a 2-inch free space at the center, with a minimum of a 2-inch free end section at both ends of the tray. The No. 16A tray shall accommodate long-handled and double-ended dental instruments.

The No. 17 tray shall have three equal size compartments with the dividers parallel to the width of the tray. The No. 17 tray shall accommodate rubber dam clamps and matrix bands.

The No. 18 tray shall have three equal size compartments with the dividers parallel to the length of the tray. The No. 18 tray shall accommodate assorted polishing strips.

The No. 19 tray shall be open with no compartments. The No. 19 tray shall accommodate foil carriers, pliers, and shears.

The No. 20 tray shall have six equal size compartments with a center divider parallel to the length of the tray and two dividers parallel to the width of the tray. The No. 20 tray shall accommodate disks, wheels, and stones.


The overall length of the trays shall be 8 +0 -1/8 inches; overall width, 4 +0 -1/8 inches; overall height, 13/16 to 1-1/8 inches; and inside depth, 5/8 ± 1/32 inch.

Workmanship. Trays shall be free from defects which detract from their appearance or impair their serviceability.


Unit. Each (EA). Each tray, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:47Z
Check the source to verify that this is the current version before use.


TRAYS, INSERT, DENTAL INSTRUMENT AND SUPPLIES CABINET, Plastic

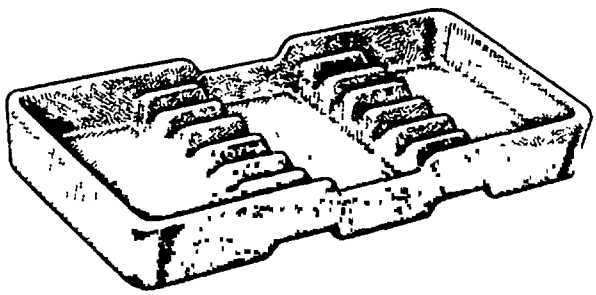


16A

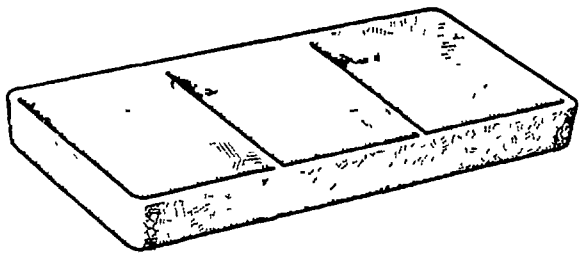


17

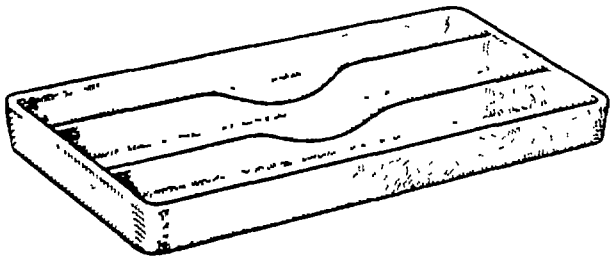

18

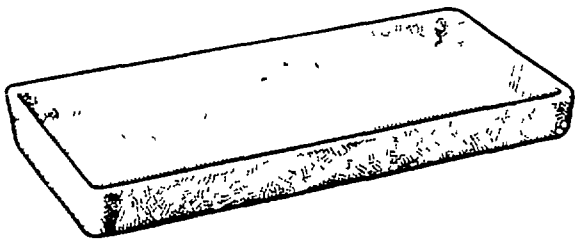

19

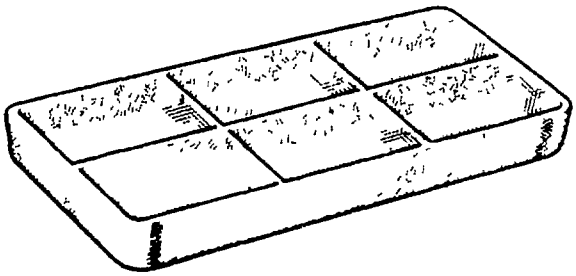

20

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:47Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets th salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices, and is the same as the produc sold in the commercial marketplace. The Government reserves the right to require proof c such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damag to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

For information only. The following products, as of the date of this document, are purported by the following companies to meet the salient characteristics of the items described herein:

Star Dental Mfg. Co.'s Product Nos: 31520(16A); 31530(17); 31540(18); 31550(19); 31560(20).

Palmero Dental Products' Product Nos: 1508(16A); 1508(17); 1508(18); 1508(19); 1508(20).

Zirc Dental Products' Product Nos: 20Z201(16A); 20Z203(17); 20Z204(18); 20Z205(19); 20Z206(20).

NOTE: The following National Stock Numbers are covered by this document:

NSN	Style No.
6520-00-435-3076	16A
6520-00-435-3077	17
6520-00-435-3078	18
6520-00-435-3079	19
6520-00-435-3080	20

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:47Z
Check the source to verify that this is the current version before use.

A-A-50826

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

95544

Project No. 6520-1606

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:47Z
Check the source to verify that this is the current version before use.