A-A-54280
14 November 1990

COMMERCIAL ITEM DESCRIPTION

SPECULUM, SIGMOID (Plastic, Disposable)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a disposable, plastic sigmoid speculum suitable for examining the sigmoid or flexure portion of the colon.

Salient characteristics:

General. The speculum shall consist of a protective distal end sleeve, inner tube, an obturator, and a transparent light-conducting outer tube graduated in 1 cm intervals and numbered graduations every 5 cm. The outer tube shall have a twist lock for connecting to the sigmoidoscope. The speculum shall be compatible with a sigmoidoscope consisting of a fiber optic light head with plano or magnifying cover, an insufflator connector for attaching to an insufflator assembly, a cord assembly with a high intensity halogen lamp, swivel magnifying lenses, and transformer with cord (See Note 2).

Material. The outer tube shall be fabricated from rigid transparent plastic. The sleeve shall be fabricated from rigid white plastic. The inner tube shall be fabricated from rigid plastic. The rigid plastic inner tube may be black. The obturator shall be fabricated from rigid transparent plastic.

Biological suitability. The outer tube, obturator and sleeve shall be biologically suitable when tested in accordance with applicable requirements of the USP for Class II plastics.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:32Z
Check the source to verify that this is the current version before use.

Finish. All exposed surfaces of the assembled speculum contacting the patient shall be smooth, with no sharp edges. The outer tube surfaces shall be free from nicks or flaws which would create light loss through internal reflection. The inner surface of the sleeve, which extends beyond the outer tube, shall have a high gloss finish. The inner wall of the inner tube shall have a non-gloss finish.

Style, design and dimensions. The distal end of the obturator shall protrude a minimum of 15 mm past the end of the sleeve when assembled and shall have no gap between the distal end of the obturator and end of the sleeve greater than 1.5 mm. The speculum shall be in accordance with Figures 1 and 2.

Requirements. The locking ring on the proximal end of the outer tube shall match the speculum mount on the light head of the sigmoidoscope. When the speculum is firmly attached to the light head with the lens cover closed, the end surface of the inner tube shall be in close contact with the seal ring of the cover. With the speculum attached to the light head and illuminated, the scales and numbers shall be clearly illuminated.

Workmanship. The speculum shall be free from defects which detract from its appearance or impair its serviceability.

Product Quality Level.

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements.

Unit. Package (PG). One package containing ten individually packaged, clean speculum packaged in a suitable container, as specified, constitutes one unit

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 with an Inspection level of S-2 and an AQL of 1.0 (percent defective). The unit of product for examination purposes shall be one speculum.

Examination. Examination shall be conducted to determined compliance with specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. At an Inspection level of S-2, the AQL shall be 1.0 (percent defective). The unit of product for test purposes shall be one speculum.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:32Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-094-8293	SPECULUM, SIGMOID, Plastic, 9.84 inches (25 cm) Long, Disposable, 10s

NOTE 2: The speculum shall be compatible with a Sigmoidoscope, with Disposable Speculum, 115 Volt, 60 HZ, AC (NSN 6515-01-094-8295).

Ordering data (Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 47087

Project No. 6515-4269

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

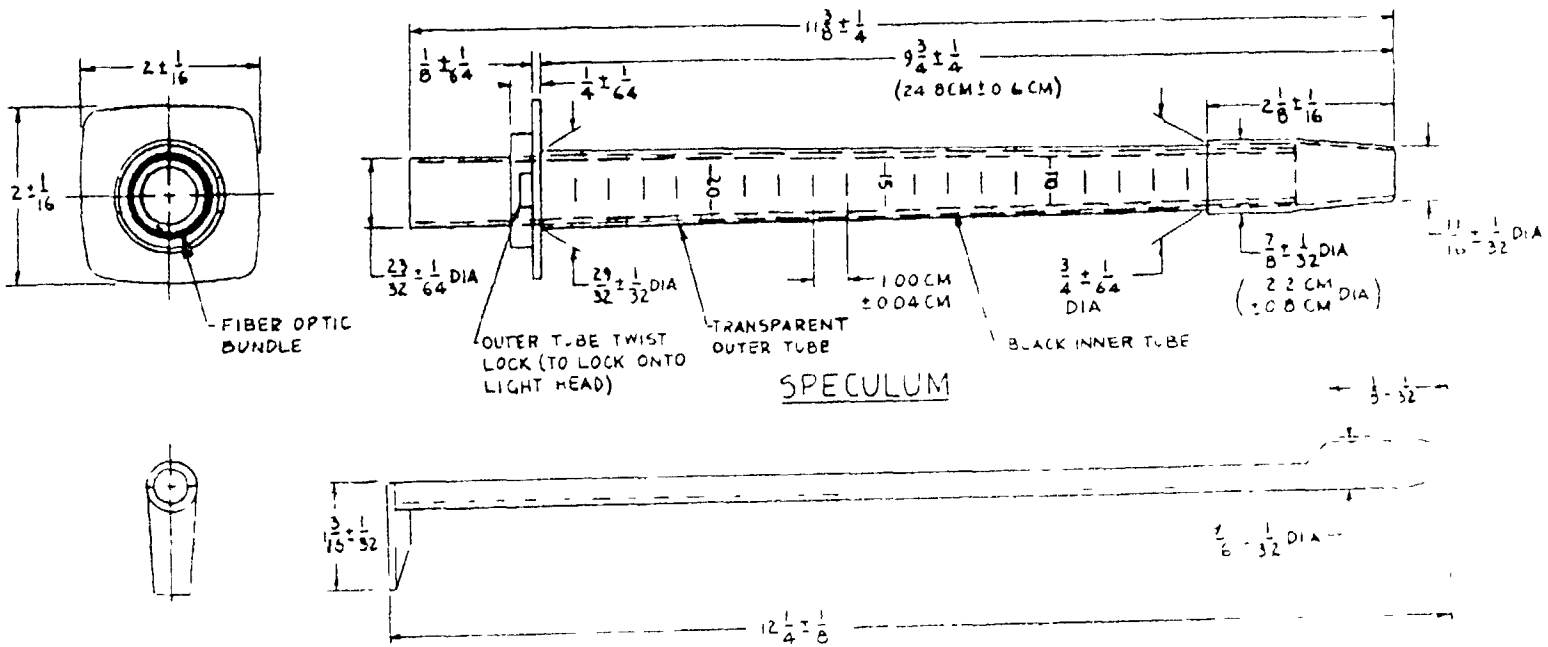

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/32	±	±

FIGURE 1. SPECULUM, SIGMOID, PLASTIC, DISPOSABLE

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:32Z
Check the source to verify that this is the current version before use.

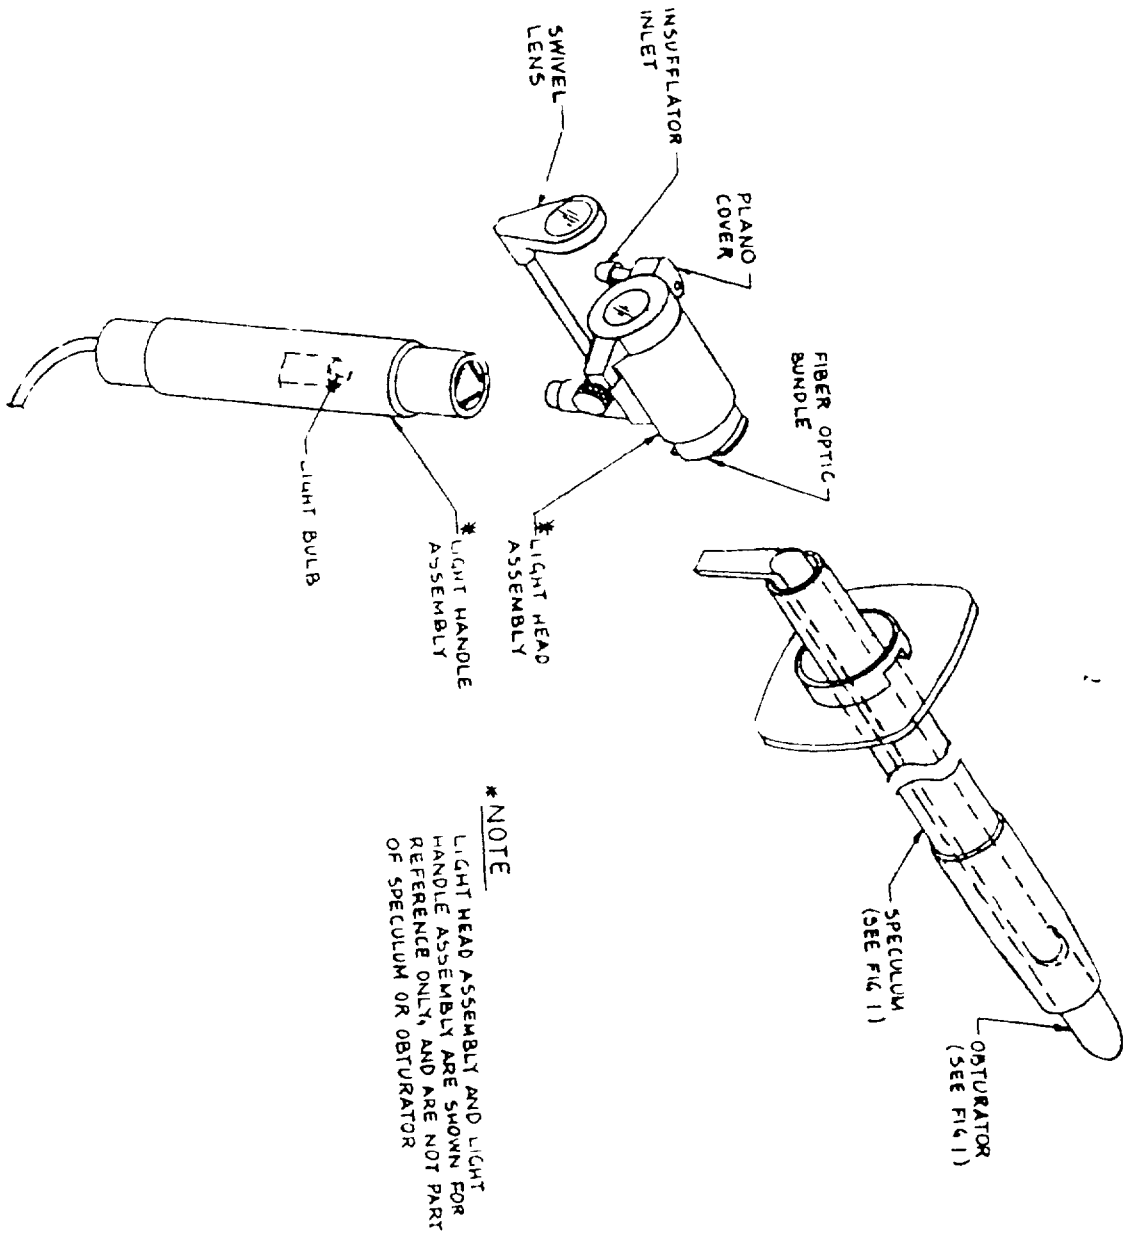


FIGURE 2 FIBER OPTIC ILLUMINATION SYSTEM

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN DPSC-RSTP
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-54280	SPECULUM, SIGMOID (Plastic, Disposable)

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI – Optional)*	b. WORK TELEPHONE NUMBER *(Include Area Code – Optional)*
c. MAILING ADDRESS *(Street, City, State, ZIP Code – Optional)*	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITIONS ARE OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:32Z
Check the source to verify that this is the current version before use.