COMMERCIAL ITEM DESCRIPTION

ADAPTER, CATHETER TO LUER SYRINGE

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a metal adapter suitable for connecting a size 6 French, flared catheter to the tip of a Luer-lock syringe.

Salient characteristics:

Shall be a catheter to Luer syringe adapter meeting the requirements listed below.

Material. Adapters shall be fabricated from a suitable brass, properly tempered.

Style and design. The style and design of the adapters shall be in accordance with Figure 1. The adapters shall have a fitting body and a backing collar. The adapter body shall contain a female Luer lock conforming to ANSI/HIMA MD70.1. The adapter body shall also contain the male end of a 45-degree flare fitting with 1/4-32 N.E.F. machine threads. The backing collar shall contain the female end of a 45-degree flare fitting with 1/4-32 N.E.F. machine threads. The exterior of the backing collar shall have a ridged finger-grip area.

Performance. Adapters shall effect a leak-tight connection between a Luer-Lock syringe and a size 6 French catheter that was suitably neat-flared prior to insertion in the adapter. Adapters shall pass the performance testing specified herein.

Finish. Adapters shall be nickel-plated on all surfaces. Plating shall conform to QQ-N-290. Except for the finger-grip, adapters shall have a smooth finish overall.

Workmanship. The adapter shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One adapter, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one Catheter-to-Luer Syringe Adapter.

Testing requirements. Adapters shall be subjected to the following tests

Corrosion-resistance. Corrosion-resistance of adapters will be determined by the salt-spray and boil-test methods in Federal Specification QQ-I-526.

For the salt-spray test, the exterior of the adapter shall be considered a significant surface. Each piece of the adapter must be tested separately.

Dimensional testing. Test adapters in accordance with Section 7 of ANSI/HIMA MD70.1, "Dimensional Test for Luer-Lock Fittings".

Performance testing. Test adapters as follows. Prepare for testing by heat-flaring a size 6 French catheter with a 45° flaring mandrel. Check the catheter for proper flare depth and angle. Connect the adapter and close the catheter with a suitable pinch-clamp. Perform the test specified in section 8 of ANSI/HIMA MD70.1, "Performance Tests for Luer-Lock Fittings".

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE. This document covers the following National Stock Number:

NSN	ITEM IDENTIFICATION
6515-01-164-8870	ADAPTER, CATHETER TO LUER SYRINGE

MILITARY INTERESTS

Custodians.

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY.

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-CSS

52804

Project No. 6515-3282

S1-8-2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

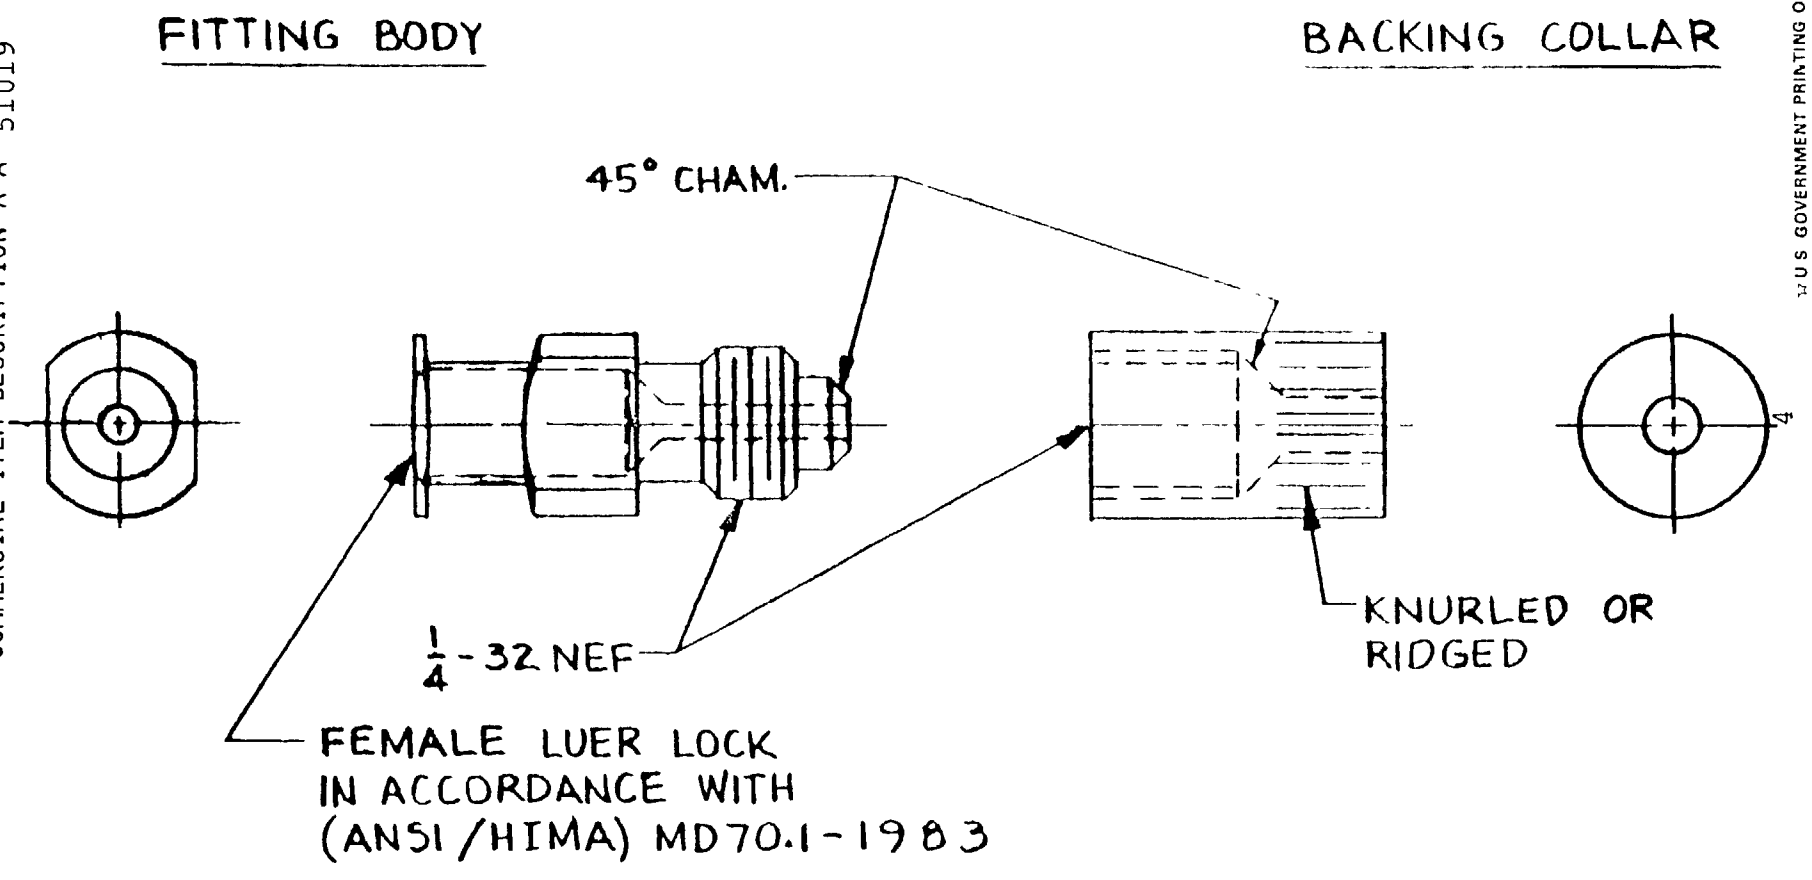


FIGURE 1 ADAPTER, CATHETER TO LUER SYRINGE

U S GOVERNMENT PRINTING OFFICE 1986 — 605 036/40742

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.