A-A-51023
15 October 1985

COMMERCIAL ITEM DESCRIPTION

PROTECTOR, DENTURE MODEL, Foamed Plastic, Three-piece

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-P-37500.

This commercial item description covers a foamed plastic protector suitable for the receipt and protection of dental models and appliances.

Salient characteristics:

The protector shall be of three-piece construction, a top piece, bottom piece and a center-piece, all separate and preformed. The top and bottom pieces shall be preformed into rectangular blocks. The center piece shall be preformed into the shape of a rectangular block having two rectangular shaped holes through the entire thickness. Style, design and dimensions of the protector shall be as shown in figure 1. The protector shall be fabricated from high quality polyurethane foam. The protector shall be a device suitable for repeated use in protecting dental models and appliances during shipment of these models and appliances between laboratories. The protector shall be free from any objectionable odor.

The protector shall have a maximum constant deflection compression set of 10 percent, an indentation load deflection of 28 to 35 pounds, a density of 1.20 $\pm$ 0.05 pounds per cubic foot, a tensile strength 10.0 pounds per square inch, a minimum elongation of 150 percent and a minimum resilience of 40 percent. All tests shall be performed in accordance with the American Society for Testing and Materials (ASTM) Designation D3574, Standard Methods of Testing Flexible Cellular Materials - Slab, Bonded and Molded Urethane Foams. The issue of the ASTM standard in effect on the date of the solicitation shall be used to determine compliance with stated requirements.


Workmanship. Protector shall be free from defects which may detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing one hundred (100) three-piece protectors, as specified, constitutes one unit.

FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

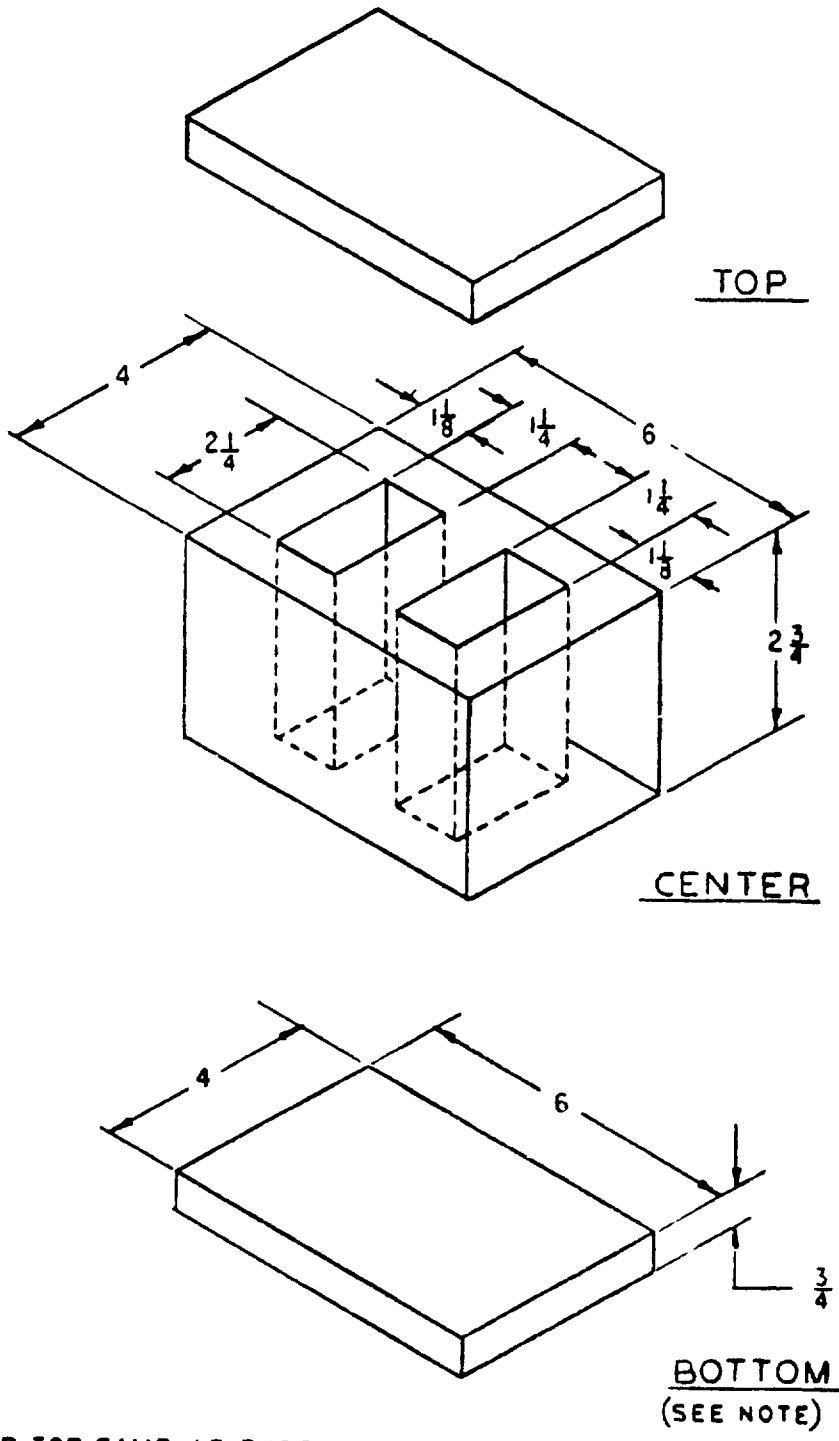

NOTE:
DIMENSIONS FOR TOP SAME AS THOSE SHOWN FOR BOTTOM

Dimensions are in inches.
Unless otherwise specified, tolerances shall be as follows:

Dimensions 2 inches and above ± 1/4.
Dimensions under 2 inches ± 1/8.

Figure 1. Protector, Denture Model.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one protector. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6520-00-142-8727	PROTECTOR, DENTURE MODEL, Foamed Plastic, Three-Piece.

Ordering data. Intermediate/exterior package quantities, labeling and marking must be as specified in the contract and/or order.

MILITARY INTEREST:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:
DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

47444

Project No. 6520-1810

Location S2-8-14

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.