A-A-51036
20 September 1985

COMMERCIAL ITEM DESCRIPTION

ADAPTER, CATHETER TO LUER SYRINGE, Small Lumen

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a metal adapter suitable for connecting small-lumen catheters to Luer-Lock syringes.

Salient characteristics:

Shall be a metal adapter with a female Luer Lock on one end and a ribbed, tapered fitting on the other end to form the secure connection of small-lumen catheters to Luer-Lock syringes.

Material. The adapters shall be fabricated from chromium over nickel plated copper alloy. The plating and corrosion tests shall be as specified in Federal Specification GG-I-526.

Style and design. The adapter shall allow the attachment of various small-lumen catheters. The catheter end shall have a tapered, ribbed construction.

The other end shall be a female Luer-Lock connector for the attachment of Luer-Lock syringes. The female Luer-Lock shall conform to the American National Standards Institute/Health Industry Manufacturers Association (ANSI/HIMA) MD 70.1. The adapter shall be in accordance with Figure 1.

Performance. The adapters shall provide a leak-tight connection between the catheter and a Luer-Lock syringe. The material, Luer-Lock performance, and adapter leak-tightness tests are specified herein.

Finish. The adapters shall be smooth, with a mirror or matte finish, except for the knurled portion.

Workmanship. The adapter shall be free from defects which detract from its appearance or impair its serviceability.

PRODUCT QUALITY LEVEL

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Unit. Each (EA). One adapter, as specified, constitutes one unit of issue.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one adapter.

Testing requirements. Adapters shall be subjected to the tests specified herein.

Corrosion-resistance. The corrosion-resistance of the adapter shall be determined by the Boil Test contained in GG-I-526.

Dimensional testing. The dimensional testing of the adapter shall be in accordance with Figure 1 and ANSI/HIMA MD70.1.

Luer-Lock performance. The adapter Luer Lock shall be tested in accordance with Section 8 of ANSI/HIMA MD70.1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

Adapter performance. A catheter of proper style shall be placed on the tapered end of the adapter. The catheter shall be closed with a pinch-clamp and tested in accordance with Section 8 of ANSI/HIMA MD70.1. The adapter shall not leak at a pressure of 20 pounds per square inch (psi) for 2 minutes, or 45 psi for 30 seconds.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6515-01-139-8759

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51036

Custodians:

Army-MD
Navy-MS
Air Force-03

Preparing Activity:

DoD-MD

Agent:

DLA-DM


CIVIL AGENCY COORDINATING AGENCY:

VA-OSS

Project No. 6515-3406

Location S1-9-9

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.

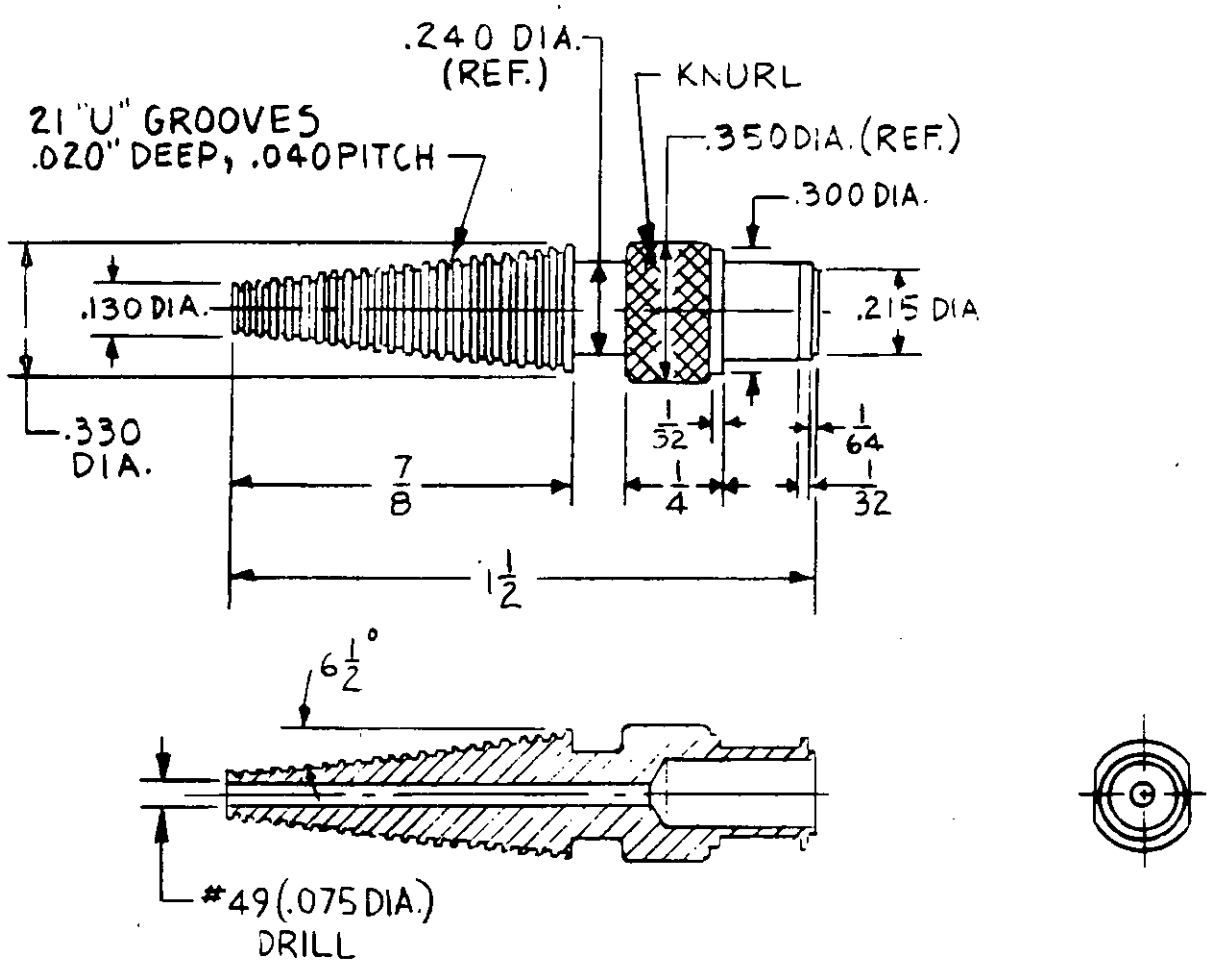

NOTES:

1. ROUND OFF ALL SHARP CORNERS.
2. FEMALE LUER LOCK FITTING DIM. SHALL BE IN ACCORDANCE WITH ANSI/HIMA MD 70.1-1983.

FIGURE 1 ADAPTER, CATHETER TO LUER SYRINGE, SMALL LUMEN

☆U.S. GOVERNMENT PRINTING OFFICE: 1986 — 605-036/40745

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:49Z
Check the source to verify that this is the current version before use.