COMMERCIAL ITEM DESCRIPTION

MALLET, ORAL SURGERY,
Hand Type, Mead

The General Services Administration has authorized the use of this commercial item description in preference to Federal Specification GG-M-105D.

This commercial item description covers a mallet for use in oral surgery.

Salient characteristics:

The mallet shall be of Mead design as shown in figure 1 and shall be suitable for use in oral surgical procedures. The mallet shall consist of a handle, head, two retaining rings, and two disks.

The handle shall be securely attached to the head by means of a suitable steel pin along the major axis of the head. The gripping portion of the handle shall be enlarged and convexly contoured to fit the hand. The neck of the handle shall be round.

The head shall be threaded at both ends, have a round cross-section, and accommodate the retaining rings.

The retaining rings shall be threaded and shall fit either threaded end of the head. The outer cylindrical surface of the rings shall be knurled for easy removal.

The disks shall sit securely, without wobble, on either end of the head when the retaining rings are in place. The exposed surfaces shall be slightly convex. Two spare disks shall be furnished with each mallet.

Dimensions of the mallet shall be as follows:

Overall length	6 ± 1/8 inches
Overall head length	2 $\mp$ 1/8, -0 inches
Head diameter (rings)	1 ± 1/32 inch
Disk thickness	5/16 ± 1/32 inch
Handle dimensions at maximum curvature:	
Width	14.68 ± 0.04 mm
Height	22.48 ± 0.04 mm
Handle diameter at head	7.93 mm (Ref.)

The mallet shall be autoclavable.

Material. The handle and disks shall be fabricated of solid, general purpose, polyhexamethyleneamide (nylon). The head and retaining rings shall be fabricated from type 416 martensitic stainless steel in accordance with Federal Specification GG-I-526b, dated October 11, 1965.

FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

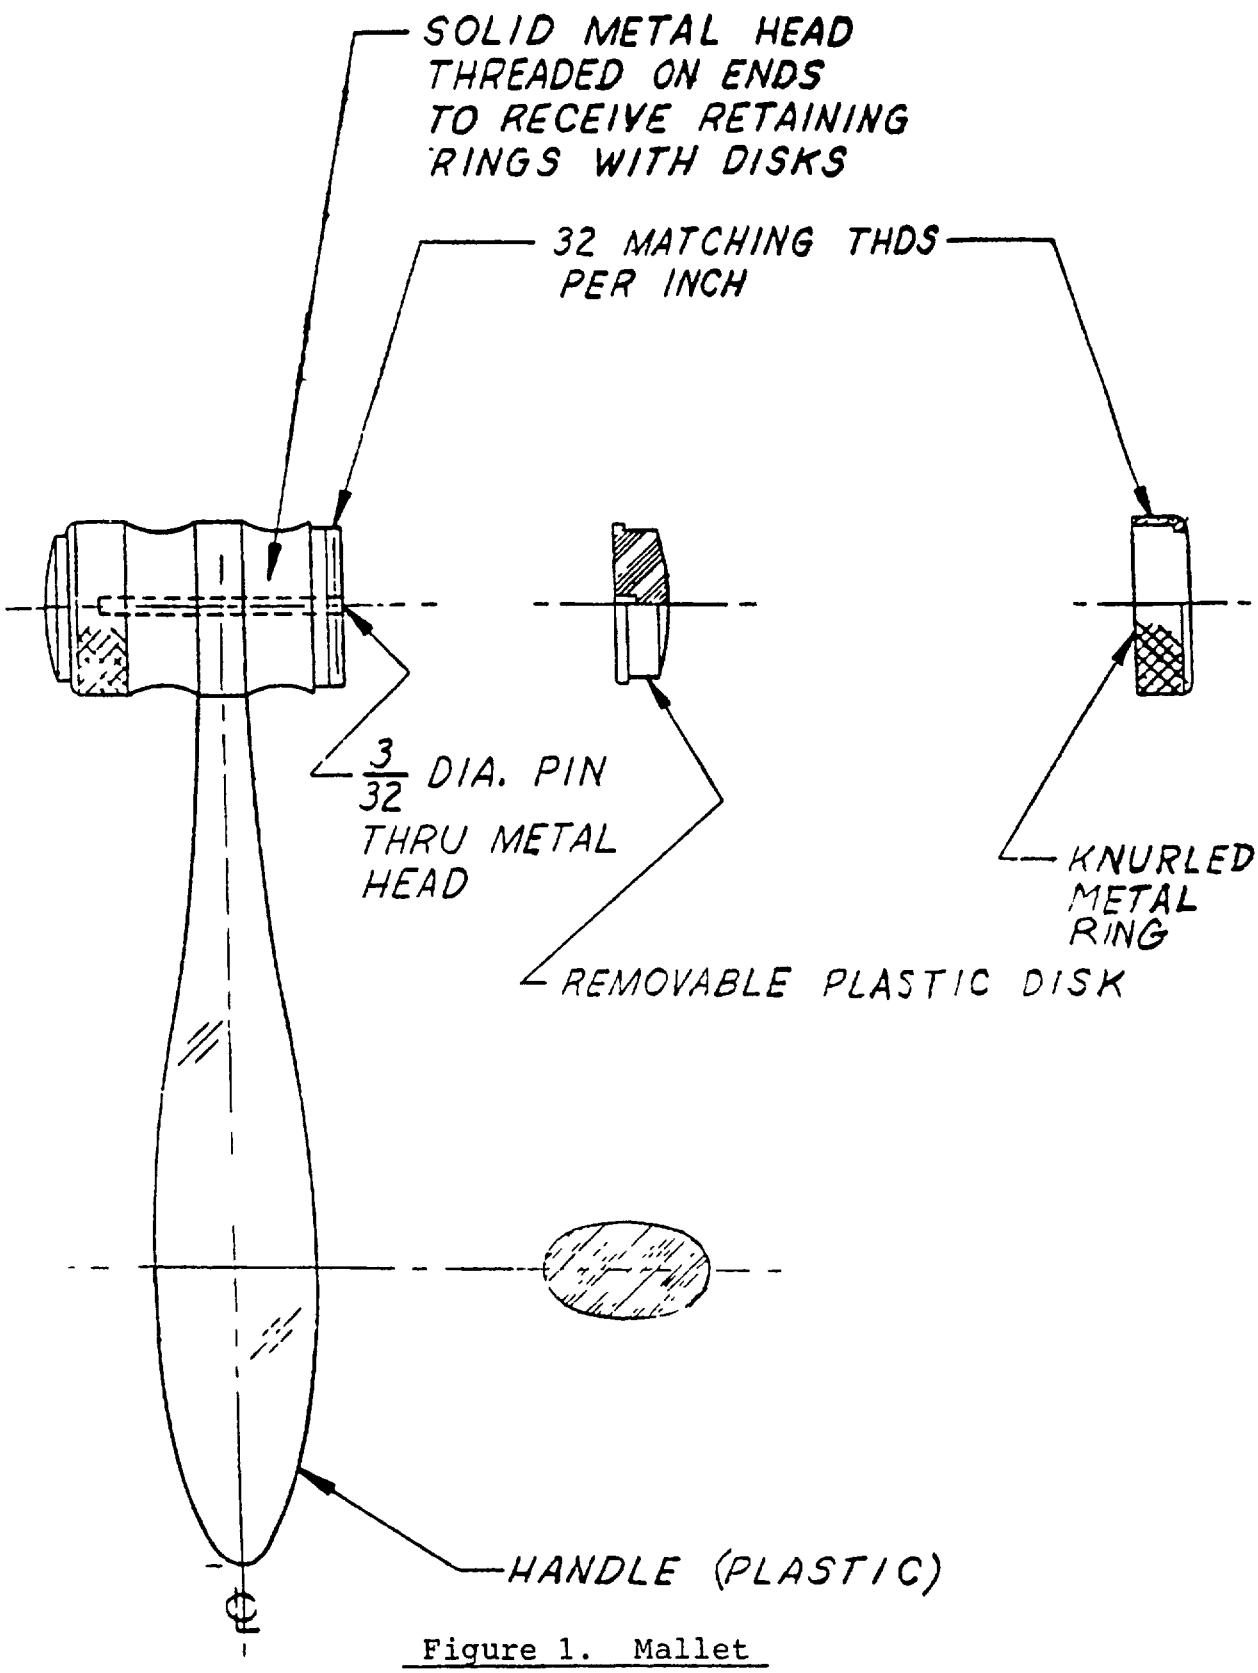


Figure 1. Mallet

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Finish. The handle and exposed surfaces of the disks shall be polished. The head shall have a mirror or satin finish.

Workmanship. The mallet shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). Each mallet, with two spare disks, as specified, constitute one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one mallet. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6520-00-540-2050 MALLET, ORAL SURGERY, Hand Type, Mead

Ordering data. Intermediate/exterior package quantities, labeling and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

48069

Project No. 6520-1861

Location S2-11-18

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.