A-A-51061
21 October 1985

COMMERCIAL ITEM DESCRIPTION

BUR, DENTURE TRIMMING (STRAIGHT HANDPIECE, TUNGSTEN CARBIDE)

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-B-37811A.

This commercial item description covers three head shapes of tungsten carbide denture trimming burs for use in dental straight headpieces, in the following shapes, as specified.

-Flame
-Pear
-Round

Salient characteristics:

Material. The bur head shall be made of cemented tungsten carbide with a cobalt binder. The shank shall be made of AISI 4130 or 4340 steel.

Description. The bur shall be for use in dental straight handpieces for trimming, carving, and finishing acrylic, chromium alloy, and gold alloy appliances. The bur shall be furnished in the shape as specified. The bur shall be of two-piece construction and shall consist of a carbide head securely and permanently welded or brazed to a steel shank. The bur head shall have 18-20 right hand flutes and shall have a finely honed finish with sharp blades. The blades shall be shaped and sharpened to cut at the tip as well as the side of the bur head and to provide automatic chip clearance. The shanks shall be straight and have a smooth bright finish. The total runout of the bur shall be less than 0.003 inch. The bur head shall have a Rockwell hardness of A90 to A92 and the bur shank shall have a Rockwell hardness of C43 to C48. The bur shapes and dimensions shall be as shown in figure 1.

Cutting test. Eighteen half-inch cuts shall be made in a 0.020 inch thick brass strip (Brinell hardness 74-81) at 12,000 revolutions per minute and a 2 pound load. The time required to cut the eighteenth one-half inch shall be no more than 2.25 times the time required to cut the second one-half inch. In addition, the bur shall show no breakage, bending, or head separation as a result of the test.

Workmanship. The bur shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One bur of the shape specified, packaged in a plastic vial, constitutes one unit.

FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

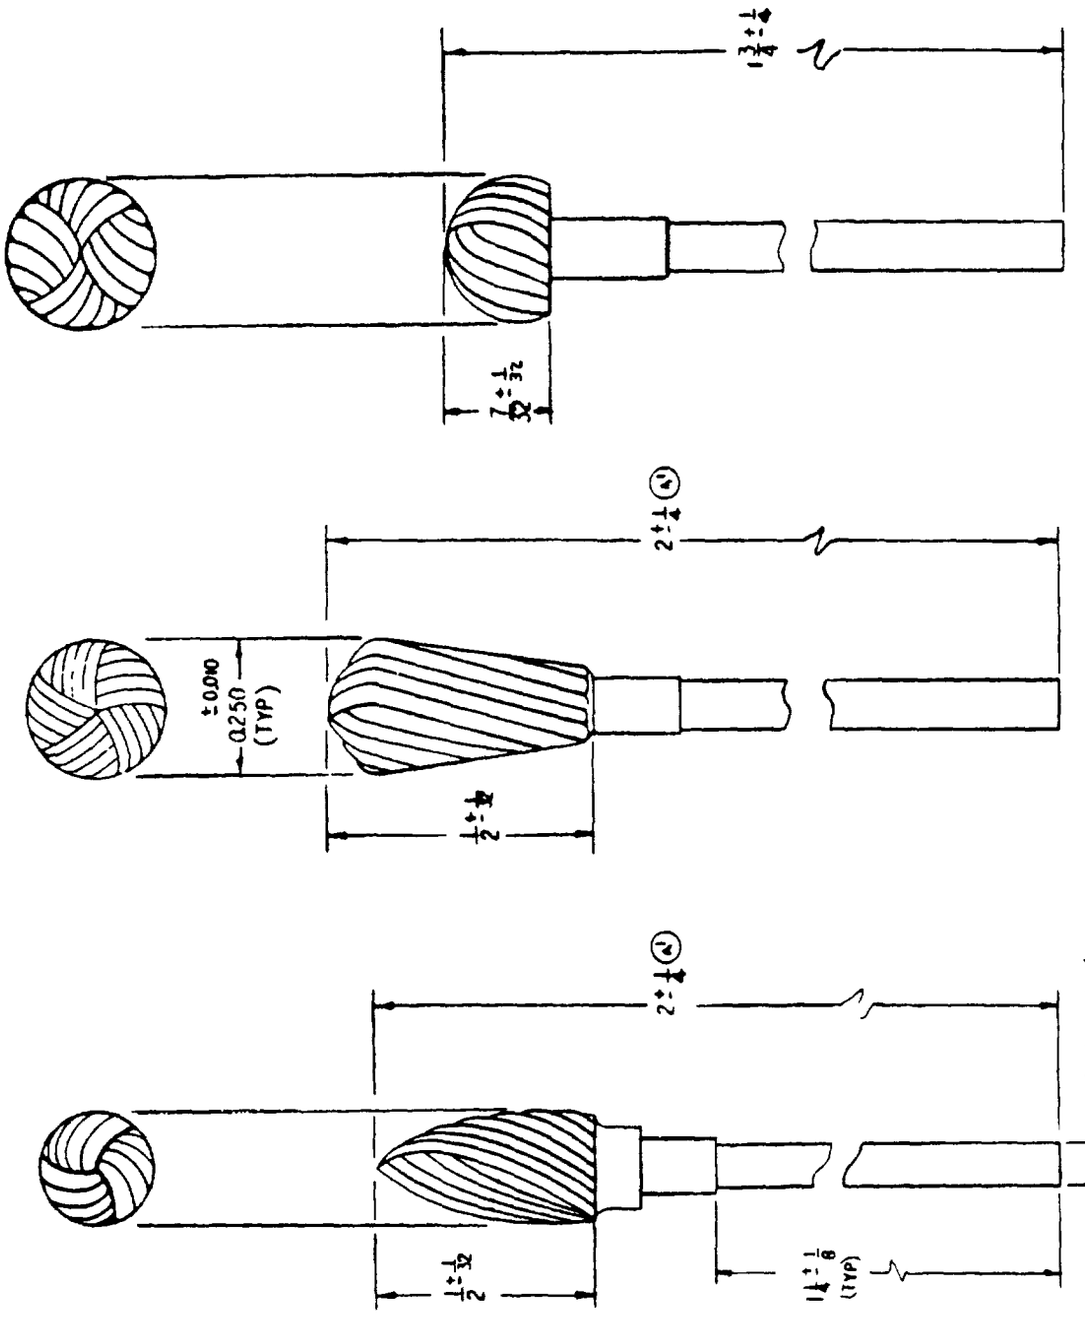


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspections. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item. Inspection shall be conducted to determine compliance with specification requirements.

Sampling for insection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more test characteristics. The unit of product for inspection purposes shall be one bur. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

6520-01-027-0344	BUR, DENTURE TRIMMING, Straight Handpiece, Tungsten Carbide: Flame.
6520-01-027-0345	BUR, DENTURE TRIMMING, Straight Handpiece, Tungsten Carbide: Pear.
6520-01-027-0346	BUR, DENTURE TRIMMING, Straight Handpiece, Tungsten Carbide: Round.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

AGENT:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

05858

Project No. 6520-1759

Location S2-11-4

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.