A-A-51066
20 December 1985

COMMERCIAL ITEM DESCRIPTION

IRRIGATION SET, UROLOGICAL, Single Port, Sterile, Disposable

The General Services Administration has authorized the use of this commercial item description

This commercial item description covers sterile, disposable, plastic single port urological irrigation sets for use in performing a cystoscopy and irrigation of the bladder

Salient characteristics

General. The urological irrigation set shall be a sterile, plastic, disposable, single port irrigation set suitable for irrigating the bladder and performing a cystoscopy.

Characteristics. The urological irrigation set shall have an overall length of 78 plus or minus 4 inches. The assembly of the urological irrigation set shall be structurally sound and shall not leak air or fluid during use.

The tubing shall have an ID of 0.30 plus or minus .064 inches. Each urological irrigation set shall have a cylindrical spike with a 0.181 plus or minus 0.006 inch ID at the proximal end of the tubing. The cylindrical spike shall facilitate connection to an irrigating container via an entry port. A clear flexible drip chamber shall be permanently attached in a leakproof manner to the tubing below the cylindrical spike.

A tapered male connector shall be supplied at the distal end of the tubing. The male connector shall have a total length of 1.35 plus or minus 0.07 inches. The connector shall be tapered at the distal end. The connector width shall vary from 0.410 plus or minus 0.010 inches, one inch from the distal end to 0.395 plus or minus 0.005 inches at the distal end. This male connector shall be compatible with a catheter and a catheter adapter.

A detachable, flexible sleeve shall be supplied at the distal end of the male connector. This sleeve shall facilitate direct connection of the urological irrigation set to a cystoscope.

A control clamp shall be provided on the tubing and be a roller type clamp from which the roller cannot be accidentally removed. The clamp shall regulate fluid flow from complete shut off to maximum flow. The clamp shall be supplied on the tubing in the open position and shall provide a constant setting and quick shut off from the operating position. The clamp shall be movable and shall be capable of one-handed operation. To assure constant delivery of fluid, it shall be impossible for the clamp setting to be changed drastically by an accidental jerk on the tubing. Each clamp shall be capable of accomplishing a complete, quick shut off (i.e., no falling drop in the drip chamber).

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release, distribution is unlimited.

'AMSC N/A'

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Roller flow clamp tests. The clamp shall be operated ten times from its fully opened position to complete shut off while the clamp is in the same position on the tubing. The tubing shall not be cut, pierced, or otherwise damaged so as to cause leakage or restriction of fluid flow.

The roller clamp shall be removed from the set together with a piece of tubing one inch longer than the clamp body. The tubing shall be present in the roller clamp in its normal position with a 1/2 inch length extending from each end of the roller clamp. The clamp (see Figure 1) shall be held vertically, with the large end down, over a supporting gap so that the roller, if forced out of the body, is free to fall. A polished steel tongue is applied to the top of the roller. The roller shall be able to rotate during the test. The vertical downward force required to separate the roller from the clamp body is measured. As an alternate, any position of the clamp is acceptable as long as the clamp body is not distorted and the load measurement is accurate. The clamp body shall be capable of withstanding a 3.65 kilogram load when tested without the roller separating from the body of the clamp.

Material. The tubing shall be fabricated from clear, colorless, flexible plastic. The material may be polyvinylchloride. The roller flow clamp shall be made from rigid plastic. The flexible sleeve shall be latex rubber.

Sterility. Each urological irrigation set shall be sterilized in accordance with USP.

Toxicity. The urological irrigation set shall meet any applicable FDA requirements for safety and toxicity for invasive and implantable devices.

Workmanship. The urological set shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package, containing forty-eight (48) irrigation sets, each set individually packaged sterile in a sealed peel-open type container, constitutes one unit.

Quality Assurance Provisions

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests Tests shall be conducted to determine compliance with specification requirements Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. AQL shall be 1.0 percent defective. Inspection level shall be S-2 The unit of product for test purposes shall be one irrigation set

Contractor certification The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements

Federal Food, Drug and Cosmetic Act If the product covered by this document has been determined by the U S Food and Drug Administration to be under its jurisdiction, the offeror contractor shall comply, and be responsible for compliance by its subcontractors suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations

Recovered materials The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE The following National Stock Number (NSN) is covered by this document:

6515-00-198-5446

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51066

Custodians.

Army-MD
Navy-MS
Air Force-Cs

Preparing Activity

DoD-MB

Agent

DLA-DH

CIVIL AGENCY COORDINATING ACTIVITY


VA-OSS

50989

Project No 6515-Cs21

Location S1-9-15

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

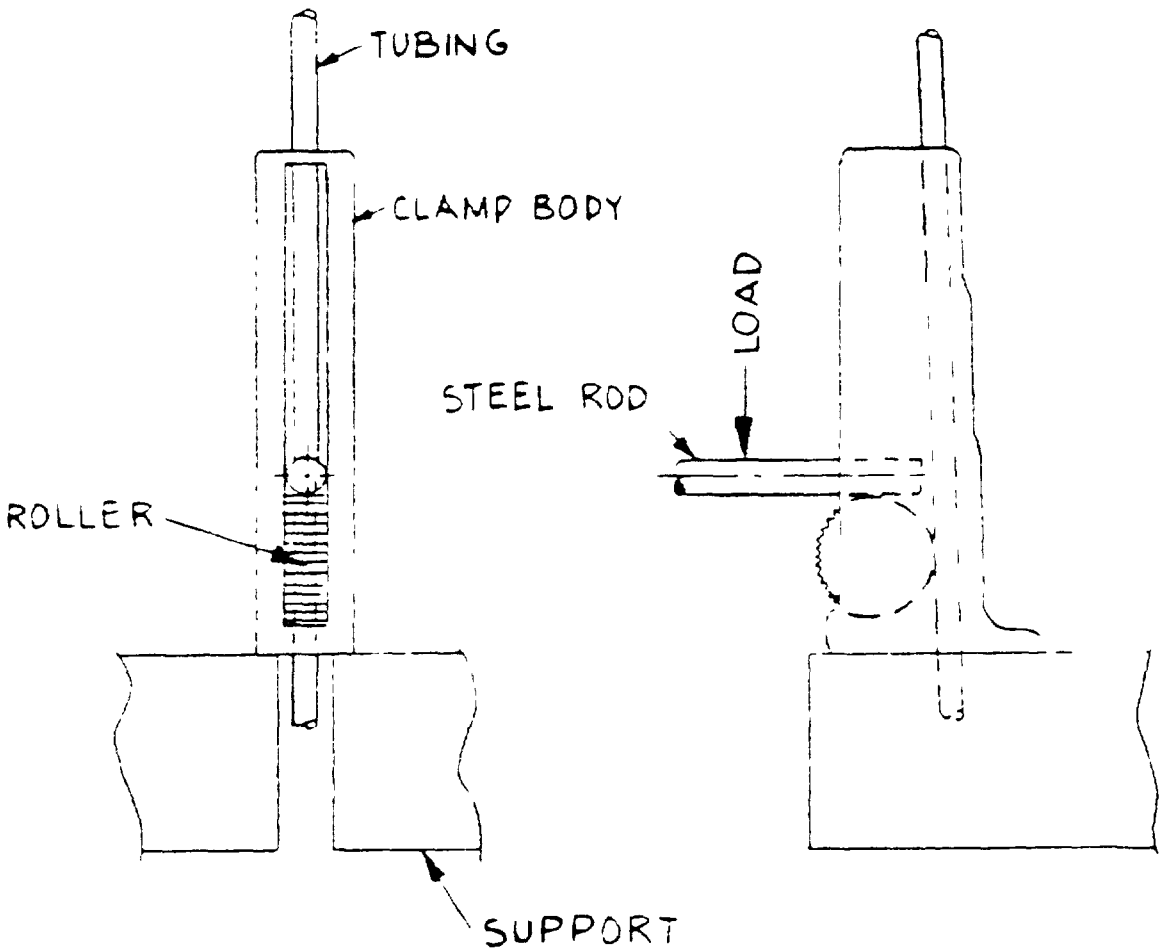

METHOD OF APPLYING LOAD TO ROLLER

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.