A-A-51072
16 October 1985

COMMERCIAL ITEM DESCRIPTION

DISH, MEDICAMENT, DENTAL

The General Services Administration has authorized the use of this commercial item description in preference to Interim Federal Specification DD-M-00200b (DSA-DM), Type II.

This commercial item description covers a dish suitable for holding medicaments or polishing materials.

Salient characteristics:

The dish shall be of design and dimensions as shown in Figure 1. The dish shall be hexagonal, octagonal, or decagonal in shape and shall have a concavity in the upper and lower surfaces. The dish shall show no evidence of corrosion, chipping, scumming or cracking when boil tested as specified herein. The dish shall show no evidence of cracking when tested for thermal resistance as specified herein. The large cavity of the dish shall have a capacity of 4.5 milliliters (ml), minimum. The small cavity shall have a capacity of 1.5 ml, minimum. The dish shall be free of open bubbles on working surfaces. The dish may have slightly concave outer sides.

Material. The dish shall be fabricated of colorless, transparent, flint glass of a quality that will retain its luster and transparency.

Workmanship. The dish shall be free from cracks, chips, or sharp edges. The glass shall be free of striae, bubbles, or other imperfections.

Unit. Each (EA). One dish, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

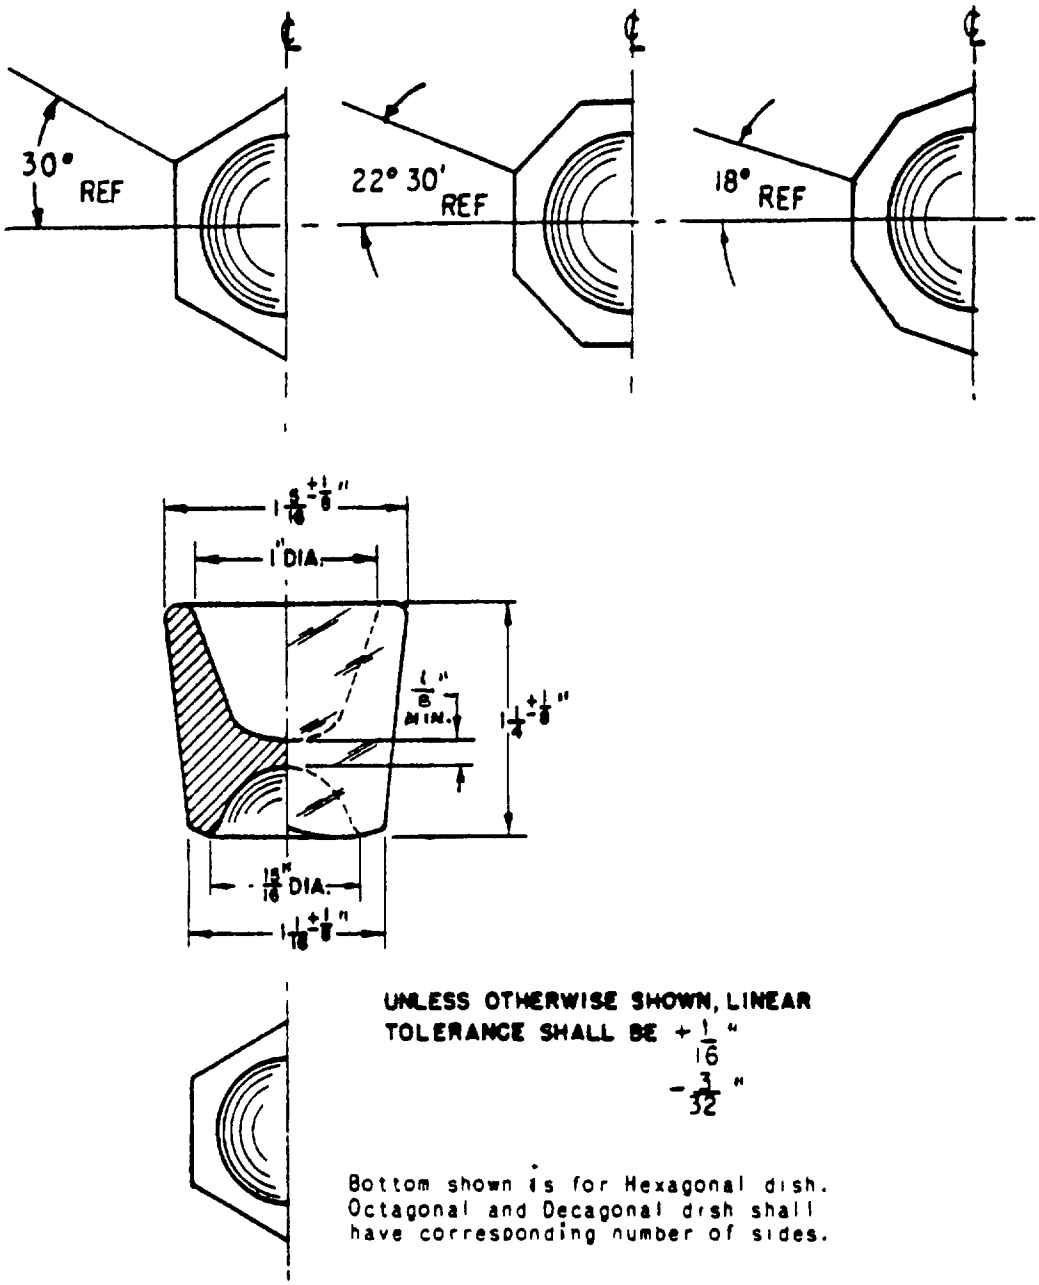


FIG. 1 - DISH, MEDICAMENT, DENTAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Inspections. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item. Inspection shall be conducted to determine compliance with specification requirements.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one dish. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Tests. Tests shall be conducted to determine compliance with specification requirements.

Boiling tests. The dish shall be placed in a closed vessel having a small steam vent, completely immersed in distilled water and boiled continuously for 4 hours. Boiling distilled water shall be added, when necessary, to compensate for evaporation losses. The dish shall be suspended in the water so that it does not come in contact with the containing vessel.

Thermal shock test. The dish shall be immersed in tap water at 18.5 ± 2.5 degrees centigrade (65 ± 5 degees Fahrenheit), allowed to remain 10 minutes, then suddenly transferred into boiling water. This operation shall be repeated four times. Samples for this test shall not be any of those subjected to the boiling test.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6520-00-550-2000 DISH, MEDICAMENT, DENTAL

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

48143

Project No. 6520-1811

Location S2-11-6

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.