GG-B-00750d (DSA-DM)
November 6, 1969
Interim Revision of
Fed. Spec. GG-B-750c
April 30, 1962

INTERIM FEDERAL SPECIFICATION

BRUSH, FIBER, ROTARY WHEEL (FOR DENTAL LATHE)

This Interim Federal Specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this Interim Federal Specification as a valid exception to Federal Specification GG-B-750c.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers rotary wheel fiber brushes suitable for cleaning and polishing prosthetic appliances.

1.2 Classification.

1.2.1 Types, classes, and size numbers. Rotary wheel fiber brushes shall be of the following types, classes, and size numbers, as specified (See 6.1):

Type I. Converging fibers.

Class A. Stiff fibers.
Size No. 12. 1-7/8 inch in diameter.
Size No. 20. 2-1/2 inches in diameter.
Size No. 23. 2-3/4 inches in diameter.

Type II. Straight fibers.

Class A. Stiff fibers.
Size No. 25. 2-3/4 inches in diameter.
Size No. 29. 3 inches in diameter.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

Class B. Soft fibers.
Size No. 26. 2-3/4 inches in diameter.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following specifications and standards, of the issue in effect on date of invitations for bid or requests for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

MMM-A-250	Adhesive, Water-Resistant, (For Sealing Fiberboard Boxes).
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.
PPP-T-76	Tape, Pressure-Sensitive Adhesive Paper (For Carton Sealing).

STANDARDS

Federal

FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Fort Worth, Denver, San Francisco, Auburn, and Washington, D.C.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of Military specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publication. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitations for bid or requests for proposal shall apply.

UNITED STATES OF AMERICA STANDARDS INSTITUTE *

USA B94.11-1967	Twist Drills, Straight Shank and Taper Shank Combined Drills and Countersinks (Revision and Redesignation of B5.12).

* Formerly the American Standards Association (ASA). All ASA Standards are now designated as USA Standards.

(Application for copies should be addressed to the United States of America Standards Institute, 10 East 40th Street, New York, N. Y. 10016).

3. REQUIREMENTS

3.1 Material.

3.1.1 Fiber.

3.1.1.1 Class A, stiff fiber. Class A, stiff fiber shall be made of either stiff hog bristle or stiff horsetail hair. The fibers shall be an undyed, natural black color.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.


3.1.1.2 Class B, soft fiber. Class B, soft fiber shall be made of soft goat hair, white in color.

3.1.2 Center block. The center block shall be fabricated from kiln-dried or air-dried dogwood, hard maple, hard birch, or hard beech wood.


3.1.3 Staples or wire. The staples or wire shall be fabricated from suitable brass.

3.2 Style and design. The rotary wheel brushes shall be suitable for use in cleaning and polishing prosthetic appliances, when mounted and secured to the chucks of dental lathes. The brushes shall be of the style and design as shown in Figure 1 for the type specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

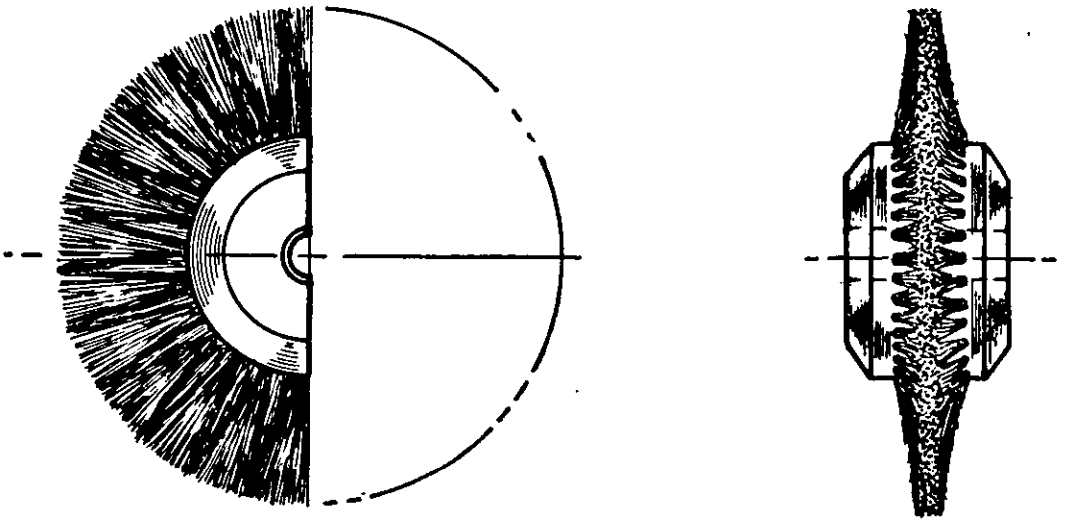

TYPE I CONVERGING

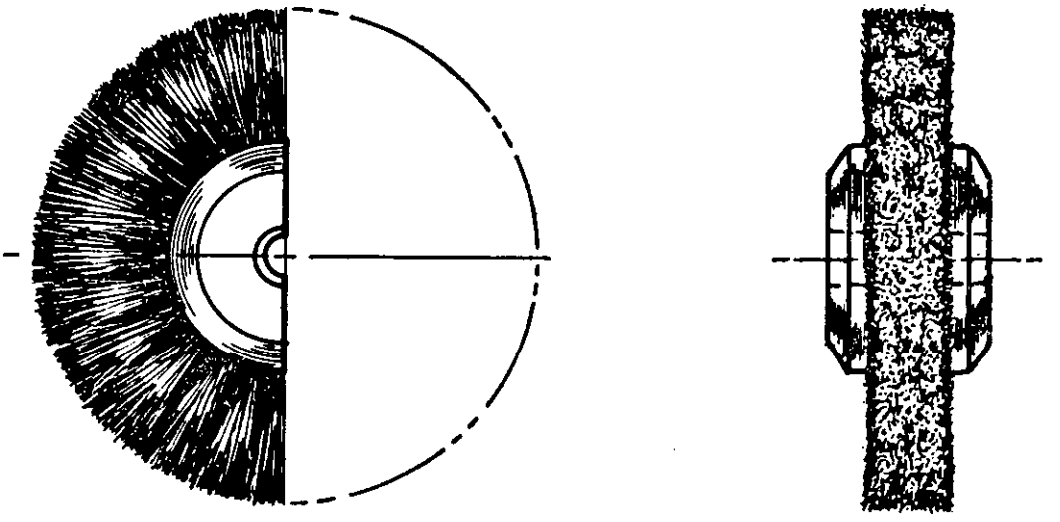

TYPE II STRAIGHT

NOTE:

SPINDLE HOLES SHALL BE EITHER TAPERED OR STRAIGHT

FIGURE 1 -TYPES OF BRUSHES

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

3.3 Construction. The holes for mounting the fibers shall be evenly spaced around the periphery of the block. The minimum number of holes for the fiber, the number of rows of holes, and the drill sizes shall be as shown in Table I for the applicable type, class, and size number brush. The fibers shall be securely staple-set or wire-drawn with brass brush wire, and shall completely fill each hole. The fibers shall be full in appearance and of even length. The spindle holes of the block shall be centered, and shall be either tapered or straight so as to fit standard lathe spindle chucks.

3.4 Dimensions. The dimensional requirements of the brushes shall be as specified in Table I for the applicable type, class, and size number. The diameter of the spindle hole at the small end of the taper (for tapered holes), or at both straight ends (for untapered holes), shall be 1/4 ± 1/64 inch.

Table I. Construction and Dimensional Requirements

	Type I			Type II		
	Class A			Class A		Class B
Size number of brush	12	20	23	25	29	26
Brush:						
Overall diameter, inches /1	1-7/8	2-1/2	2-3/4	2-3/4	3	2-3/4
Center block:						
Diameter, inch(es) /1	7/8	1-1/4	1-1/4	1-1/4	1-1/2	1-1/4
Thickness, inch /1	9/16	5/8	1-3/16	7/8	1	7/8
Minimum number of holes for fiber	40	54	75	75	96	75
Number of rows of holes	2	2	3 /2	3	4	3
Drill size for hole /3	40-43	34-35	33-35	33-35	30-32	35
Fiber:						
Minimum length of fiber held in block, inch	1/8	1/8	1/8	1/8	1/8	3/16
Minimum length outside of block, inch	1/2	9/16	11/16	11/16	3/4	3/4

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

/1 Tolerance shall be + 1/16 inch.

/2 Only the outer rows of fiber shall converge.

/3 The drill sizes shall be as specified in the United States of America Standards Institute publication USA B94.11-1967.

3.5 Loosening of fibers. There shall be no evidence of loosening of the wire-drawn or staple-set fibers, and there shall be no evidence of foreign material present in the brush, when the brush is tested as specified in 4.4.1.

3.6 Finish. The center block and the spindle hole in the block shall be finished smooth.

3.7 Identification marking. The exterior portion of the center block of each brush shall be permanently and legibly marked with the name or trademark of the contractor.

3.8 Workmanship. Workmanship shall be first class throughout. The rotary wheel fiber brushes shall be free from defects which detract from their appearance or may impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification, where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

4.1.2 Certificates of quality. Certificates of quality, supplied by the manufacturer of the fiber, the block, and the brass, may be furnished in lieu of actual performance of such testing by the contractor, provided that lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the item identification, the name of the material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered are classified as specified in tables II and IV (see 4.2.1 and 4.3) and table III (see 4.2.2).

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQLs) shall be as indicated in table II. The unit of product for examination purposes shall be one brush.

Table II. Examination Criteria

Type of defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-1	1.5
Minor A	II	2.5
Minor B	S-1	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and table III, except that the acceptance number shall be zero for all sample sizes. The unit of product for test purposes shall be one brush.

Table III. Test Criteria

Characteristic	Requirement	Test procedure	Inspection level
Loosening of fibers	3.5	4.4.1	S-2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

4.3 Examination. The rotary wheel fiber brushes shall be examined for defects including, but not limited to, those listed in Table IV.

Table IV. Classification of defects

Category	Defect
Major A:	
101	Type, class, or size number not as specified.
102	Blocks not free from cracks or splits.
103	Fibers do not completely fill each drill hole.
104	Spindle holes are not centered.
105	Style and design of brush not as shown in applicable figure.
Major B:	
151	Drill size of holes for containing fiber not as specified.
152	Minimum number of holes for fiber not as specified.
153	Number of rows of holes in center block not as specified.
154	Minimum length of fiber outside block not as specified.
Minor A:	
201	Color of fibers not as specified.
202	Fiber holes not evenly spaced around periphery of block.
203	Center block and spindle hole in block not finished smooth.
204	Identification marking not as specified.
205	Packaging and packing not as specified.
206	Marking on packaging and pack not as specified.
Minor B:	
251	Diameter and thickness of center block not within the tolerances specified.
252	Length of fiber hold in center block less than the minimum specified.
253	Diameter of spindle hole not within tolerances specified.
254	Overall diameter of brush not within tolerances specified.

4.4 Test procedure.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

4.4.1 Loosening of fibers. The rotary wheel fiber brush shall be placed on a dental lathe and rotated at a speed of 3600 revolutions per minute (r.p.m.). A coarse, hard steel file, which completely covers the width of the area occupied by the fibers, shall be gradually pushed into the brush until the fibers are bent over at right angles tangent to the circumference of the center block. Observation shall be made for loose fibers and foreign material present in, or falling from, the brush.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be Level A, or C, as specified (see 6.1).

5.1.1 Unit of issue. One brush, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table V shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table V. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	480 units

5.1.2.1 Variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each brush shall be completely wrapped in tissue paper and packaged in a carton of appropriate size, constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors are acceptable. Carton shall contain a sufficient quantity of flake naphthalene to insure against insect or vermin infestation. Closure shall be adequate to prevent spilling of contents under normal handling.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design, constructed in accordance with PPP-B-636, type CF, class weather-resistant. Boxes shall be closed by taping the top and bottom flaps with 2-inch wide tape conforming to PPP-T-76. Closing of bottom flaps with either adhesive (conforming to MMM-A-250) or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers, of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B, or C, as specified (see 6.1).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and shall be constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers, of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with FED-STD-123.

5.3.2 Military activities.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Type, class, and size required (see 1.2.1).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 Specification changes. The margins of this specification have not been annotated with asterisks to indicate where changes from the previous issue were made due to the extensive changes to this document.

6.3 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

☆ U. S. GOVERNMENT PRINTING OFFICE: 1969-393-092/5-3242

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
MAR 68

EDITION AUG 66, WILL BE USED UNTIL EXHAUSTED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements .

SPECIFICATION

GG-B-00750d(DSA-DM) FSN

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.