GG-B-735B
16 September 1985
(SUPERSEDING)
GG-B-00735A (DSA-DM)
15 May 1974
Interim Revision of
GG-B-735
August 9, 1960

FEDERAL SPECIFICATION

BRUSH, BRISTLE, DENTAL HANDPIECE (Mandrel Mounted)

This specification is approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope. This specification covers mandrel mounted bristle brushes suitable for polishing plastic dentures.

1.2 Classification.

1.2.1 Types. Brushes shall be of the following types, as specified (see 6.1).

Type I. Stiff bristle.
Type II. Soft bristle.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein.

SPECIFICATIONS

Federal

GG-I-526	Instrument, Dental and Surgical; General Specification
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.

FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

(Activities outside the Federal Government may obtain copies of Federal specifications, standards, and commercial item descriptions as outlined under General Information in the Index of Federal Specifications, Standards and Commercial Item Descriptions. The Index, which includes cumulative bimonthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, US Government Printing Office, Washington, DC 20402.

(Single copies of this specification, other Federal specifications, and commercial item descriptions required by activities outside the Federal Government for bidding purposes are available without charge from General Services Administration Business Service Centers in Boston, MA; New York, NY; Philadelphia, PA; Washington, DC; Atlanta, GA; Chicago, IL; Kansas City, MO; Fort Worth, TX; Houston, TX; Denver, CO; San Francisco, CA; Los Angeles, CA; and Seattle, WA.

(Federal Government activities may obtain copies of Federal standardization documents and the Index of Federal Specifications, Standards and Commercial Item Descriptions from established distribution points in their agencies.)

SPECIFICATIONS

Military

MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-vaporproof, or Waterproof, Flexible.
MIL-P-116	Preservation, Methods of.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.
MIL-STD-147	Palletized Unit Loads.
MIL-STD-794	Parts and Equipment, Procedures for Packaging of.

(Copies of military specifications and standards required by contractors in connection with specific acquisition functions should be obtained from the contracting activity or as directed by the contracting activity.)

2.2 Order of precedence. In the event of a conflict between the text of this specification and the references cited herein, the text of this specification shall take precedence. Nothing in this specification, however, shall supersede applicable laws and regulations unless a specific exemption has been obtained.

3. REQUIREMENTS

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

and depressing a start button, no further operator attention shall be necessary

3.1 Material.

3.1.1 Bristles.

3.1.1.1 Type I. Type I shall be top-grade, stiff, silver gray or white natural bristles, or silver gray, stiff horsehair.

3.1.1.2 Type II. Type II shall be top-grade soft, white or gray goat's hair.

3.1.2 Metal components. Metal components, including mandrels, shall be fabricated of brass or steel, nickel or chromium plated.

3.2 Figures. The figure forming a part of this specification is a specification control figure. The supplier shall be responsible for preparing his own snop drawings. Where tolerances prescribed could cumulatively result in improper design, the supplier shall provide a product with dimensions within the tolerances prescribed on the drawing to insure proper design, function, fit, assembly or operation of the item. No deviation from the prescribed dimensions or tolerances is permissible without prior approval of the contracting officer.

3.3 Style, design and dimensions. Brushes shall be of the style, design and dimensions shown in Figure 1. The bristles shall be held securely in place by a washer assembly. The washer assembly shall consist of two halves. The two halves shall be fitted together in such a manner that when the brush is used in a high-speed straight laboratory dental handpiece, having a no load speed of 34,000-40,000 RPM, there shall be no significant bristle loss when tested as specified in 4.4.2. The assembly shall be mounted true on the mandrel, and permanently affixed, such that the eccentricity of the brush shall not be effected at high speeds, as a result of loosening of the washer assembly on the mandrel, even after repeated uses. The mandrel shall be suitable for use with high-speed straight laboratory dental handpieces. The brushes shall function satisfactorily when used in dental operative procedures in cleaning and polishing dental restorations and prosthetic appliances. All edges of the brush shall be rounded and smooth to prevent cutting of the bristle as a result of pressure exerted on brush during dental procedures.

3.4 Corrosion resistance. The metal components shall show no more than 2 percent corrosion when subjected to the boil test as specified in 4.4.1.

3.5 Finish. The exposed metal components of the brush shall have a bright smooth finish.

3.6 Identification marking. Each brush shall be permanently and legibly marked with the name or registered trademark of the manufacturer.

3.7 Workmanship. Brushes shall be free from defects which detract from their appearance or impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

The sterilant-changing components shall include a sterilant filter, supply hand-

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.


4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the components may be furnished in lieu of actual performance of such testing by the contractor, provided that lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component or material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirement.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered are classified as specified in tables I and II (see 4.2.1 and 4.3) and table II (see 4.2.2).

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQLs) shall be indicated in table I. Unit of product for examination purposes shall be one brush.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

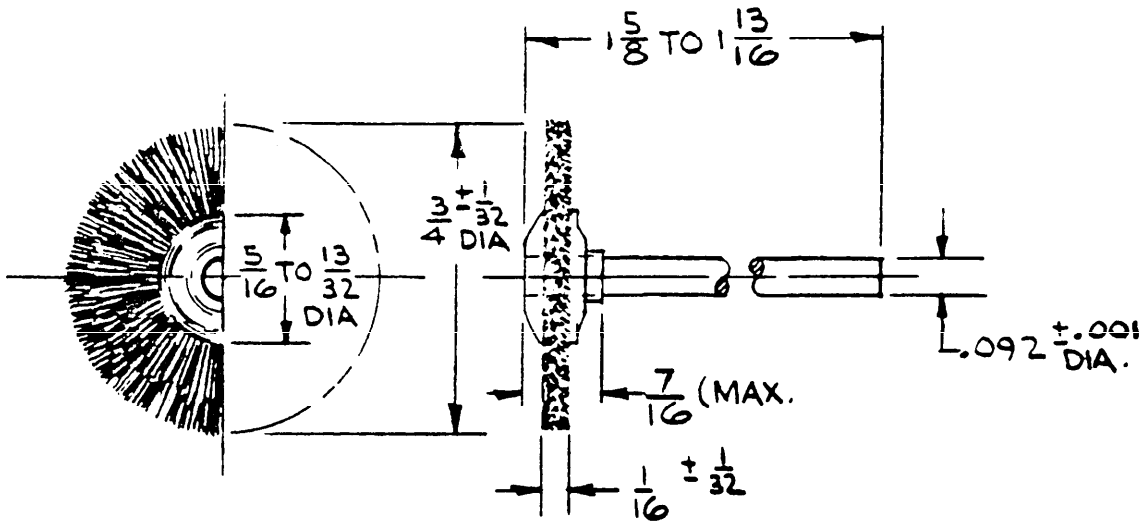

NOTES:

DESIGN OF BRISTLE HOLDING COMPONENTS IS FOR ILLUSTRATION PURPOSES ONLY.

ALL DIMENSIONS ARE IN INCHES.

FIGURE 1.

MANDREL MOUNTED BRISTLE BRUSH

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

TABLE I. Examination criteria.

Type Defect	Inspection Level	AQL (Percent Defective)
Major A	II	1.0
Major B	S-2	1.5
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and Table II, except that the acceptance number shall be zero for all sample sizes. The unit of product for test purposes shall be one brush.

TABLE II. Test criteria.

Characteristic	Require-ment	Test procedure	Inspection level
Corrosion resistance	3.4	4.4.1	S-2
Bristle test	3.3	4.4.2	S-2

4.3 Examination. The brushes shall be examined to determine compliance with the requirements of this specification. Examination shall be conducted in accordance with the following classification of defects. Examination shall include, but shall not be limited to, the defects listed in table III.

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T11:52Z
Check the source to verify that this is the currentversion before use.

TABLE III. Classification of Defects.

Categories	Defects
Major A:	
101	Type not as specified.
102	Style and design of brush not as shown in Figure 1.
103	Bristles not securely fastened in the washer assembly.
104	Washer assembly not permanently mounted on the mandrel.
Major B:	
151	Diameter of mandrel not as specified.
Minor A:	
201	Finish not as specified.
202	Color of bristles not as specified.
Minor B:	
251	Dimensions (other than 151) not as specified.

4.4 Test procedure.

4.4.1 Boil test. Brushes shall be tested as specified in GG-I-526, boil test.

4.4.2 Bristle test. Brushes shall be tested using a wet pumice abrasive on a plastic denture. The brushes shall be run for a minimum of five 2 minute intervals, where at the end of each interval the brushes shall be rinsed off with clean water and inspected for bristle loss.

4.5 Inspection of packaging. The sampling and inspection of the preservation and interior package marking shall be in accordance with groups A and B quality conformance inspection requirements of MIL-P-116. The sampling and inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C as specified (see 6.1).

5.1.1 Level A.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.1.1.1 Unit package. Twelve brushes of one type only shall be clean, dry and packaged in accordance with MIL-P-116, method III within a box of appropriate size and design conforming to PPP-B-566 or PPP-B-676. Closure shall be as specified in the applicable box specification. As an alternate, brushes may be blister packaged in multiple compartments. Each compartment shall be furnished with perforation or tear lines to permit easy removal of each brush, or the brushes shall be packaged in a plastic box of appropriate size and design having a friction closure.

5.1.1.2 Intermediate package. Twelve units containing brushes of one type shall be packed in a snug fitting box conforming to PPP-B-566, PPP-B-636, class domestic or PPP-B-676. Closure of box shall be as specified in the applicable box specification.

5.1.2 Level C. The level C preservation for brushes shall conform to MIL-STD-794 requirements for this level.

5.2 Packing. Packing shall be level A, B, or C as specified (see 6.1).

5.2.1 Level A. Twelve intermediate packages containing brushes of one type shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant. Fiberboard boxes shall be waterproofed as specified in PPP-B-636. Closure and strapping shall be as specified in the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall be as specified in the liner specification.

5.2.2 Level B. Twelve intermediate packages containing brushes of one type shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-601, domestic type; PPP-B-621, class 1, or PPP-B-636, class domestic. Closure shall be as specified in the applicable box specification.

5.2.3 Level C. The level C packing for brushes shall conform to MIL-STD-794 requirements for this level.

5.2.4 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantities for shipment to one destination equal 40 cubic feet or more. Quantities less than 40 cubic feet need not be unitized. Unitized loads shall be uniform in size and quantities to the greatest extent practicable.

5.2.4.1 Levels A and B. Brushes packed as specified in 5.2.1 and 5.2.2, shall be unitized on pallets conforming to MIL-STD-147.

5.2.4.2 Level C. Brushes packed as specified in 5.2.3, shall be unitized as specified in MIL-STD-794.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the currentversion before use.

5.3 Marking.

5.3.1 Civil agencies. Marking shall be as specified in FED-STD-123.

5.3.2 Military activities.

5.3.2.1 Levels A, B, and C. Each unit package, intermediate package, exterior container and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1, 5.2.2, and 5.2.3) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest extent practicable.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.5.

6. NOTES

6.1 Ordering data.

6.1.1 Acquisition requirements. Acquisition documents should specify the following:

(a) Title, number, and date of this specification.
(b) Type required (see 1.2.1).
(c) Selection and applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 National Stock Number (NSN) Coverage. This specification covers the following items appearing in the Federal Supply Catalog:

Stock Number	Item Identification
6520-01-056-7375	BRUSH, BRISTLE, DENTAL HANDPIECE, Mandrel Mounted, 3/4 inch, Soft bristle, 12s
6520-01-056-7376	BRUSH, BRISTLE, DENTAL HANDPIECE, Mandrel Mounted, 3/4 inch, Stiff bristle, 12s

6.3 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover those items which are normally procured to meet Federal requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Review activities:

Army - MD
Navy - MS
Air Force - 03

CIVIL AGENCY COORDINATING ACTIVITY:

VA-OSS

Preparing activity:

DoD-MB

Agent:

DLA-DM

Project No. 6520-1829

Location S2-9-14

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:52Z
Check the source to verify that this is the currentversion before use.