GG-T-00750a (DSA-DM)
June 22, 1970
Interim Revision of
Fed. Spec. GG-T-750
March 4, 1958

INTERIM FEDERAL SPECIFICATION

TUBE, DUODENAL, SURGICAL, Rehfuss

This interim Federal specification was developed by Defense Personnel Support Center, 2800 South 20th St., Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above.

The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification GG-T-750.

1. SCOPE

1.1 This specification covers one type of duodenal tube assembly, of Rehfuss design, suitable for siphonage of stomach and duodenal contents.

2. APPLICABLE DOCUMENTS

2.1 The following documents, of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
MMM-A-250	Adhesive, Water-Resistant (for sealing Fiberboard Boxes).
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.
PPP-T-76	Tape, Pressure Sensitive Adhesive Paper, (for Carton Sealing).

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

Fed. Test Method Std. No. 601	Rubber: Sampling and Testing.
Fed-STD-No. 123	Marking for Domestic Shipment (Civilian Agencies)

(Activities outside the Federal Government may obtain copies of Federal Specifications and standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D. C. 20204.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston; New York; Atlanta; Chicago; Kansas City, Mo.; Fort Worth; Denver; San Francisco; Auburn, Washington; and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

SPECIFICATIONS

Military

MIL-P-116	Preservation, Methods of.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

3. REQUIREMENTS

3.1 Material. All material used in the fabrication of the duodenal tube assemblies shall be capable of withstanding steam sterilization without evidence of damage or deformation, when tested as specified in 4.4.3.

3.1.1 Rubber. The duodenal tube and syringe connecting tube shall be fabricated of a good quality, soft, natural or synthetic rubber or a mixture of the two and shall be colored red or maroon.

3.1.2 Metal. The Rehfuss bucket or tip shall be fabricated of chromium over nickel plated brass conforming to class 8, type 260, 270, or 360 material of GG-I-526.

3.1.3 Glass. The observation tube shall be fabricated of a good quality clear, colorless glass suitable for the purpose intended.

3.2 Style, design, and dimensions. The complete duodenal tube assembly shall consist of a rubber duodenal tube, a metal Rehfuss tip or bucket, a glass observation tube, and a rubber syringe connecting tube. Style, design, and dimensions shall be in accordance with Figure 1 and as specified herein.

3.2.1 Duodenal tube. The duodenal tube shall be one continuous piece of rubber tubing, nominal size 14 French, and shall have smooth interior and exterior walls, permitting unrestricted passage of fluids. The tube shall be permanently marked in contrasting color with a series of encircling bands at three points - 16, 27, and 31 inches - measured from the bucket end of the tube to indicate the distance from the incisor teeth to the cardia, to the pylorus, and to the duodenum.

3.2.2 Rehfuss bucket (tip). The Rehfuss bucket shall be constructed in one piece of chromium over nickel-plated brass, as specified in 3.1.2. The bucket shall be olive shaped, open or closed at the distal end, and shall be provided with a hollow tubular extension at the proximal end. The extension shall be designed to provide maximum security when inserted into the duodenal tube. The lumen of the extension shall communicate with the central opening of the bucket. The bucket shall have four longitudinal slots, located one in each quadrant, which shall communicate with the central opening.

3.2.3 Observation tube. The glass observation tube shall be designed to provide a secure connection between the duodenal tube and the syringe connecting tube and shall provide for visual inspection of duodenal fluid as it is withdrawn. The lumen diameter of the glass tube shall be equal to or greater than that of the duodenal tube so as to permit unrestricted flow of fluid.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

* 3.2.4 Syringe connecting tube. The syringe connecting tube shall consist of a single piece of rubber tubing. One end shall be constructed to fit securely over one end of the observation tube and the other end shall fit securely over the tip of standard syringes.

* 3.2.5 Assembly. The duodenal tube shall be securely attached to the Rehfuss bucket by whipping with strong, undyed twisted silk thread. The thread shall be smoothly wound while wet and securely fastened by knotting the ends. The knot shall not extend beyond the widest portion of the bucket. When tested as specified in 4.4.1, the Rehfuss bucket shall not become detached or separate from the duodenal tube.

3.3 **Physical properties of the rubber tubing.**

3.3.1 Tensile strength. The minimum tensile strength shall be 1500 pounds per square inch (p.s.i.), when tested as specified in 4.4.2.

3.3.2 Ultimate elongation. The minimum ultimate elongation shall be 350 percent, when tested as specified in 4.4.2.

3.3.3 Resistance to accelerated aging. The tensile strength and elongation shall not decrease by more than 25 percent nor shall the rubber tubing become tacky or brittle, when tested as specified in 4.4.2.

* 3.4 Compatibility. The materials of which the duodenal tube assemblies are manufactured shall not react with, or be acted upon by, the liquids with which they will be in contact during normal use and operation, nor shall there be any materials incorporated in the assemblies which will cause any harmful or deleterious effect when the assembly is used for the purpose intended.

3.5 Identification marking. Each duodenal tube shall be legibly and permanently marked on the proximal end with the name or registered trademark of the manufacturer, the French size, and the date of manufacture (month and year).

* 3.6 Workmanship. Workmanship shall be first class throughout. The duodenal tube assemblies shall be symmetrical in shape and shall have smoothly finished outer and inner surfaces, free from irregularities and imperfections of any kind which detract from their appearance or which may impair their serviceability. The tubing shall be free from porosity, blisters, bleeding, blooming, brittleness, tackiness, and foreign particles. The assemblies shall be visually clean and free from foreign substances and particulate matter.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality supplied by the manufacturer of the rubber, the metal, or the glass may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the PSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in Table I. The unit of product for examination purposes shall be one duodenal tube assembly.

Table I. Sampling Criteria for Examination

Defect category	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics. The unit of product shall be one duodenal tube assembly.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL (percent defective)
Duodenal assembly	Steam sterilization	3.1	4.4.3	S-1	*
	Dimensions	3.2	-----	S-2	*
	Security of assembly	3.2.5	4.4.1	S-2	*
Duodenal tube and syringe connecting tube	Tensile strength	3.3.1	4.4.2	S-2	*
	Elongation	3.3.2	4.4.2	S-2	*
	Accelerated aging	3.3.3	4.4.2	S-2	*
Refuse bucket	Corrosion resistance	GG-I-526	GG-I-526	S-2	*
	Plating-(Thickness and Adhesion)	3.1.2 and GG-I-526	QQ-N-290 and QQ-C-320	S-2	*

* Acceptance number shall be zero.

4.3 Examination. The duodenal tube assemblies shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted in accordance with MIL-STD-105 and the classification of defects specified in Table III. Inspection, however, shall not be restricted to the classified possible defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	One or more components missing.
102	Bucket not free of cracks, burrs, slivers, or sharp edges.
103	Bucket outer surface not smoothly finished or free of pits, tool marks, scale or corrosion.
104	Bucket lumen or longitudinal slots not free of obstructing material, scale, burrs, chips, dirt, deep pits, deep furrows, or die marks.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

GG-T-00750a (DSA-DM)

:ion of Defects (Cont'd)

C:	M:
lenal tube or syringe connecting tube not d or free of blooming, bleeding, brittle- or embedded particles.	
rt free of cuts, slits, perforations, or	
or glass tubing not free of obstructing :iculate matter.	
glass tube not free of rough edges.	
not make a secure connection with rubber	
:ely knotted on tubing.	
	of discoloration.
	ree of blisters, stones, checks, crizzle,
	arking on tube not present, complete, , or permanent.

specified in the
· the performance
: as otherwise
s own or any other
equirements speci-
ernment reserves
e specification
ies and services

formed by or for
de available to the
from time to time,
3 years after

:ication, is de-
rtigation without
l testing (determi-
es) of the item.

ity supplied by the
furnished in lieu of
ided lot identity has
The certificate shall
he name of the manu-
e name of the component/
he date of testing,
ation requirements.

ducted to determine compliance with specif:

assembly. The bond between the duodenal tube ared by exerting a steady force of 5 pounds tant less than one minute, with the duodenal tve the tubular extension of the bucket.

ts. The physical properties of the rubber ts with the test methods of Federal Test M4 in Table IV. A straight specimen shall b

steam sterilization. The duodenal tube eat 15 pounds per square inch gage and 250 dautes and then allowed to cool at room t

ll be conducted in
the unit of product
ly.

m (percent defective)
1.0
2.5

:ed in accordance with
the same sample unit
aracteristics. The unit

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

Table IV. Testing of Physical Properties

Characteristic	Test Method No.
Tensile strength	4111
Ultimate elongation	4121
Resistance to accelerated aging	7221 or 7231

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C as specified (see 6.2).

5.1.1 Unit of issue. One duodenal tube, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in Table V shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table V Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	360 units

5.1.2.1 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be formed into a coil of such diameter that it will not kink or acquire a permanent set and shall be further packaged in accordance with MIL-P-116, method 1A-15.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design constructed in accordance with PPP-B-636, type CF, class weather-resistant, Boxes shall be closed by taping the top and bottom flaps with 2 inch wide tape conforming to PPP-T-76. Closing of bottom flap with adhesive conforming to MMM-A-250 or metal stitches is permitted.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Marking for shipment shall be in accordance with Fed. Std. No. 123.

5.3.2 Military activities.

5.3.2.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 This specification is intended to cover duodenal tubes which are normally procured to meet military requirements. It does not include all types indicated by the title, nor all types which are commercially available.

6.2 Ordering data. Procurement documents should specify the following:

(a) Number, title and date of this specification.
(b) Applicable levels of packaging and packing.

6.3 The margins of this specification are marked with asterisks to indicate where changes (additions, modifications, corrections, deletions) from the previous issue were made. This was done as a convenience only and the Government assumes no liability whatsoever for any inaccuracies in these notations. Bidders and contractors are cautioned to evaluate the requirements of this document based on the entire content irrespective of the marginal notations and relationship to the last previous issue.


Custodians:
Army - MD
Navy - MS

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM
Project No. 6515-1475

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

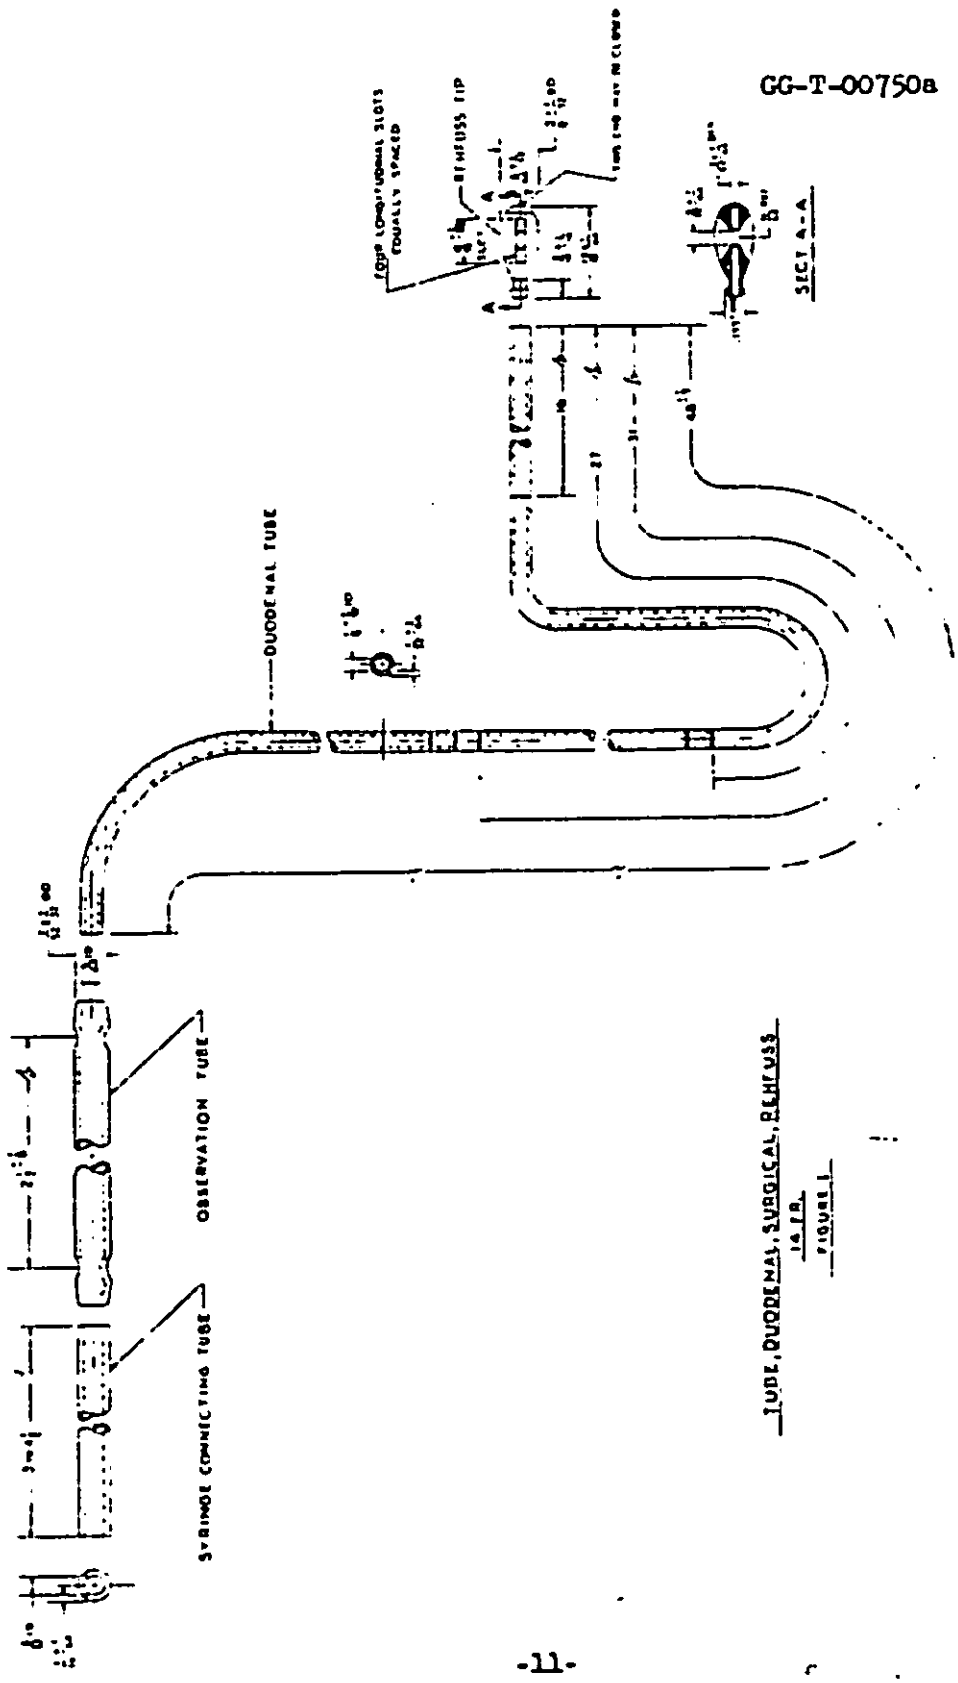

TUBE, DUODENAL, SURGICAL, REHFUSS
14 FR.
FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R355

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION

00-T-00750a(DSA-DM) FSN:

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO (If "yes", in what way?)

4. REMARKS (Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)

SUBMITTED BY (Printed or typed name and activity - Optional) | DATE

DD FORM 1 JAN 68 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE INFORMATION SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE SPECIFICATIONS MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CANNOT BE CONSIDERED FOR AWARD.

Fold

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

Fold

DPSC FORM 2418
MAR 68

EDITION AUG 66, WILL BE USED UNTIL EXHAUSTED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.