INTERIM AMENDMENT
TO
FEDERAL SPECIFICATION

URINAL, MALE PATIENT, GLASS AND CORROSION-RESISTING STEEL

This interim amendment was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, PA 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement documents and forward recommendations for changes to the preparing activity at the address shown above.

The General Services Administration has authorized the use of this interim amendment as a valid exception to Federal Specification GG-U-675C, dated July 19, 1977.

Page 1

Add "AND PLASTIC" at the end of the title.

Page 2

1.2.1 Types. Add "Type III. - Plastic, Disposable."

Page 3

Add:

"3.2.3 Plastic. Shall be fabricated of a durable plastic substance as described in 3.2.3.1 and 3.2.3.2 except any excess plastic arising from normal blow molding may be reground and blended with virgin material but shall not exceed 30 percent of the blend."

"3.2.3.1 Polypropylene. Polypropylene material shall be translucent, inert and chemically resistant."

"3.2.3.2 Polyethylene. Polyethylene shall be translucent, inert and chemically resistant. Density of the polyethylene shall be suitable for the intended use of the part."

"3.3 Design and construction. Third sentence, after "style B" delete "and"; after "type II" add: "and type III."

FSC 6530

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

Page 4

Add:

"3.3.3 Type III. Plastic urinals shall be as shown in figure 3. The handle shall be integral to the urinal. A tight-fitting lid shall be attached to the urinal as shown in figure 3. The bottom and side sitting surfaces shall be formed in such a manner that will not allow the urinal to rock when resting on a smooth surface.

"3.4.3 Type III. The plastic urinals shall have a nominal capacity of 1000 ml when placed in the upright position.

"3.6.3 Type III. Type III urinals shall be finished smooth on all edges and surfaces and shall be free of flaws which may serve as focal points for subsequent failure due to stress concentration."

Page 7

Add:

"3.7.1.1 Type III. Type III (plastic) urinals are not required to be graduated; however, plastic urinals having graduation markings are acceptable.

"3.7.2.3 Type III. Each plastic urinal shall have molded in raised letters or impressed on the bottom or outside of the handle or lid, the name or registered trademark of the manufacturer.

"3.8.3 Type III. The urinals shall be free from defects which may affect their appearance or serviceability and shall be free of grease, oil, burrs, cracks, pits, scratches and foreign embedded material visible to the naked eye."

Page 9

4.2.2 For tests. - Table II. The following should be added to the table: "Component (unit of product) - Plastic urinal; Characteristic - Stability; Requirement - 3.5; Test procedure - 4.4.3."

Page 10

4.3.1 Classification of defects - Table III. Add the following:

"Major:	Type III.	Plastic
101	Urinal including handle and lid not free from deformation.	
102	Urinal not free from rocking when bottom and side resting surfaces are placed on a smooth, flat surface.	
103	Urinal or handle not free from pits, scratches, cracks, burrs and abrasions.	
104	Urinal not translucent.	
Minor:		
201	Urinal, including handle and lid, not free from flash greater than 1/16 inch.	
202	Urinal not free from foreign embedded material.	
203	Urinal not free from oil or grease smears on either inside or outside surfaces."	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

Page 12

5.1.1.1 Unit package. In line 1, following "Each" insert: "type I and type II". At end of paragraph add: "Fifty type III urinals shall be packaged in a box as specified for the type I and type II urinals."

5.1.2 Level C. Delete and substitute:

"5.1.2 Level C. Each type I and type II urinal or fifty type III urinals shall be clean, dried and packaged in a manner that will afford adequate protection against damage during shipment from the supply source to the first receiving activity."

5.2.1 Level A. Lines 1 and 2, delete "of one type and style only" and substitute: "of type I or type II of one style only." At end of paragraph add: "Type III urinals packaged as specified in 5.1.1.1 shall require no further packing except that the unit package shall be a weather-resistant box closed, waterproofed and banded as specified in PPP-B-636.

5.2.2 Level B. Lines 1 and 2, delete "of one type and style only" and substitute: "of type I or type II of one style only." At end of paragraph add: "Type III urinals packaged as specified in 5.1.1.1 shall require no further packing.

5.2.3 Level C. Delete and substitute:

"5.2.3 Level C. The packaged urinals shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the carriers rules and regulations."

Page 13

6.2 Ordering data. Delete "c. Type and style required (see 1.2)." and substitute "c. Type required."

6.4 Add the following:

"6530-01-042-2485 URINAL, MALE PATIENT, Plastic, 50s."

Add: "Figure 3. Urinal, Male Patient, Plastic." to the specification.

MILITARY CUSTODIANS:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Logistics Agency - DM

Project No. 6530-1441

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.

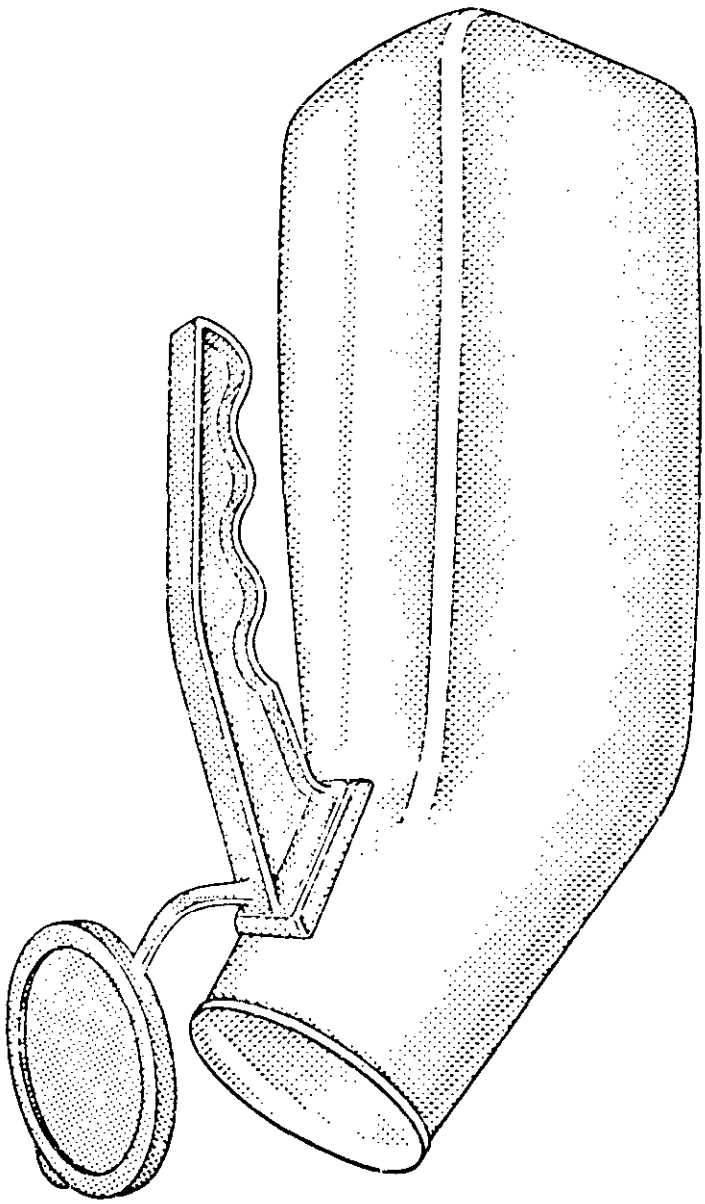


FIGURE 3. Urinal, Male Patient, Plastic

☆U.S. GOVERNMENT PRINTING OFFICE: 1977 — 703-122/350

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:52Z
Check the source to verify that this is the current version before use.