A-A-0051579(DM)
16 September 1986

INTERIM COMMERCIAL ITEM DESCRIPTION

SPECULUM, EYE (BARRAQUER)

The General Services Administration has authorized the use of this interim commercial item description which was developed by the Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA, 19101, based upon currently available technical information.

This interim commercial item description covers one adult size of eye specula of the Barraquer design.

Salient characteristics.

Material. Specula shall be manufactured of quarter-hard austenitic corrosion-resistant steel wire of composition in accordance with American Society for Testing and Materials (ASTM) Standard F899.

Style Design. Specula shall be of the style and dimensions shown in figure 1. The specula shall be manufactured from wire 0.039 $\pm$ 0.001 inches in diameter. The ends of the wire shall be permanently attached to the body of the specula such that there are no small gaps or sharp edges.

Workmanship. The item shall be processed in such a manner as to be uniform and free from defects that will affect life, serviceability, or appearance.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (EA). One eye speculum, as specified, constitutes one unit.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The specula shall be examined to determine compliance with all requirements contained in this specification. Sampling shall be conducted in accordance with MIL-STD-105, sampling level S-II, AQL 4.0. The unit of product for test purposes shall be one speculum.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 , sampling level S-1, AQL 1.0. The unit of product for test purposes shall be one speculum..

Corrosion-test. Specula shall be tested for corrosion resistance in accordance with the Resistance to Boil test of Federal Specification GG-I-526.

Steel composition. A sufficient amount of raw material shall be tested for chemical composition as to be representative of the lot or batch.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:58Z
Check the source to verify that this is the currentversion before use.

Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of composition testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer, or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the test method, and the test results.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-121-2347	SPECULUM, EYE, BARRAQUER, ADULT

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 47286

Project No. 6515-3793

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

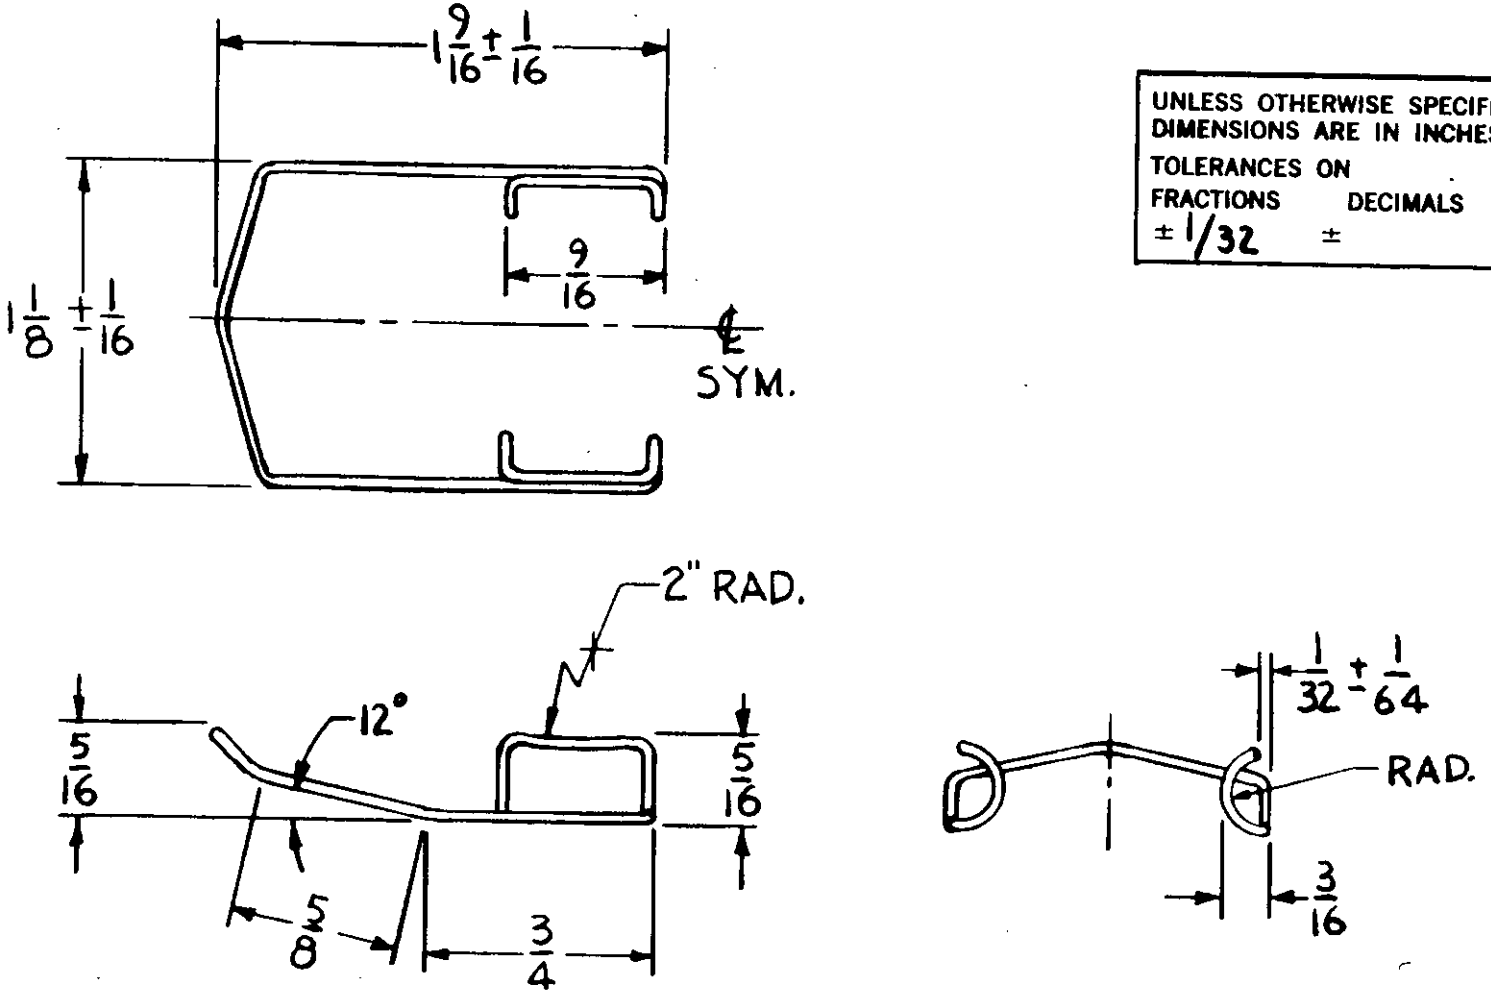

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/32	±	± 2°

FIGURE 1 SPECULUM, EYE, BARRAQUER

☆ U.S. GOVERNMENT PRINTING OFFICE: 1988 — 605-036/45220

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:58Z
Check the source to verify that this is the current version before use.