A-A-51579A
12 June 1989
SUPERSEDING
A-A-0051579(DM)
16 September 1986

COMMERCIAL ITEM DESCRIPTION

SPECULUM, EYE (BARRAQUER)

This commercial item description covers one type of eye speculum for use in ocular surgery.

Salient characteristics.

Style and design. The wire-frame eye speculum shall be in accordance with Figure 1 or Figure 2. Either design shall be designated as the "Barraquer" design.

Dimensions. The wire diameter of Figure 1 speculum shall be 0.039 ± 0.001 inch, and the wire diameter of Figure 2 speculum shall be 0.032 ± 0.001 inch (see note 2).

Material. The speculum shall be fabricated from austenitic stainless steel wire stock, in accordance with American Society for Testing and Materials (ASTM) Designation F899.

Hardness. The speculum shall have a final hardness of HRC 40 to HRC 45. Sample speculum shall be tested for hardness in accordance with ASTM Designations E18 or E92.

Corrosion-resistance. The speculum shall show no evidence of corrosion when tested in accordance with ASTM Designation F1089.

Finish. The speculum shall have a mirror finish.

Workmanship. The speculum shall be free from gaps, sharp points, sharp edges, cracks, burrs, nicks, dents, pits, corrosion, and any other defects that detract from its appearance or impair its serviceability.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

Unit. Each (EA). One eye speculum, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics. The unit of product for test purposes shall be one eye speculum.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105 at Level S-1, AQL (Acceptable Quality Level) 1.0 percent.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specification, standard, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as acceptable, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

NOTE 1: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-121-2347	SPECULUM, EYE, Barraquer, Adult

NOTE 2: Elements from these two designs shall not be interchanged.

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
PHS
FDA-MPQAS

PGC 47286

Project No. 6515-4413

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.


A-A-51579A

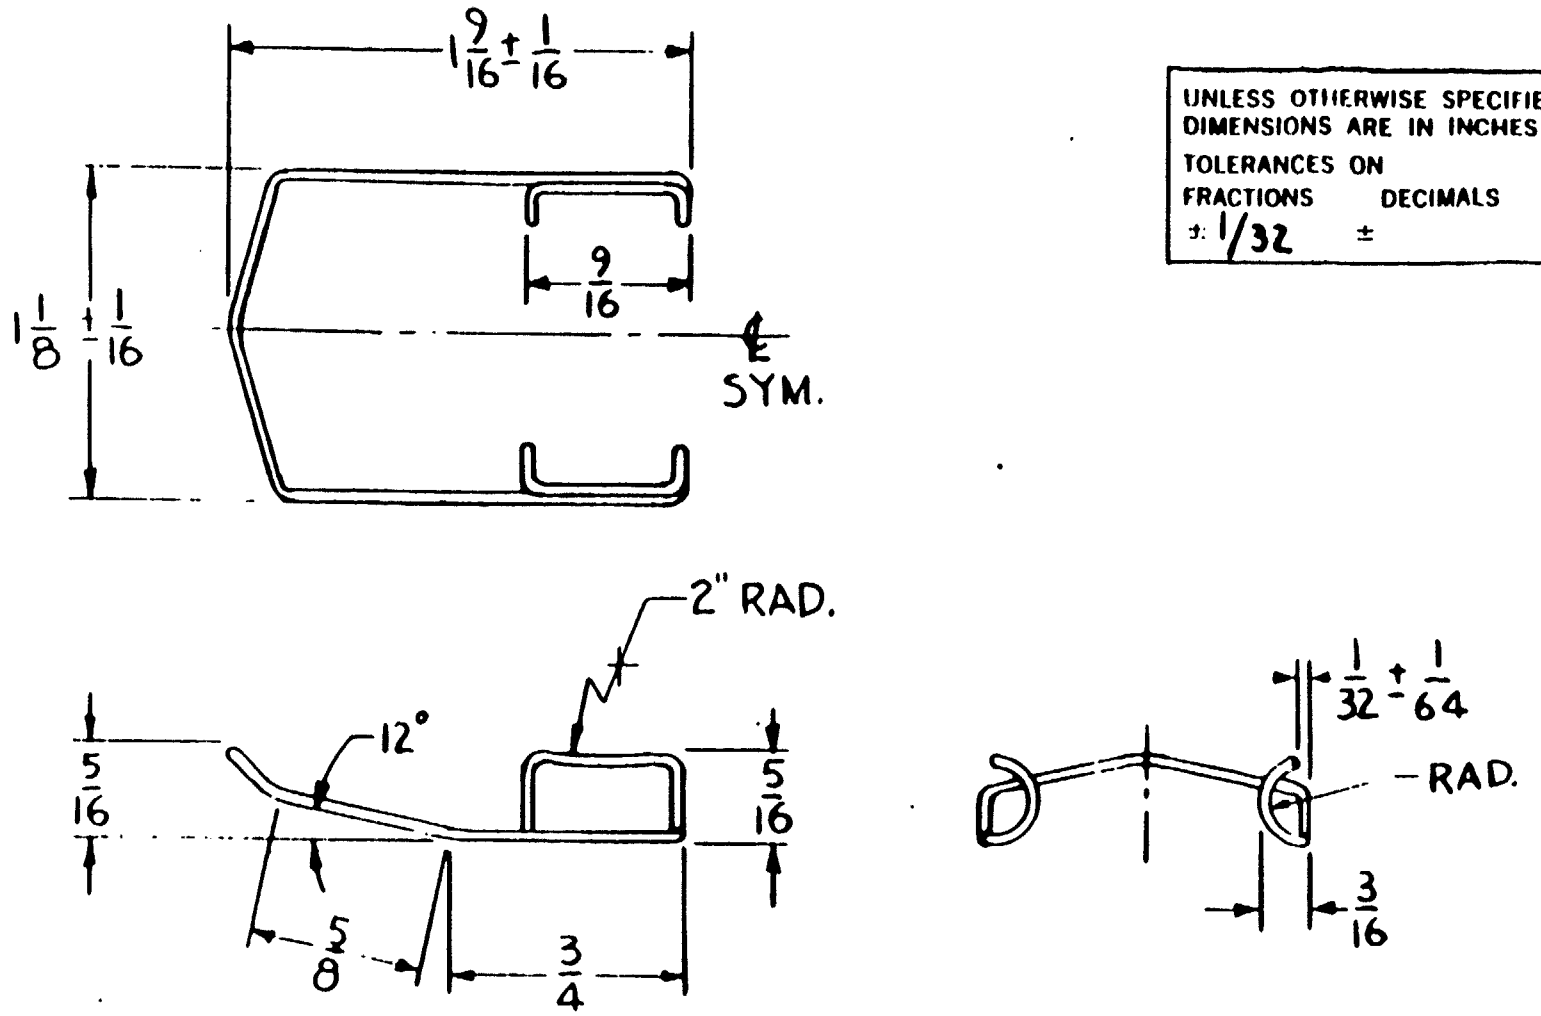


UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/32	±	± 2°

FIGURE 1 SPECULUM, EYE, BARRAQUER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

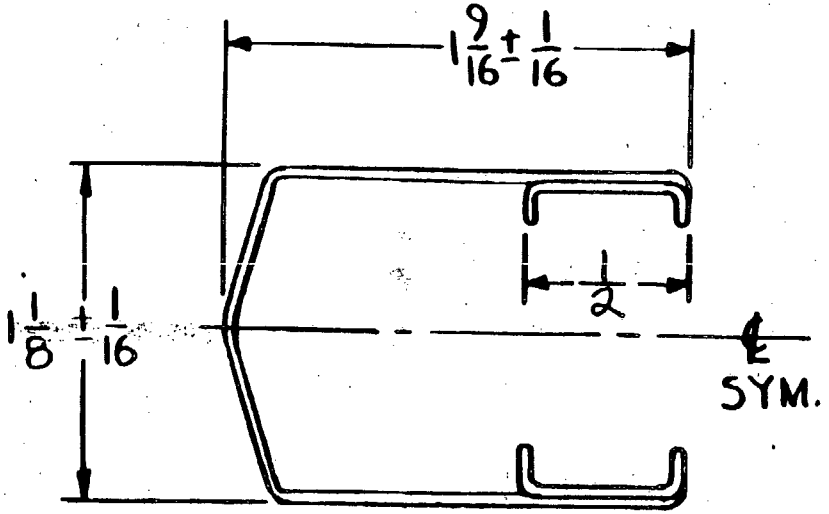

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/32	±	± 2°

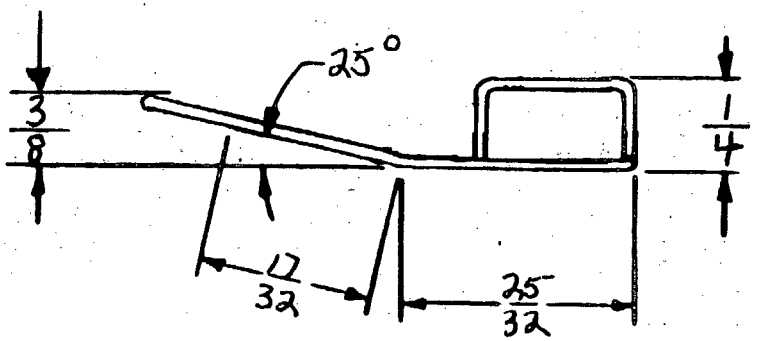

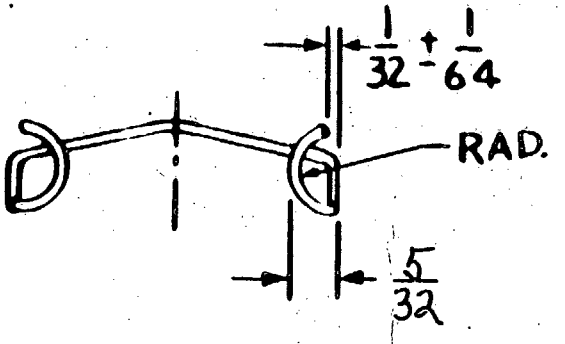


FIGURE 2 SPECULUM, EYE, BARRAQUER
(Alternate Style and Design)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.