A-A-51583A
30 June 1987
SUPERSEDING
A-A-0051583A
4 August 1986

COMMERCIAL ITEM DESCRIPTION

CRUCIBLE, CASTING MACHINE, DENTAL

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers a zircon alumina crucible which shall be suitable for use with dental metals casting machine, NSN 6520-00-511-6350.

Salient characteristics:

The crucible shall be designed to withstand a minimum temperature of 3000 degrees Fahrenheit, without showing any degradation. Shall not contaminate high fusing metal alloys or porcelain. Shall be self-glazing. Shall be capable of holding no less than 30 pennyweights (dwt) of gold casting alloy and shall feature high wall design to prevent metal spillage during casting.

The crucible shall be suitable for use in casting gold inlays and full crowns.

Material. The crucible shall be fabricated from zircon alumina.

Shape and dimensions. The crucible shall conform to the shape and dimensions of figure 1.


Workmanship. The zircon alumina crucible shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One crucible, as specified, constitutes one unit.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:58Z
Check the source to verify that this is the current version before use.

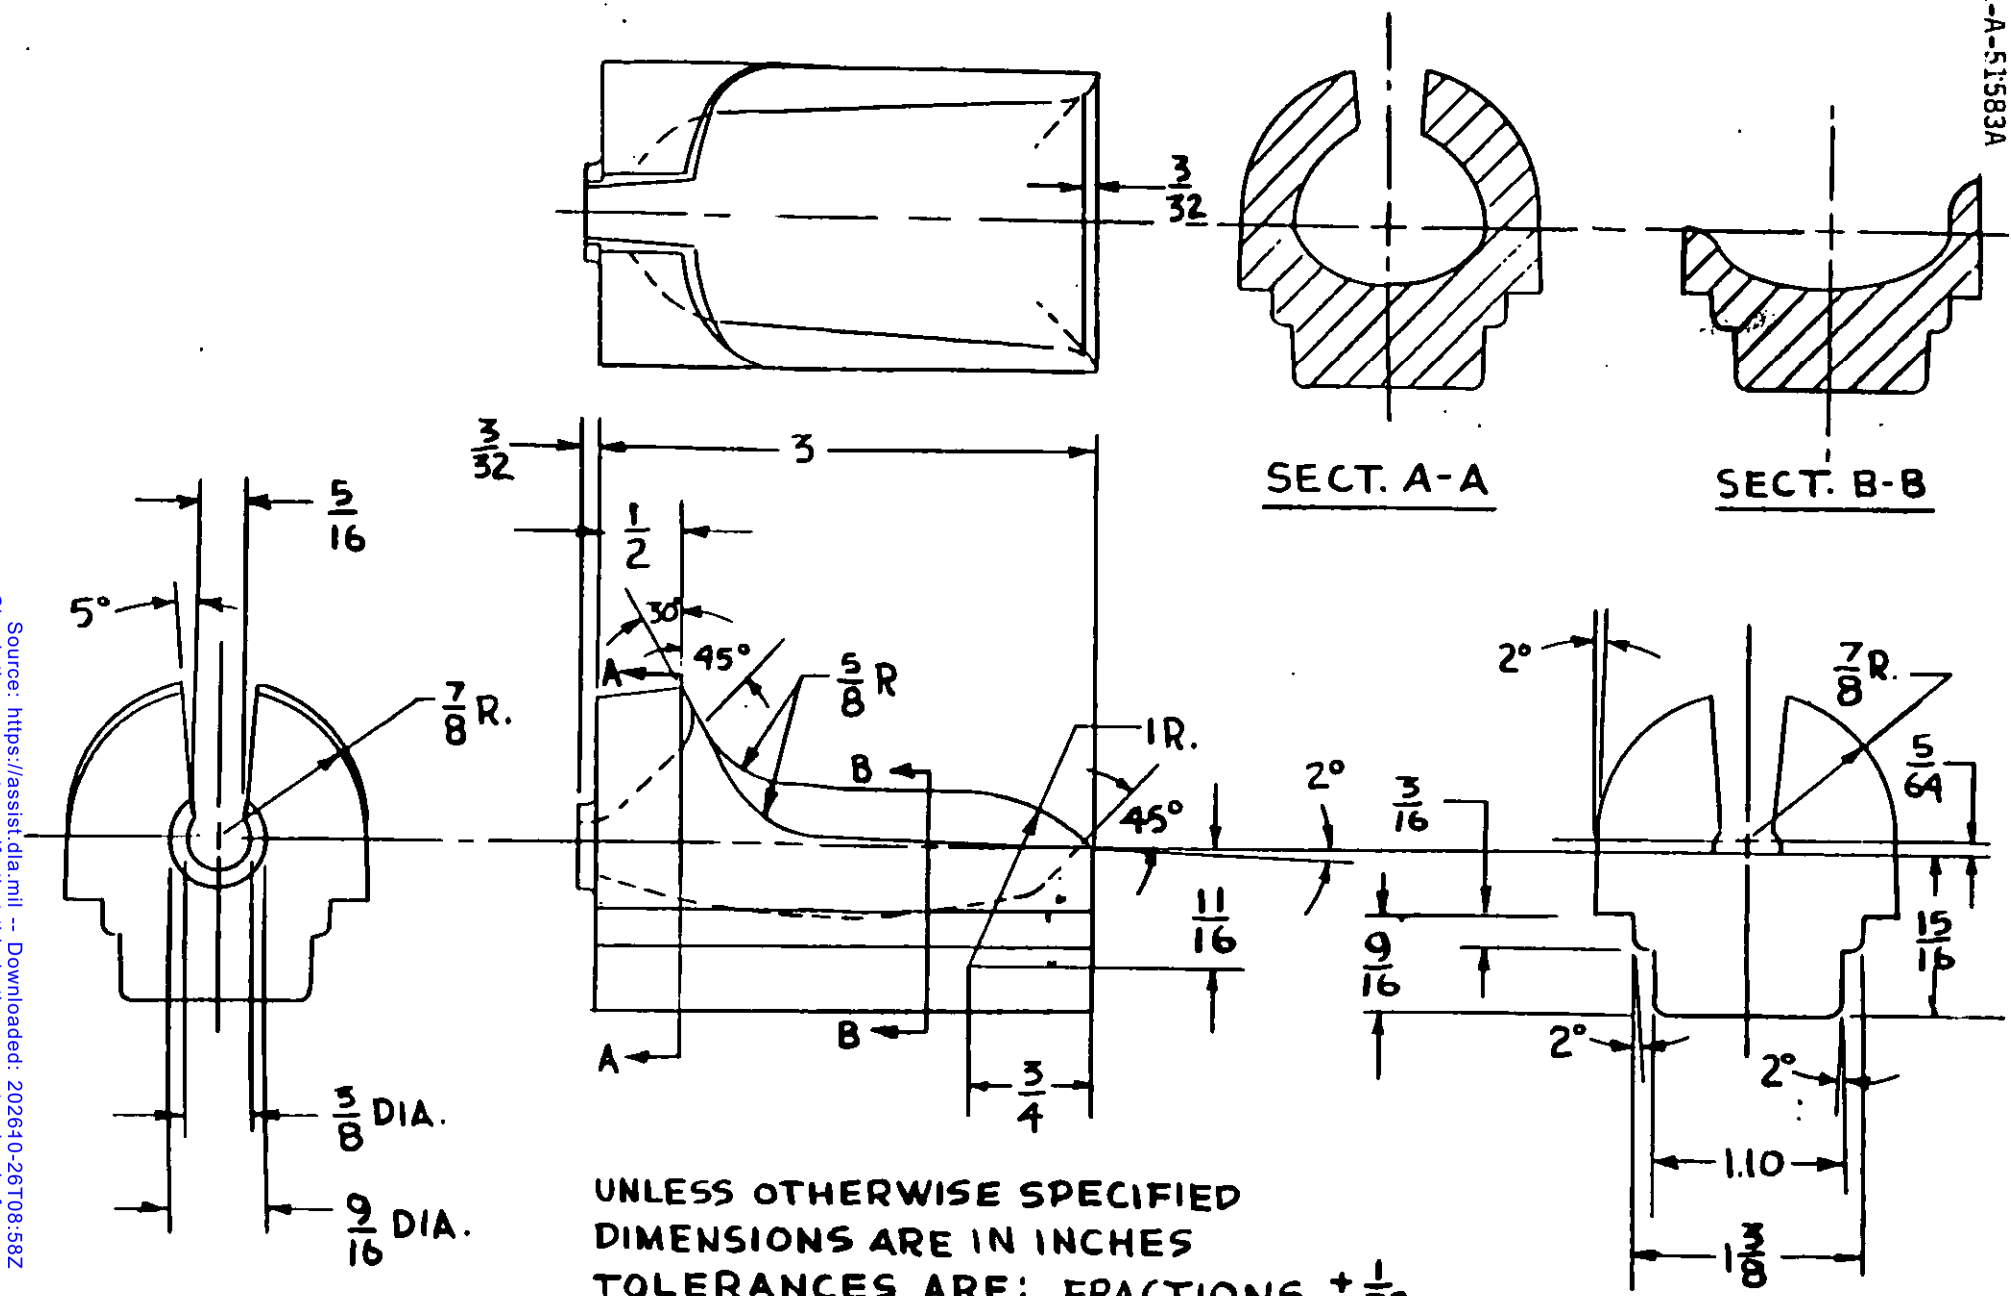

UNLESS OTHERWISE SPECIFIED
DIMENSIONS ARE IN INCHES
TOLERANCES ARE: FRACTIONS ±1/32,
DECIMALS .030, ANGLES ±1°

FIGURE 1 CRUCIBLE, CASTING MACHINE, DENTAL

Source: https://assist.dla.mil -- Downloaded: 2026/10-26T08:58Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Resonsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one crucible. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:58Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractor/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

National Stock Number	Item Identification
6520-01-224-3516	CRUCIBLE, CASTING MACHINE, DENTAL, Zircon Alumina, Self-Glazing.

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:58Z
Check the source to verify that this is the current version before use.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD - MB

Agent:

DLA - DM

CIVIL AGENCY COORDINATING ACTIVITIES:
VA-OSS
PHS
FDA-MPQAS

60076

PROJECT NO. 6520-2002

Location: NCR - Disk 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.