A-A-51617
31 October 1986

COMMERCIAL ITEM DESCRIPTION

PLIERS, OPTICIANS, LENS AXIS ALIGNING, 6 INCH

The General Services Administration has authorized the use of this commercial item description which was developed by the Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RST, 2800 South 20th Street, Philadelphia, PA, 19101, based upon currently available technical information.

This commercial item description covers one type of opticians' pliers to be used for aligning lenses in spectacles after glazing.

Salient characteristics:

The pliers shall be fabricated with two flat metal jaw plates which are attached to the jaw of the pliers by a screw and lock washer and shall have an aligning rivet to prevent rotation. A rubber gripping pad shall be securely adhered to each jaw plate. The back surface of the pad shall be flat to assure an adequate bonding surface for the jaw plate. A rectangular section shall be removed from the center to permit the pad to conform to the lens contour and distribute pressure equally. The plier handles shall be spring loaded to keep jaws open when not in use.

The pliers shall conform to the style and dimensions shown in fig 1. Overall length in the closed position shall be 6-1/8 inches minimum.

The handles, jaws, jaw plates and screws shall be made of low carbon steel, 1006 to 1020.

The coil spring shall be made of spring steel of sufficient quality to hold the jaws in an open position.

The rivets shall be made of brass, copper alloy number 230, 240, 260, or 268 in conformance with QQ-B626.

The body and jaws shall be bright nickel plated. The screws and washers shall be zinc or cadmium plated.

The jaw plates and brass rivets shall be unplated.

The jaw pad shall be made of black neoprene rubber with a hardness of 60-65 durometer.

AMSC N/A FSC 6540

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

The adhesive for mounting the jaw pad to the jaw plate shall have a minimum of two years storage life without being dried up.

The pliers shall be permanently marked with manufacturer's name or logo.

All surfaces shall be smooth and free from sharp edges and corners.

The pliers shall be furnished with two extra pairs of jaw plates with attached rubber pads.

Workmanship. The pliers shall be free from defects which detract from their appearance or impair their serviceability.

Unit. Each (EA). One pair of pliers, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one pair of pliers.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontrators/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

The following National Stock Number is covered by this document:

6540-00-135-9645

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51617

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITY:

PHS
VA-OSS
FDA-MPQAS

PGC 51108

Project No. 6540-1176
Location: CID/PLIERS,OPTICIANS
NCR, disk 6

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

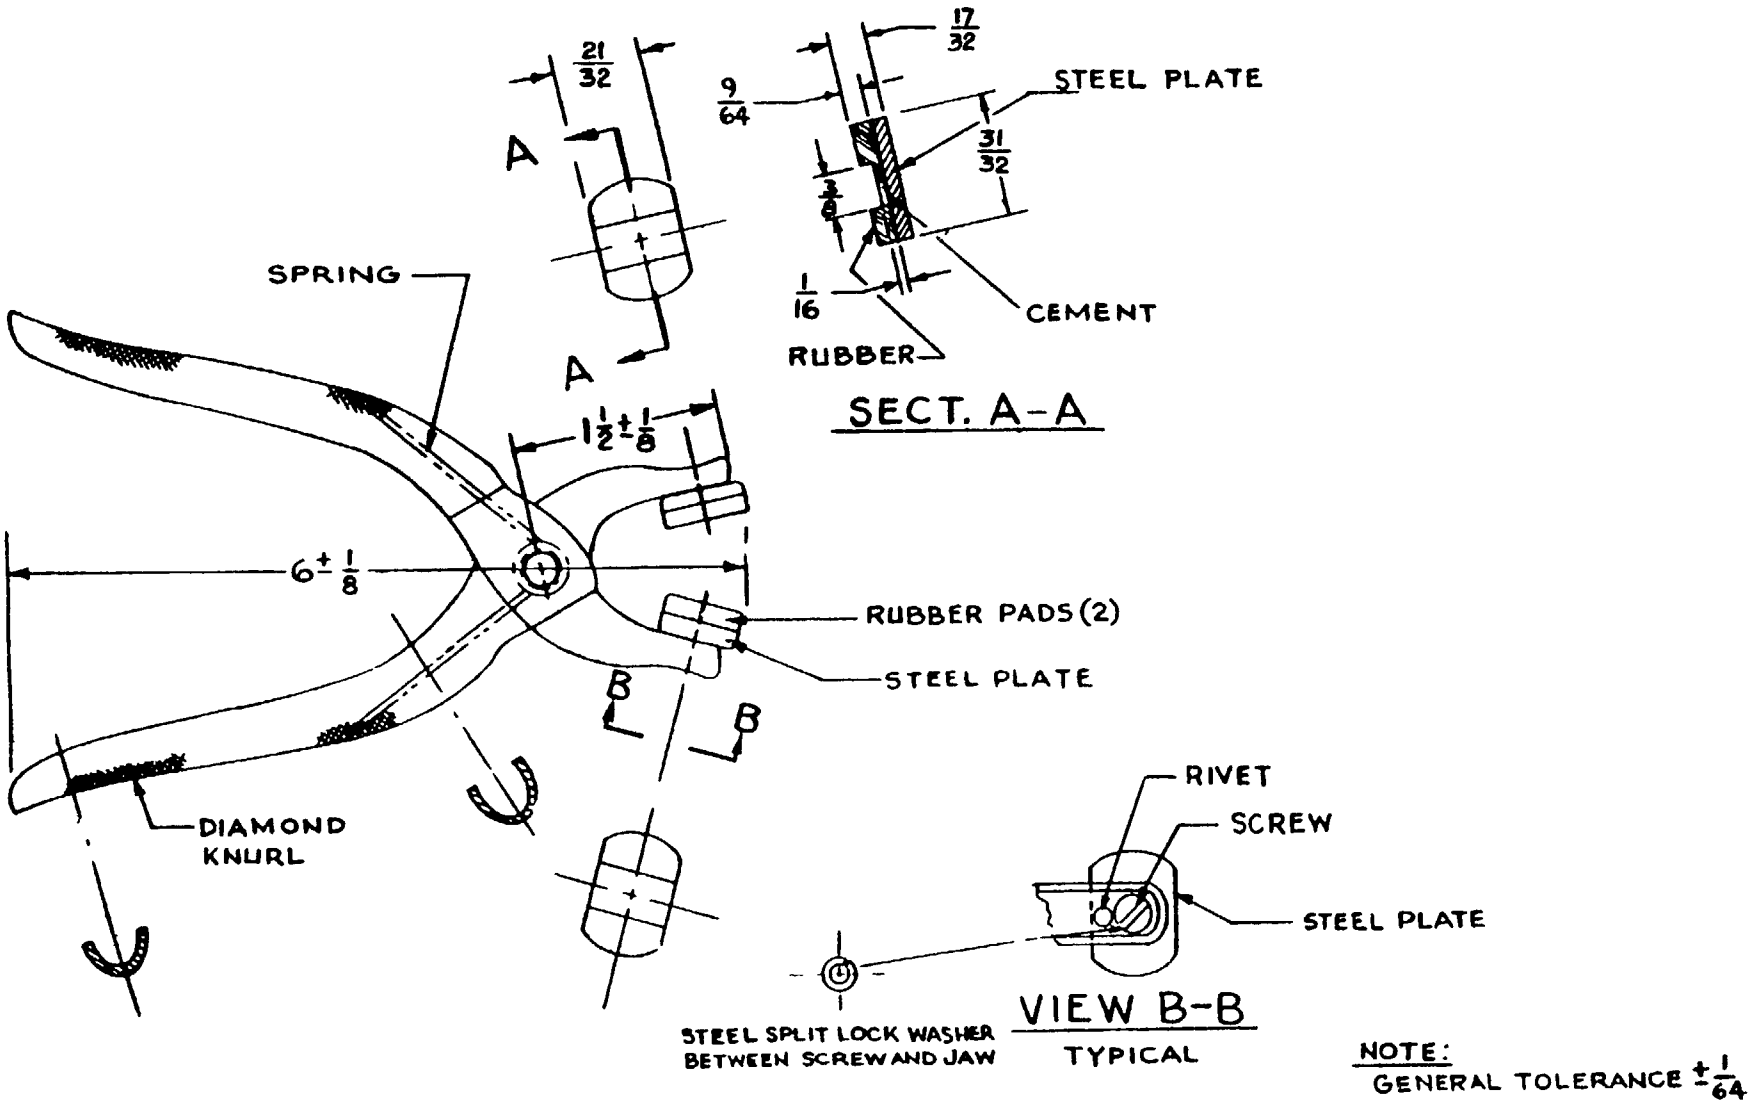

PLIERS, OPTICIANS, LENS AXIS ALIGNING, TYPE II

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

ISTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in ıbmitting comments and suggestions for improvements. All users of military standardization documents are invited to provide ıggestions This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and ıiled. In block 6, be as specific as possible about particular problem areas such as wording which required interpretation, was rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the ·oblems Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an ·knowledgement will be mailed to you within 30 days to let you know that your comments were received and are being ɔnsidered

OTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of ɔecification requirements on current contracts Comments submitted on this form do not constitute or imply authorization ɔ waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

FENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

, FICIAL BUSINESS
:NALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 WASHINGTON D C
POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN: DPSC-LS
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-51617	PLIERS, OPTICIANS, LENS AXIS ALIGNING, 6 INCH

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b Recommended Wording

c Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426

PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.