A-A-51619
25 August 1986

COMMERCIAL ITEM DESCRIPTION

MATRIX SET, DENTAL (Cervical)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers an assortment of plastic-covered aluminum cervical matrices suitable for use in dental restorative procedures.

Salient characteristics:

The matrix set shall be an assortment of plastic-covered aluminum cervical matrices suitable for use on anterior and bicuspid teeth in dental restorative procedures.

Material.

The matrices shall be fabricated of the following:

Aluminum	99.0% minimum.
Iron	0.6% maximum.
Silicon	0.2% maximum.

The matrices shall be coated on both sides with a suitable polyester resin. The convex surface shall be coated with a tooth colored polyester resin and the concave surface shall be coated with a clear polyester resin.

The matrices shall be suitable for burnishing to teeth.


Dimensions and design.

The matrices shall be preformed with a convex curvature so as to generally conform to the cervical anatomy of the teeth and shall be readily adaptable by burnishing to the specific cervical anatomy of the tooth to be restored. Matrices shall be furnished in the sizes as specified in Figure 1.


AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

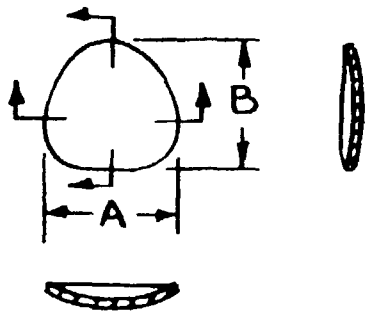


SIZE 1

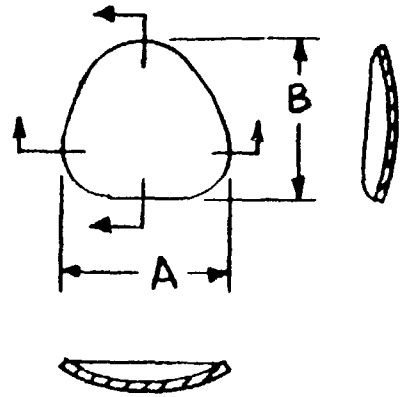


SIZE 2

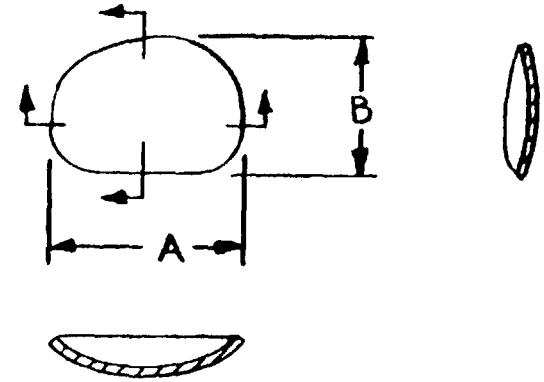

SIZE 3

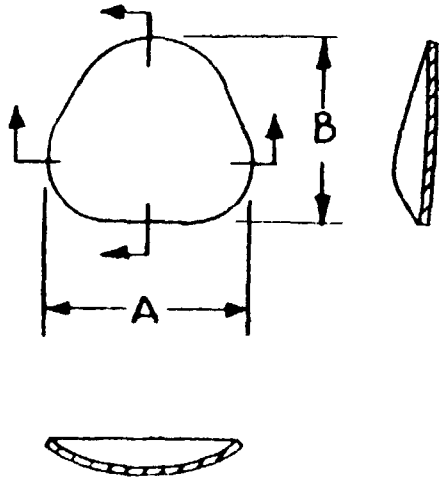

SIZE 4

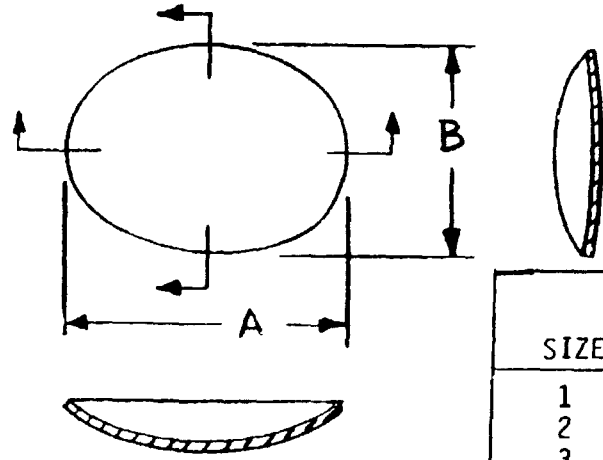

SIZE 5

SIZE	MM 1/		INCH 2/
	A	B	RADIUS OF CURVATURE
1	4.2	4.0	3/16
2	5.3	5.0	17/64
3	6.2	4.3	1/4
4	6.5	5.8	9/32
5	9.0	6.4	11/32

1. Tolerance shall be 0.1 mm for both measurements A and B.

2. This is a nominal value. Radius is measured with the grain on the concave surface.

FIGURE 1 MATRIX SET, DENTAL, ALUMINUM, PLASTIC COATED, CERVICAL, ASSORTED

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

All five sizes shall be 0.2 ± 0.05 mm thick.

The matrices shall impart a glossy finish to restorative surfaces.

The unit of issue shall be a set consisting a 20 each of the five sizes, as specified.

The inclusion of wood wedges in the package is optional.

Directions for use shall be included with the unit of issue.

Workmanship. The matrices of the set shall have smoothly trimmed and finished peripheral edges and shall be free of burrs, improper or not uniform coating, or any defect which detracts from their appearance or impairs their serviceability.

Unit. Set (SE). One matrix set, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one matrix set, as specified. Unless otherwise specified, sampling for examination shall be conducted at level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document.

Stock Number	Item Identification
6520-01-103-8585	MATRIX SET, DENTAL, Aluminum, Plastic Coated, Cervical, Assorted, Set of 100

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

MILITARY INTERESTS:

Custodians:
Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA - DM

CIVIL AGENCY COORDINATING ACTIVITY
VA-OSS
PHS
FDA-MPQAS

49093

PROJECT NO. 6520-1891

Location: NCR Disk 2

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge (*DO NOT STAPLE*), and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

Fold along this line)

DEPARTMENT OF THE ARMY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 12062 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEPARTMENT OF THE ARMY

Commander
Defense Personnel Support Center
Directorate of Medical Materiel
ATTN: DPSC-RSTS (9-3-F)
2800 South 20th Street
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-51619	MATRIX SET, DENTAL (CERVICAL)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE.

(FOLD BACK THIS FORM, CUT ALONG THIS LINE)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:58Z
Check the source to verify that this is the current version before use.