A-A-51115
15 January 1986

COMMERCIAL ITEM DESCRIPTION

TRACHEOSTOMY KIT, EMERGENCY, Sterile

The General Services Administraton has authorized the use of this commercial item description.

This commercial item description covers sterile, disposable, emergency tracheostomy kit suitable for performing emergency tracheostomies due to larynospasm, trauma to the neck or destruction, collapse or blockage of the airway.

Salient characteristics:

General. The tracheostomy kit shall consist of a disposable syringe with a male Luer slip tip and cannula lancet needle with an integral throat plate and a female Luer slip hub

Characteristics. The cannula tube shall be 8 gauge by 1-1/2 plus or minus 0.10 inches with the distal end 7/8 plus 0 minus 0.062 inches long and curved at a 30 plus or minus 5^{0} angle to the hub. The The cannula tube shall have an I.D. of 0.135 plus or minus 0.005 inches. The leading edge of the cannula tube shall be sharpened to form a point. In addition, the back edge of the point shall be sharpened starting one-half diameter from the edge. The cannula shall be in accordance with Figure 1.

A throat plate that limits the needle penetration shall be provided. The throat plate shall be 1.25 plus or minus 0.1 inches long, 0.50 plus or minus 0.05 inches wide and 0.020 plus or minus 0.002 inches thick. Each throat plate shall have one slot at each end suitable for the attachment of a 36 inch polyester tie. The tie shall hold the needle in place on the patient. A 10 cc syringe shall be part of the kit.

Luer fittings. Both the male and female Luer fittings shall meet the dimensional requirements of ANSI MD 70.1. The tracheostomy kit shall meet the performance test requirements for Luer slip fittings of ANSI MD 70.1.

Materials. The cannula tube shall be fabricated from type 304 austenitic corrosion-resistant steel. The throat plate and hub shall be fabricated from corrosion-resistant metallic alloy. The disposable syringe shall be fabricated from plastic suitable for the intended use.

Sterility. Each tracheostomy kit shall be sterilized in accordance with the USP.

Instructions. An instruction sheet detailing the proper use of the tracheostomy kit shall be provided with each kit.

Workmanship. The tracheostomy kit shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Package (PG). One package containing ten tracheostomy kits, as specified, constitutes one unit. The tracheostomy kits shall be individually packaged sterile in a peel-open type container capable of maintaining sterility of contents unless package is damaged or opened.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release, distribution is unlimited

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. AQL shall be 1.0 percent defective. The unit of product for test purposes shall be one inspection level shall be S-2. tracheostomy kit.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U. S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE The following National Stock Number is covered by this document:

6515-01-159-8969

Custodians.

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITY
VA-OSS

58315

Project No. 6515-3355

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.

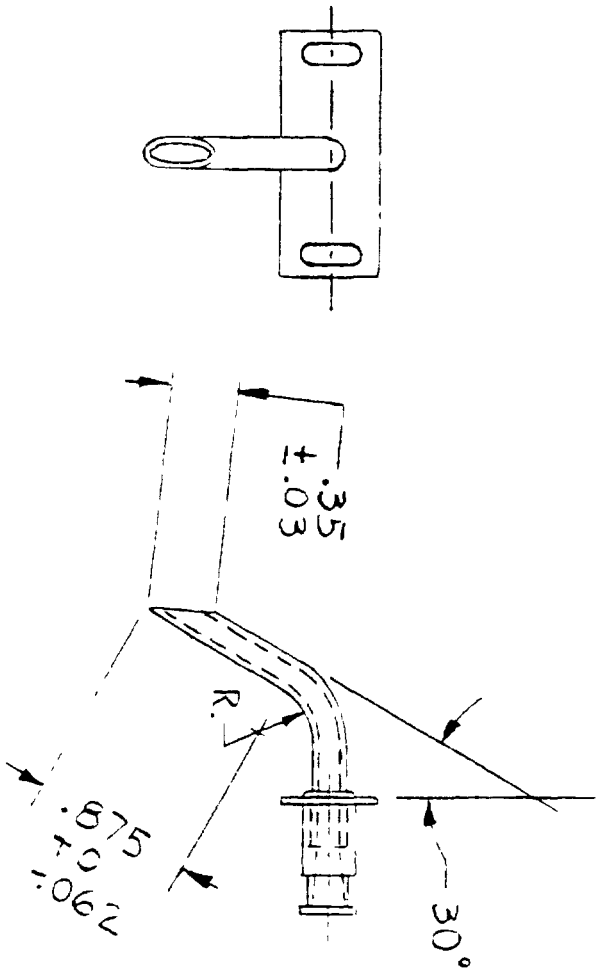


FIGURE 1 Cannula

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:50Z
Check the source to verify that this is the current version before use.