A-A-51499A
22 April 1987
SUPERSEDING
A-A-0051499(DM)
14 July 1986

COMMERCIAL ITEM DESCRIPTION

OSTEOTOME SET (Hoke)

The General Services Administration has authorized the use of this Commercial Item Description.

This commercial item description covers an osteotome set, of the Hoke design, suitable for use in orthopedic surgery.

Salient characteristics.

Components. The osteotome set shall consist of a sterilizing rack comprised of a carrying post, cap assembly, adjustable stop, spring, and a base. Additionally, the set shall include five straight osteotomes of the Hoke design, each six inches in length. Blade widths of the osteotomes shall vary as follows:

Style	Blade width (inches)
1	1/8
2	3/16
3	1/4
4	5/16
5	3/8

Style and design of osteotomes shall be in accordance with Figure 1.

Each osteotome shall be fabricated of a Class 4 martensitic corrosion-resistant steel in accordance with ASTM F899. Rockwell hardness of the osteotome set shall be C50 to C56. Completed osteotomes shall be passivated and shall have a satin finish.

Rack shall be capable of securely holding five osteotomes during sterilization procedures. The rack shall be designed to allow adequate sterilization of instruments. Rack shall be comprised of the following components:

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

Post. The post shall run from the base to the protector cap, extending through the protector cap to act as a carrying handle. The post shall be fabricated of stainless steel.

Protector cap. The protector cap shall be able to be secured to the post. The protector cap shall cover and protect osteotome blades. Area of underside of cap which comes in contact with the blades shall be plastic. The plastic shall be able to withstand repeated sterilizations. Protector cap body shall be fabricated of a corrosion-resistant metal alloy.

Adjustable stop. The adjustable stop shall be able to be secured to the post. The adjustable stop shall be fabricated of stainless steel.

Spring. The spring shall wrap around the post between the protector cap and the adjustable stop. The spring shall apply outward force along the axis of the post to the cap and the stop. The spring shall be fabricated of stainless steel.

Base. The base shall be able to be secured to the post. The base shall be able to accommodate the handle ends of the five osteotomes. The base shall be fabricated of a corrosion-resistant metal alloy.

The assembled rack shall have an overall height of 8-1/2 inches and a diameter of 2-1/2 inches. The rack shall be able to stand upright by itself.

Set shall be capable of withstanding repeated sterilizations. Osteotomes shall show no evidence of corrosion when autoclaved at 270 $\pm$ 5 degrees F and 27 $\pm$ 1 PSI for a minimum of 20 minutes.

Identification markings. In addition to the requirements specified in GG-I-526, osteotomes shall be marked "stainless." Manufacturers name (or trademark), manufacturers catalog number, and blade width shall be marked on the instrument. Marking shall be done in a manner that will not impair the mechanical properties or the corrosion resistance of the instrument. In addition, marking shall be located in such a manner as not to intersect the edges of the instrument. Markings shall be located at a point of low stress.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:56Z
Check the source to verify that this is the current version before use.

Workmanship. The osteotome set shall be free from defects which detract from its appearance or impair its serviceability.

Set. (SE). One osteotome set, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Responsibility for compliance. All items must meet all requirements specified herein. The inspection set forth in this specification shall become a part of the contractor's overall inspection system or quality program. The absence of any inspection requirements in the specification shall not relieve the contractor of the responsibility of assuring that all products or supplies submitted to the Government for acceptance comply with all the requirements of the contract. Sampling in quality conformance does not authorize submission of known defective material, either indicated or actual, nor does it commit the Government to acceptance of defective material.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:56Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The acceptable quality level (AQL) shall be 1.0 for an inspection level of S-2. The unit of product for test purposes shall be one osteotome set.

Metric Products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:56Z
Check the source to verify that this is the current version before use.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-107-0188	OSTEOTOME SET, HOKE, Straight, Set of 5

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:


VA-OSS
PHS
FDA-MPQAS

PGC 47129

Project No. 6515-3879

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:56Z
Check the source to verify that this is the currentversion before use.

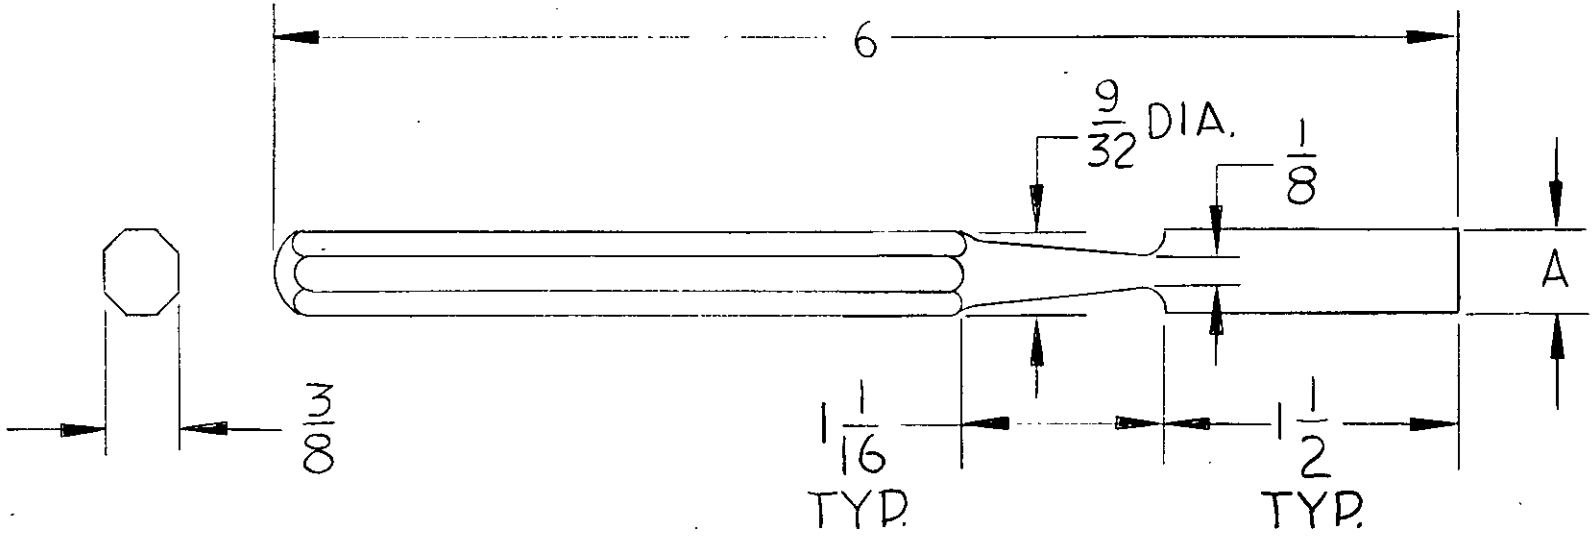

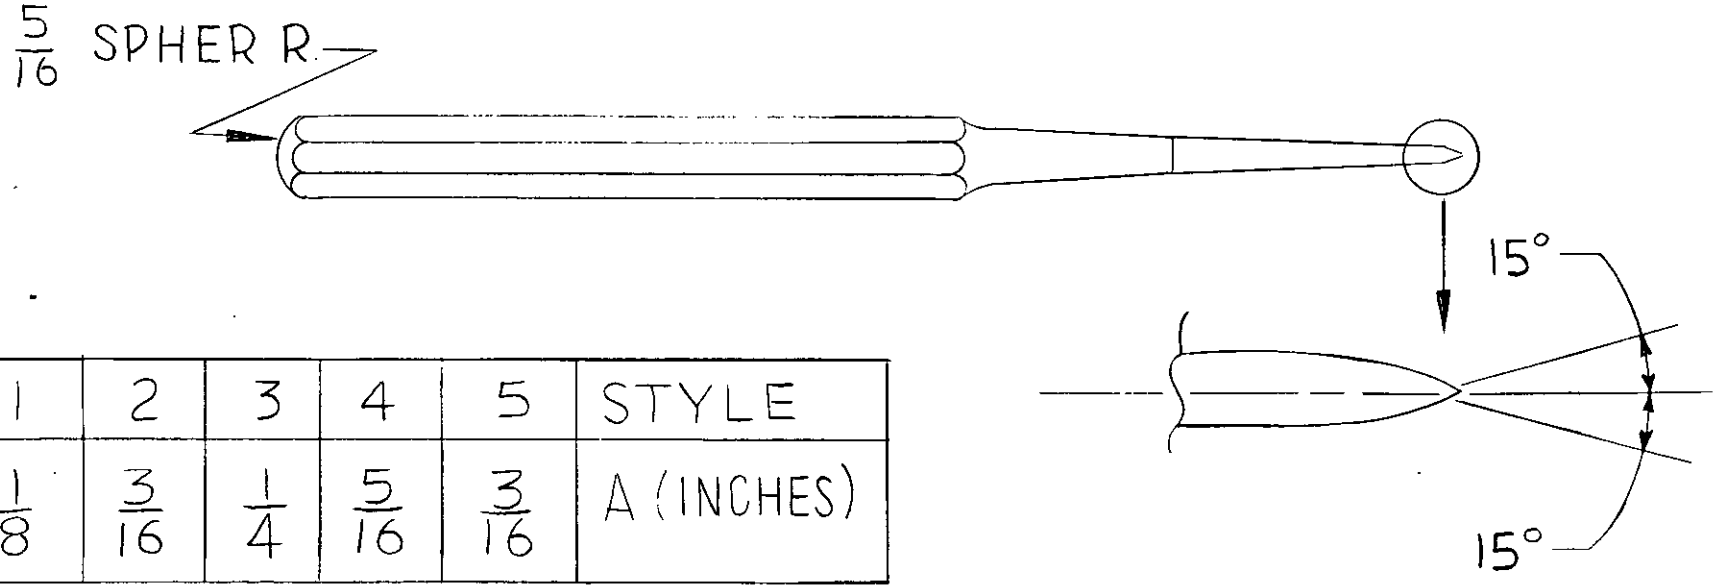

1	2	3	4	5	STYLE
1/8	3/16	1/4	5/16	3/16	A (INCHES)

6515-01-107-0188

BLADE END DETAIL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:56Z
Check the source to verify that this is the current version before use.

FIGURE 1. OSTEOTOME SET, HOKE, STRAIGHT, SET OF 5