A-A-51524
7 July 1986

COMMERCIAL ITEM DESCRIPTION

BLADE and FRAME, DENTAL LABORATORY SAW
(Die Materials)

The General Services Administration has authorized the use of this commercial item description in preference to Military Specification MIL-B-36411 (DM).

This commercial item description covers a saw frame and blade suitable for crown and bridge die cutting.

Class 1 - Saw Frame
Class 2 - Saw Blade

Salient characteristics:

The saw frame shall be suitable for use with the saw blade to form a dental laboratory die saw used in cutting dies from casts in crown and bridge procedures and other dental laboratory operations.

Frame. The U-shaped bow shall be formed of a suitable steel rod connected to a wooden handle by a suitable steel ferrule. The wooden handle shall be thoroughly seasoned, straight clear grained, solid hardwood, suitable for the purpose intended. The frame shall consist essentially of an inverted U-shaped bow, a wooden handle and a connecting steel ferrule. The frame shall be constructed so as to act as a spring for applying proper tension to the blade when in position, and for maintaining blade rigidity and alignment during use. The bow shall be tightly fitted into the wooden handle and all parts shall be securely connected together. The maximum weight of the frame shall be 1-1/2 ounce. The frame shall be of the design and dimensions shown in figure 1. The frame shall be furnished with two (2) blades at the option of the vendor. All metals parts of the frame shall be plated to render them corrosion-resistant. The wooden handle shall be smoothly finished and lacquered or suitably painted black. Each frame shall be legibly and permanently marked with the name or registered trademark of the manufacturer. Instruments of foreign (other than U.S.) manufacture shall also be marked with the name of the country of origin.

AMSC N/A FSC 6520

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:57Z
Check the source to verify that this is the current version before use.

Blade. The blade and pins at each end of the blade shall be fabricated of heat treated steel. The blade shall be flat with teeth filed and set in alternate opposite directions in accordance with standard commercial practice. The blade shall include a securely fitted pin through each end which shall engage and tension the blade into the frame. The blade shall be of the design and dimensions shown in figure 2. The blade shall be hardened and tempered and shall have a Rockwell hardness of C50 to C53. The blade pins shall be hardened and shall have a Rockwell hardness of C35 to C45 when determined in accordance with ASTM Designation E-18 (Rockwell) or E-92 (Vickers or Diamond Pyramid). The back ends of the blade shall have squared, dressed edges.

Workmanship. All parts shall be symmetrically made, smoothly and properly finished, and shall be free from defects which detract from their appearance or may impair their serviceability.

Unit.

Class 1. Each (EA). One (1) saw frame, as specified, constitutes one unit.

Class 2. Package (PG). One package containing six blades, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.


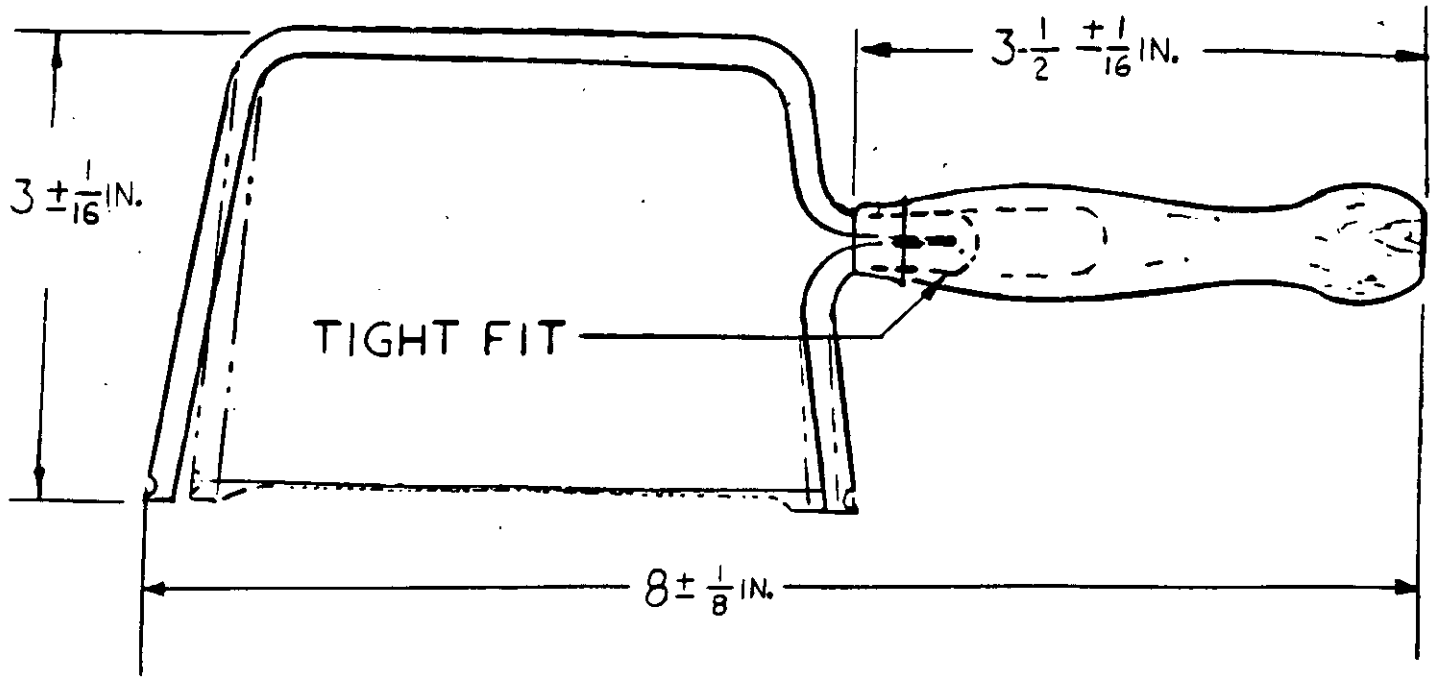


FIGURE 1 : DENTAL LABORATORY SAW, FRAME

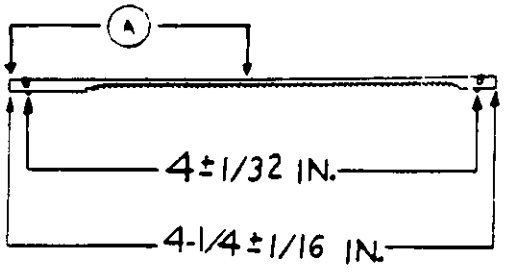

WIDTH OVER TEETH: 0.070 ± 0.004 IN.

THICKNESS OVER TEETH : 0.014 ± 0.001 IN.

18 ± 1 TEETH/IN.

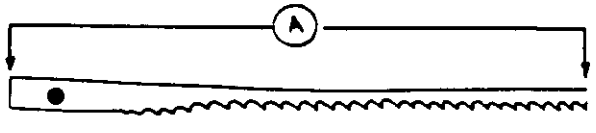


FIGURE 2 : DENTAL LABORATORY SAW, BLADE

Source: https://assist.dla.mil -- Downloaded: 202610-26T08:57Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characteristics. The unit of product for inspection purposes shall be one frame or package of blades. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2.5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:57Z
Check the source to verify that this is the currentversion before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

Stock Number	Item Identification	Designation
6520-00-055-1518	FRAME, DENTAL LABORATORY SAW	Class 1
6520-00-055-1519	BLADE, DENTAL LABORATORY SAW	Class 2

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:57Z
Check the source to verify that this is the current version before use.

A-A-51524

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Civil Agency Coordinating Activity:
VA-OSS

47322
47323

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

Project No. 6520-1929

Location: NCR

☆U.S. GOVERNMENT PRINTING OFFICE: 1988 — 605-036/44830

Source: https://assist.dla.mil -- Downloaded: 202640-26T08:57Z
Check the source to verify that this is the currentversion before use.