KKK-A-1822A
AMENDMENT -2
JULY 1, 1983
SUPERSEDING
AMENDMENT -1
APRIL 1, 1981

FEDERAL SPECIFICATION

AMBULANCE

EMERGENCY MEDICAL CARE SURFACE VEHICLE

THIS AMENDMENT FORMS A PART OF FEDERAL SPECIFICATION KKK-A-1822A DATED APRIL 1, 1980, AND IS APPROVED BY THE GENERAL SERVICES ADMINISTRATION FOR USE BY ALL FEDERAL AGENCIES.

PAGE 1

* PARAGRAPH 1.1 SCOPE. LINE 2, CHANGE "CAN BE" TO "ARE"; AFTER THE LAST SENTENCE, ADD "MILITARY AGENCIES PURCHASING TYPE IIM AMBULANCE, MUST REFER TO THE APPENDIX SECTION (PAGE 59)."

PARAGRAPH 1.1.3 DELETE ENTIRELY AND SUBSTITUTE:

PARAGRAPH 1.1.3 CERTIFIED "STAR OF LIFE" AMBULANCE. AFTER JULY 1, 1981, THE AMBULANCE MANUFACTURER/CONTRACTOR SHALL FURNISH THE PURCHASER(S) CITING THIS SPECIFICATION AN AUTHENTICATED CERTIFICATION AND LABEL (SEE 3.19, PAGE 36) CERTIFYING A "STAR OF LIFE" AMBULANCE. THE CERTIFICATIONS VERIFY THAT THE AMBULANCE FURNISHED COMPLIES WITH THIS SPECIFICATION AND APPLICABLE AMENDMENTS (IF ANY) IN EFFECT ON THE DATE OF MANUFACTURE (SEE 4.3). AMBULANCE VEHICLES SO CERTIFIED MAY DISPLAY THE REGISTERED "STAR OF LIFE" SYMBOL, AS DEFINED BY THE U.S. DEPARTMENT OF TRANSPORTATION (DOT) AND THE NATIONAL HIGHWAY TRAFFIC SAFETY ADMINISTRATION (NHTSA) SYMBOL, SEE FIGURE 4.

PAGE 2

UNDER FEDERAL SPECIFICATIONS, ADD:

* FEDERAL STANDARDS:

FEDERAL STANDARD NO. 297, RUSTPROOFING OF AUTOMOTIVE VEHICLES

(NOTE: RUSTPROOFING IS BEING DELETED FROM MIL. STD. 1223.)

PAGE 3

* MILITARY STANDARDS: CHANGE MIL-STD-1223 TO READ:

"MIL-STD-1223 - NON-TACTICAL WHEELED VEHICLES TREATMENT, PAINTING, IDENTIFICATION MARKING, AND DATA PLATES STANDARD."

PARAGRAPH 2.2 OTHER PUBLICATIONS. UNDER SOCIETY OF AUTOMOTIVE ENGINEERS (SAE), DELETE: "J555: TRUCK, TRUCK-TRACTOR, TRAILER, AND MOTOR COACH WIRING."

ADD TO THE BOTTOM OF THE LIST:

"J1292: AUTOMOBILE, TRUCK, TRUCK-TRACTOR, TRAILER, AND MOTOR COACH WIRING."

PAGE 4

AT THE BOTTOM OF THIS PAGE, ADD:

* 2.3 ORDER OF PRECEDENCE. IN THE EVENT OF A CONFLICT BETWEEN THE TEXT OF THIS SPECIFICATION AND THE REFERENCES CITED HEREIN, THE TEXT OF THIS SPECIFICATION SHALL TAKE PRECEDENCE.

FSC 2310

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

PAGE 5

AFTER PARAGRAPH 3.1.5, ADD:

* 3.1.6 FOUR WHEEL DRIVE, CLASS 2, 4X4. CLASS 2 AMBULANCE SHALL BE THE TRUCK ORIGINAL EQUIPMENT MANUFACTURER'S (OEM) 4X4 VEHICLE, OR SHALL BE AN OEM 4X2 MODEL PROFESSIONALLY ENGINEERED CONVERSION TO A FOUR WHEEL DRIVE VEHICLE, CONFORMING TO ALL APPLICABLE REQUIREMENTS HEREIN.

PAGE 6

PARAGRAPH 3.3 DELETE ENTIRELY AND SUBSTITUTE:

* 3.3 RECOVERED MATERIALS. ALL EQUIPMENT, MATERIAL, AND ARTICLES INCORPORATED IN THIS SPECIFICATION ARE TO BE NEW AND FABRICATED USING MATERIALS PRODUCED FROM RECOVERED MATERIALS TO THE MAXIMUM EXTENT POSSIBLE WITHOUT JEOPARDIZING THE INTENDED USE. THE TERM "RECOVERED MATERIALS" MEANS MATERIALS WHICH HAVE BEEN COLLECTED OR RECOVERED FROM SOLID WASTE AND REPROCESSED TO BECOME A SOURCE OF RAW MATERIALS, AS OPPOSED TO VIRGIN RAW MATERIALS. NONE OF THE ABOVE SHALL BE INTERPRETED TO MEAN THAT THE USE OF USED OR REBUILT PRODUCTS IS ALLOWED UNDER THIS DOCUMENT.

PARAGRAPH 3.4.2 DELETE ENTIRELY AND SUBSTITUTE:

* 3.4.2 TEMPERATURE CONDITIONS. THE AMBULANCE VEHICLE AND THE EXTERIOR MOUNTED EQUIPMENT AND DEVICES SHALL BE CAPABLE OF NORMAL SATISFACTORY PERFORMANCE IN AMBIENT TEMPERATURES OF -30 DEGREES TO +125 DEGREES F., WHEN SERVICED IN ACCORDANCE WITH THE MANUFACTURER'S RECOMMENDATIONS (SEE 4.4). OTHER AMBULANCE EQUIPMENT (INCLUDING MEDICAL DEVICES, EXCEPT RELATED BATTERIES) FURNISHED INSIDE THE AMBULANCE SHALL BE CAPABLE OF NORMAL OPERATION AFTER STORAGE IN -30 DEGREES F. AND +150 DEGREES F. FOR 12 HOURS, THEN OPERATED FOR ONE HOUR AT 0 DEGREES F. AND 110 DEGREES F. AFTER A 5 HOUR STORAGE AT THESE TEMPERATURES. TYPE CERTIFICATIONS ARE ACCEPTABLE WHEN IN ACCORDANCE WITH 4.3.4.

PAGE 7

PARAGRAPH 3.4.10 DELETE ENTIRELY AND SUBSTITUTE:

3.4.10 FORDING. THE VEHICLE SHALL BE CAPABLE OF THREE (3) FORDINGS, WITHOUT STALLING THE ENGINE, OR DAMAGE TO RUNNING GEAR, WHILE BEING DRIVEN THROUGH A MINIMUM OF EIGHT INCHES OF WATER AT SPEEDS OF FIVE TO TEN MPH FOR A DISTANCE OF AT LEAST 100 FEET. TEST UNDER 4.4.4.

PARAGRAPH 3.4.11.6 DELETE ENTIRELY AND SUBSTITUTE:

* PARAGRAPH 3.4.11.6 TURNING CLEARANCE. UNLESS OTHERWISE SPECIFIED, SHALL BE CHASSIS OEM STANDARD.

PAGE 8

PARAGRAPH 3.5.6 DELETE ENTIRELY AND SUBSTITUTE:

3.5.6 CAB TO AXLE (CA) TYPE I AND III VEHICLES. CAB TO AXLE (CA) DIMENSION OF THE VEHICLE CHASSIS SHALL PERMIT A MINIMUM OF 50 PERCENT OF THE OUTSIDE BODY LENGTH FORWARD OF THE REAR AXLE CENTERLINE, INCLUDING THE CAB TO BODY CLEARANCE. BODIES DESIGNED WITH WHEEL OPENING SHALL HAVE THE REAR WHEELS CENTERED ± 2 INCHES WITHIN THE OPENING.

PAGE 9

PARAGRAPH 3.6.4.5 DELETE ENTIRELY AND SUBSTITUTE:

3.6.4.5 COOLING SYSTEM. THE ENGINE COOLING SYSTEM SHALL BE A CLOSED, AIR FREE LIQUID STATE TYPE, WITH A COOLANT OVERFLOW RECOVERY TANK AND COMPENSATING SYSTEM. THE SUPPLIER SHALL PROVIDE THE HEAVIEST DUTY COMPONENTS AND MAXIMUM SIZE COOLING SYSTEM AVAILABLE FROM THE CHASSIS MANUFACTURER APPLICABLE TO THE VEHICLE OFFERED. THE COOLING SYSTEM DESIGN SHALL MAINTAIN THE ENGINE AT SAFE OPERATING TEMPERATURES AT ALL

Source: https://assist.dla.mil -- Downloaded: 20261O-26T12:46Z
Check the source to verify that this is the current version before use.

DRIVEABLE ALTITUDES AND GRADES ENCOUNTERED DURING ON AND OFF ROAD VEHICLE USE. VERIFICATION TEST; THE COOLING SYSTEM SHALL BE CAPABLE OF MAINTAINING A SAFE ENGINE OPERATING TEMPERATURE FOR A PERIOD OF NOT LESS THAN 40 MINUTES AT SEA LEVEL IN AN AMBIENT TEMPERATURE OF 95 DEGREES F., ± 2 DEGREES, AT THE ENGINE SPEED REQUIRED TO MAINTAIN THE GENERATING SYSTEMS AS SPECIFIED IN 3.7.6.

PARAGRAPH 3.6.4.6 EXHAUST SYSTEM. AFTER THE LAST SENTENCE IN THIS PARAGRAPH, ADD THE FOLLOWING:

"EXHAUST TAILPIPE (OUTLETS) SHALL NOT TERMINATE WITHIN SIX INCHES OF THE VERTICAL AXIS OF FUEL FILLER OPENING(S)."

AFTER PARAGRAPH 3.6.5.3, ADD:

* 3.6.5.3.1 HEAVY-DUTY SKID PLATE (CLASS 2, 4X4). UNLESS OTHERWISE SPECIFIED (SEE 6.2), A HEAVY-DUTY SKID PLATE SHALL BE INSTALLED PROTECTING ENGINE AND TRANSMISSION (FROM GROUND CONTACT) IF THERE IS LESS THAN 15 INCHES OF CLEARANCE TO THE GROUND. SKID PLATE SHALL BE DEMOUNTABLE FOR SERVICING THE ENGINE AND TRANSMISSION. OPENINGS SHALL BE PROVIDED TO ENABLE DRAINING OF TRANSMISSION AND SERVICING THE UNDERSIDE OF THE ENGINE. FOR FUEL TANK PROTECTION, SEE 3.6.4.4.

PAGE 11

PARAGRAPH 3.7.2 DELETE ENTIRELY THE PORTION OF THE PARAGRAPH ON THIS PAGE AND SUBSTITUTE THE FOLLOWING:

3.7.2 WIRING INSTALLATION. THE AMBULANCE BODY AND ACCESSORY ELECTRICAL EQUIPMENT SHALL BE SERVED BY CIRCUIT(S) SEPARATE AND DISTINCT FROM VEHICLE CHASSIS CIRCUITS. ALL VEHICLE WIRING SHALL BE COPPER AND CONFORM TO ALL THE SAE J1292 REQUIREMENTS AND HAVE TYPE GPT THERMOPLASTIC OR BETTER INSULATION CONFORMING TO SAE J1128. THE WIRING SHALL BE COLOR CODED OR PERMANENTLY MARKED FOR IDENTIFICATION WITH EASILY READ NUMBERS AND/OR LETTERS AND ROUTED IN CONDUIT OR LOOMS CONFORMING TO SAE J562 AS APPLICABLE. ALL WIRING SHALL BE LOCATED IN ACCESSIBLE, ENCLOSED, AND PROTECTED LOCATIONS AND KEPT AT LEAST SIX INCHES AWAY FROM EXHAUST SYSTEM COMPONENTS. ELECTRICAL WIRING AND COMPONENTS SHALL NOT TERMINATE IN THE OXYGEN STORAGE COMPARTMENT EXCEPT FOR THE COMPARTMENT LIGHT AND SWITCH PLUNGER OR TRIGGER DEVICE. WIRING NECESSARILY PASSING THROUGH AN OXYGEN COMPARTMENT SHALL BE ROUTED IN A METALLIC CONDUIT (SEE 3.11.3). ALL CONDUITS, LOOMS, AND WIRING SHALL BE SECURED TO THE BODY OR FRAME WITH INSULATED METAL CABLE STRAPS IN ORDER TO PREVENT SAGGING AND MOVEMENT WHICH RESULTS IN CHAFING, PINCHING, SNAGGING, OR ANY OTHER DAMAGE. ALL APERTURES ON THE VEHICLE...

PAGE 13

PARAGRAPH 3.7.7 DELETE THE 2ND PARAGRAPH AND SUBSTITUTE:

"BATTERY RATINGS SHALL CONFORM TO SAE J537. BATTERIES SHALL BE LOCATED IN A VENTILATED AREA, SEALED OFF FROM OCCUPANT COMPARTMENTS, AND SHALL BE READILY ACCESSIBLE FOR SERVICING AND REMOVAL. WHEN BATTERIES ARE MOUNTED IN THE ENGINE COMPARTMENT, THEY SHALL BE PROVIDED WITH A HEAT SHIELD AS A SAFEGUARD AGAINST HIGH UNDERHOOD TEMPERATURES."

PAGE 14

PARAGRAPH 3.7.7.3 DELETE ENTIRELY AND SUBSTITUTE:

3.7.7.3 INTERNAL 12 VDC POWER, (REFERENCE FIGURE 5). THE PATIENT COMPARTMENT SHALL BE FURNISHED WITH A 12 VDC, 20 AMPERE CAPACITY, SEPARATELY PROTECTED CIRCUIT, WITH TWO (2) OUTLET RECEPTACLES. THIS CIRCUIT SHALL ALSO INCLUDE A (LOW VOLTAGE DROP) "SCHOTTKY" DIODE TO ISOLATE MEDICAL EQUIPMENT BATTERIES FROM ANY ELECTRICAL LOADS THAT THE REMAINDER OF THE AMBULANCE ELECTRICAL SYSTEM MAY IMPOSE. THE SCHOTTKY DIODE SHALL BE HEAT-SINK MOUNTED, HAVE AN INVERSE VOLTAGE RATING OF AT LEAST 45 VOLTS, AND ALSO BE RATED TO CARRY THE MAXIMUM SHORT CIRCUIT CURRENT UNTIL THE CIRCUIT BREAKER OPENS. THE DIODE SHALL BE PHYSICALLY LOCATED IN AN ACCESSIBLE LOCATION AND BE ELECTRICALLY CONNECTED BETWEEN THE CIRCUIT BREAKER AND THE "ACTION

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T12:46Z
Check the source to verify that this is the currentversion before use.

WALL" MOUNTED RECEPTACLE. UNLESS OTHERWISE SPECIFIED, THE RECEPTACLES SHALL BE A MILITARY TYPE CONNECTOR OF THE FOLLOWING GENERIC DESIGNATION. MS3112E12-3S, OR ITS INTERCHANGEABLE COMMERCIAL EQUIVALENT. THE POLARITY OF THE CONNECTOR SHALL BE AS FOLLOWS: PIN A -+12V, PIN B - GROUND, PIN C - NOT USED. THE RECEPTACLES SHALL BE LOCATED ON A VERTICAL SURFACE OF THE "ACTION WALL." THE MATING PLUG ATTACHED TO THE MEDICAL EQUIPMENT SHALL BE AN MS3116F12-3P OR ITS INTERCHANGEABLE COMMERCIAL EQUIVALENT. THE POLARITY FOR THE PLUG SHALL BE THE SAME AS ABOVE. TWO OF THESE UNWIRED PLUGS SHALL BE FURNISHED AND TAGGED WITH POLARITY REQUIREMENTS AND SHALL BE CONNECTED TO THE RECEPTACLES. (NOTE: THESE CONNECTORS ARE WIDELY AVAILABLE DIRECTLY FROM MOST MAJOR INDUSTRIAL ELECTRONICS DISTRIBUTORS.)

PAGE 15

PARAGRAPH 3.7.12 DELETE ENTIRELY AND SUBSTITUTE:

3.7.12 ELECTROMAGNETIC RADIATION AND SUPPRESSION. IN ADDITION TO OEM CHASSIS, ALL ELECTRICALLY OPERATED OR ELECTRICAL GENERATING DEVICES, INCLUDING ALTERNATORS, AIR CONDITIONING, AND WARNING LIGHT SYSTEMS SHALL BE ELECTROMAGNETIC RADIATION SUPPRESSED, FILTERED, OR SHIELDED TO PREVENT INTERFERENCE TO RADIOS AND TELEMETRY EQUIPMENT ABOARD THE VEHICLE AND THE SURROUNDING AREA. WHEN SPECIFIED UNDER 6.2, THE COMPLETED AMBULANCE VEHICLE SHALL BE TESTED AND CERTIFIED TO PROVE THAT THE RFI DOES NOT EXCEED THE MAXIMUM LIMITS OF SAE J551.

PAGE 16

PARAGRAPH 3.8.2 DELETE ENTIRELY AND SUBSTITUTE:

3.8.2 AMBULANCE EMERGENCY LIGHTING. THE EMERGENCY LIGHTING SYSTEM MUST PROVIDE THE AMBULANCE WITH 360 DEGREES OF CONSPICUITY FOR SAFETY DURING ITS MISSIONS. THE SYSTEM MUST DISPLAY HIGHLY RECEPTIBLE AND ATTENTION-GETTING SIGNALS THAT FUNCTION IN A MODAL SYSTEM AND CONVEY THE MESSAGE IN THE PRIMARY MODE - "CLEAR THE RIGHT-OF-WAY" AND IN THE SECONDARY MODE - "HAZARD VEHICLE STOPPED ON RIGHT-OF-WAY." THE AMBULANCE STANDARD WARNING LIGHT SYSTEM SHALL NOT IMPOSE AN ELECTRICAL LOAD EXCEEDING 40 AMPERES. ADDITIONAL AUXILIARY WARNING LIGHTS, IF SPECIFIED (SEE 6.2), SHALL NOT OBSCURE THE LIGHT OUTPUT OF THE STANDARD WARNING LIGHT SYSTEM. AUXILIARY WARNING LIGHTS FURNISHED SHALL BE SEPARATELY SWITCHED. ANY WARNING DEVICES FURNISHED IN ADDITION TO THE SPECIFIED SYSTEM SHALL BE COMPENSATED FOR WITH RESERVE OR ADDITIONAL GENERATING CAPACITY AS REQUIRED IN 3.7.6.

THE AMBULANCE STANDARD EMERGENCY WARNING LIGHT SYSTEM SHALL CONTAIN TEN (10) FIXED RED LIGHTS AND ONE (1) FIXED CLEAR LIGHT. THESE LIGHTS SHALL FUNCTION IN A DUAL MODE SYSTEM AS SHOWN IN TABLE I, AND MEET THE PHYSICAL AND PHOTOMETRIC REQUIREMENTS OF 3.8.2.1. THE UPPER BODY WARNING LIGHTS SHALL BE IDENTICAL AND MOUNTED AT THE EXTREME UPPER CORNER AREAS OF THE AMBULANCE BODY BELOW THE HORIZONTAL ROOFLINE, WITH THE SINGLE CLEAR LIGHT MOUNTED MIDWAY BETWEEN THE TWO FRONT FACING RED UPPER CORNER LIGHTS (SEE FIGURES 1, 2, AND 3). THE STANDARD WARNING LIGHTS SHALL NOT BE OBSTRUCTED BY DOORS, AUXILIARY LIGHTS, OR SIREN(S). THE RED "GRILLE" LIGHTS SHALL BE LOCATED AT LEAST 30 INCHES ABOVE THE GROUND BUT BELOW THE BOTTOM EDGE OF THE WINDSHIELD AND BE LATERALLY SEPARATED BY AT LEAST 24 INCHES. ALL WARNING LIGHTS FURNISHED SHALL BE MOUNTED TO PROJECT THEIR HIGHEST EFFECTIVE INTENSITY BEAMS ON THE HORIZONAL AXIS.

* PARAGRAPH 3.8.2.1 PHOTOMETRIC AND PHYSICAL REQUIREMENTS. LINE 4, CHANGE "20" TO "45" AND SUBSTITUTE THE FOLLOWING CHART:


MINIMUM EFFECTIVE INTENSITY (CANDELA)

COLOR / CONDITION	RED	CLEAR
DAY	800 CD. @ H-V	3,000 CD. @ H-V
	50 CD. AT ALL 5°V-45°H POINTS	200 CD. AT ALL 5°V-45°H POINTS
NIGHT	10-30% OF ABOVE	

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

PAGE 17

DELETE "FLASH PATTERN" AND SUBSTITUTE THE FOLLOWING:

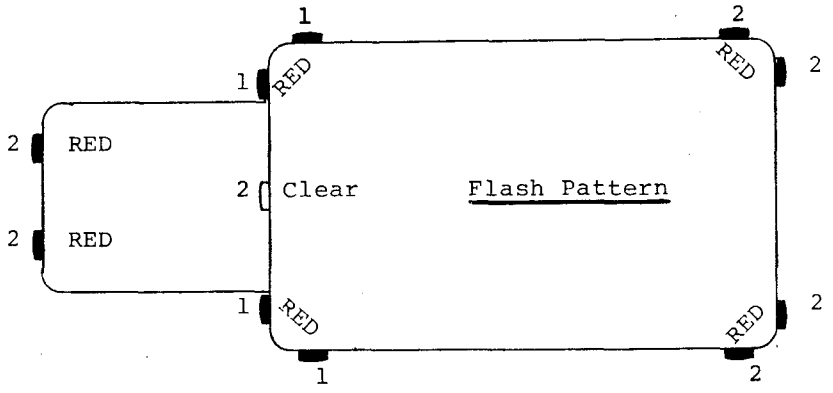

1 - INDICATES LIGHTS FLASHING AT THE SAME TIME
2 - INDICATES LIGHTS FLASHING 180° OUT OF PHASE WITH 1
**THE "TERTIARY MODE" WHICH USES THE VEHICLE'S 4-WAY FLASHERS (DIRECTIONAL SIGNALS) SHOULD ONLY BE USED WHILE THE VEHICLE IS STATIONARY.

PAGE 18

* PARAGRAPH 3.8.2.2 TENTH LINE DOWN AFTER "ACTIVATED" ADD ", AND WHEN FURNISHED THE SETTING OF DAY-NIGHT SWITCH."

PARAGRAPH 3.8.2.3 DELETE ENTIRELY AND SUBSTITUTE:

3.8.2.3 TESTS, WARNING LIGHT SYSTEM. THE AMBULANCE MANUFACTURER SHALL MEASURE AND RECORD THE TOTAL CURRENT LOAD OF THE STANDARD EMERGENCY WARNING LIGHT SYSTEM ON THE VEHICLE AS MANUFACTURED, WHEN OPERATED IN THE MODE WHICH DRAWS MAXIMUM CURRENT. THIS LOAD CURRENT TEST SHALL BE CONDUCTED DURING THE "AMBULANCE'S ELECTRICAL SYSTEM TEST" (3.7.6 AND AMD STD. 005). THE STANDARD WARNING LIGHT SYSTEM AND RELATED COMPONENTS AND DEVICES SHALL BE TESTED, APPROVED, AND LISTED WITH THE AMERICAN ASSOCIATION OF MOTOR VEHICLE ADMINISTRATORS (AAMVA) FOR CONFORMANCE TO THE REQUIREMENTS IN THE SPECIFICATION.

* PARAGRAPH 3.8.3 FLOOD AND LOADING LIGHT (EXTERIOR). LINE 6, CHANGE "1500" TO "800" AND,

DELETE ON LINE 7 THE WORD "TRAPEZOIDAL" AND SUBSTITUTE "FLOOD"; CHANGE THE WORD "EQUIVALENT" TO "SIMILAR".

PARAGRAPH 3.8.5 DELETE ENTIRELY AND SUBSTITUTE:

3.8.5 AMBULANCE INTERIOR LIGHTING. THE BASIC INTERIOR AMBULANCE LIGHTING CONFIGURATION SHALL BE DESIGNED TO MINIMIZE ELECTRICAL LOADS AND INCLUDE: A DRIVER'S COMPARTMENT DOME LIGHT, INSTRUMENT PANEL LIGHTS, MASTER SWITCH PANEL AND CONSOLE LIGHT(S). LIGHTING SHALL BE DESIGNED AND LOCATED SO THAT NO GLARE IS REFLECTED INTO THE DRIVER'S EYES OR HIS LINE OF VISION FROM SWITCH CONTROL PANELS OR OTHER AREAS THAT ARE ILLUMINATED WHILE THE VEHICLE IS IN MOTION. THE PATIENT COMPARTMENT DOMELIGHTING (3.8.5.1) SHALL BE SUFFICIENT AT STEPWELL(S) (3.10.12), AND CONTROL PANEL TO BE CLEARLY VISIBLE OR SEPARATELY ILLUMINATED.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

PAGE 20

* PARAGRAPH 3.9.6.1 DELETE ENTIRELY AND SUBSTITUTE:

3.9.6.1 OVERRIDE FRONT BUMPER GUARD. WHEN SPECIFIED (SEE 3.15.3, ITEM 21), A HIGHRISE HEAVY-DUTY GRILLE GUARD SHALL BE FURNISHED TO PROTECT THE VEHICLE GRILLE, RADIATOR, AND AIR CONDITIONER CONDENSER. THE HEAVY-DUTY GRILLE GUARD SHALL BE CUSTOM FIT TO THE FRONT BUMPER AND BOLTED TO THE VEHICLE FRAME. THE GRILLE GUARD SHALL BE OF ALL WELDED STEEL CONSTRUCTION WITH NOT LESS THAN 3/8-INCH THICK SIDE PLATES AND TWO HORIZONTAL TWO-INCH DIAMETER TUBE CROSSMEMBERS. THE GRILLE GUARD SHALL BE OF A HEIGHT TO EXTEND FROM THE BOTTOM EDGE OF THE FRONT BUMPER TO NOT LESS THAN EIGHT INCHES ABOVE THE TOP EDGE. UNLESS OTHERWISE SPECIFIED, THE GRILLE GUARD SHALL BE CHROME PLATED OR PAINTED TO MATCH THE VEHICLE EXTERIOR COLOR.

PAGE 21

PARAGRAPH 3.10.2 DELETE ENTIRELY AND SUBSTITUTE:

3.10.2 CAB AND BODY ACCESS BETWEEN COMPARTMENTS, TYPE I. THE AMBULANCE AND BODY BULKHEADS SHALL HAVE AN ALIGNED WINDOW OPENING OF AT LEAST 150 SQUARE INCHES FOR VISUAL AND VOICE CHECK OF CONDITIONS IN THE PATIENT'S COMPARTMENT. THE WINDOW OPENING SHALL BE AN ADJUSTABLE, TRANSPARENT, SHATTERPROOF PANEL TREATED OR LOCATED IN THE BULKHEAD(S) TO PREVENT INTERFERRING WITH THE DRIVER'S NIGHT VISION (SEE 3.9.9 AND 3.10.14).

* TABLE II, STYLE 5 -- STANDARD ARMY AND NATO LITTERS (WITH POLES), CORRECT THE DIMENSIONS TO READ: "LENGTH TO 90 (+0, -1/4)," WIDTH TO "23 (+6/10, -3/4)."

PARAGRAPH 3.10.4 DELETE THE THIRD PARAGRAPH "WIDTH", AND SUBSTITUTE:

"WIDTH: THE WIDTH OF THE COMPARTMENT, AFTER INSTALLATION OF THE CABINETS SHALL PROVIDE 18 INCHES ± 6 INCHES OF CLEAR AISLE WALKWAY BETWEEN THE SECURED PRIMARY COT AND THE SQUAD BENCH OR COT."

PAGE 22

PARAGRAPH 3.10.6 DELETE ENTIRELY AND SUBSTITUTE:

3.10.6 AMBULANCE BODY STRUCTURE. ALL PARTS OF THE AMBULANCE BODY AND ATTACHMENTS SHALL BE FASTENED WITH RUST-RESISTANT FASTENERS IN A MANNER WHICH WILL PRECLUDE LOOSENING. CABINETS, BENCHES, PARTITIONS, OXYGEN CYLINDER HOLDERS, GUIDE RAILS, AND COT HOLDERS SHALL BE ATTACHED TO METAL TAPPING PLATES AND/OR FRAMING WELDED TO THE BODY STRUCTURE. THESE COMPONENTS SHALL BE FASTENED BY WELDING, BOLTING, OR USING TAPERED TAPPING SCREWS, AT LEAST ON 24 INCH CENTERS OR LESS AS APPLICABLE TO THE COMPONENT BEING INSTALLED. SELF-TAPPING WOOD/METAL SCREWS OR NAILS SHALL NOT BE USED IN ASSEMBLING THE AMBULANCE EXCEPT FOR LIGHT TRIM PANELS AND WOOD FLOORING.

VEHICLES FURNISHED WITH FIBERGLASS/PLASTIC EXTERIOR ROOF PANEL SHALL HAVE THE CENTER SECTION REINFORCED WITH METAL WIRE SCREENING (SEE 3.14.3 FOR A RADIO ANTENNA GROUND PLANE). AMBULANCE BODIES WITH AN EXTENDED ROOF SHALL HAVE THE ROOF STRUCTURAL MEMBERS PERMANENTLY FASTENED TO STRUCTURAL MEMBERS OF THE BODY (WELDED, BOLTED, AND SEALED) TO PREVENT SEPARATION IN AN ACCIDENT. DRIP RAIL(S) SHALL BE PROVIDED OVER DOORS OF TYPE I AND III OR AROUND THE ENTIRE MODULE UNIT AND HAVE DRAIN POINTS AT EACH CORNER. BODY SKIRT(S) SHALL NOT EXTEND MORE THAN 3 INCHES BELOW THE VEHICLE CAB/BODY. ON TYPE I AND III BODIES, WHEN SPECIFIED (SEE 3.15.3 - 18), A MINIMUM 1X2 INCH PROTECTIVE RUBRAIL ON THE RIGHT AND LEFT SIDES LOCATED IN THE LOWER THIRD SECTION OF THE BODY SHALL BE PROVIDED. THE BODY, ROOF, AND PANEL JOINTS SHALL BE WATERTIGHT. ALL OPENINGS BETWEEN THE CHASSIS-BODY AND OCCUPANT CARRYING COMPARTMENTS DUE TO ALTERATION OR CONSTRUCTION SHALL BE SEALED, INCLUDING THE BULKHEAD SPACE BETWEEN CAB AND BODY OF TYPE I AND III (SEE 3.9.9).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

* PARAGRAPH 3.10.8 DOORS. AFTER THE LAST SENTENCE, ADD:

"THE INTERIOR OF THE UPPER DOOR FRAME(S) SHALL BE PADDED TO PREVENT HEAD INJURY TO PERSONNEL. TWO RED REFLECTORS OF THREE-INCH MINIMUM DIAMETER SHALL BE INSTALLED, ONE ON THE INTERIOR SURFACE OF EACH SIDE OR TOP HINGED REAR DOOR. THE REFLECTORS SHALL BE SO POSITIONED AS TO PROVIDE MAXIMUM VISIBILITY WHEN THE DOORS ARE IN THE FULLY OPEN POSITION. AT THE MANUFACTURER'S OPTION, REFLECTIVE TAPE, DARK RED, CONFORMING TO L-S-300, TYPE I, CLASS 3, REFLECTIVITY 1, MAY BE FURNISHED. THE TAPE SHALL BE FOUR INCHES WIDE AND SHALL EXTEND THE FULL WIDTH OF EACH REAR DOOR PANEL.

PAGE 23

PARAGRAPH 3.10.9 DELETE ENTIRELY AND SUBSTITUTE:

3.10.9 DOOR LATCHES, HINGES, AND HARDWARE. DOOR LATCHES, HINGES, AND HARDWARE FURNISHED BY CHASSIS MANUFACTURERS SHALL COMPLY WITH FMVSS 206. WHEN DOORS ARE OPEN, THE HINGES, LATCHES, AND DOOR-CHECKS SHALL NOT PROTRUDE INTO THE ACCESS AREA. ALL DOORS SHALL HAVE HARDWARE OR DEVICES TO PREVENT INADVERTENT OPENING AND CLOSING. A MINIMUM 6-INCH GRAB HANDLE ON THE INSIDE OF EACH DOOR, IN ADDITION TO A DOOR OPERATING HANDLE; DOOR STOPS TO PREVENT DAMAGE TO BODY SIDES; A HANDLE WITH
* LATCHES OPERABLE FROM INSIDE, EVEN IF KEY LOCKED, AND OUTSIDE OF THE BODY, WITH ONE EXTERNAL OPERATED LOCK WITH KEY PER DOOR OPENING SHALL BE PROVIDED. HARDWARE SHALL BE CHROME PLATED, STAINLESS STEEL, OR ANODIZED ALUMINUM. INSIDE DOOR HANDLES SHALL BE DESIGNED AND PLACED SO THEY CANNOT BE OPERATED (OPENING A DOOR) WHEN ACCIDENTALLY HIT OR USED AS A GRAB HANDLE. AMBULANCE BODY, SIDE AND REAR DOOR HARDWARE INSTALLED BY THE AMBULANCE BODY MANUFACTURER SHALL BE TESTED TO PROVE INSTALLATION MEETS OR EXCEEDS THE REQUIREMENTS OF AMD STANDARD 002 - BODY AND DOOR RETENTION COMPONENTS TESTS.

PARAGRAPH 3.10.15 DELETE ENTIRELY THE PORTION ON THIS PAGE AND SUBSTITUTE:

3.10.15 PARTITION FOR TYPE II AND III VEHICLES. A FULL HEIGHT AND WIDTH PARTITION OR BULKHEAD (WITH OR WITHOUT COMPARTMENTS) HAVING ROLLBAR CHARACTERISTICS AND AN OPENING WITH A DOOR, SHALL BE PLACED BETWEEN THE DRIVER AND PATIENT'S COMPARTMENT. THIS PARTITION SHALL BE LOCATED DIRECTLY BEHIND THE DRIVER AND COMPANION SEATS WHEN IN THE...

PAGE 24

FIRST PARAGRAPH (3.10.15 CONTINUED) DELETE ENTIRELY AND SUBSTITUTE:

"REARMOST POSITION. THE PARTITION SHALL BE SECURED ON THE SIDES, CEILING, AND FLOOR, BY WELDING OR BOLTING TO TAPPING PLATES. A PARTITION OPENING AT LEAST 17 INCHES WIDE AND 46 INCHES HIGH SHALL PROVIDE AN AISLE BETWEEN THE COMPARTMENTS. THE DOOR SHALL HAVE AT LEAST A 150 SQUARE INCH TRANSPARENT SHATTERPROOF VIEWING PANEL IN THE CENTER SECTION AT THE DRIVER'S EYE LEVEL. THE DOOR SHALL BE SECURABLE WITH A SELF-LATCHING DEVICE IN THE OPEN AND CLOSED POSITIONS FROM THE DRIVER'S SIDE (SEE 3.10.2)."

PAGE 26

PARAGRAPH 3.11.3 DELETE ENTIRELY AND SUBSTITUTE:

3.11.3 STORAGE COMPARTMENTS AND CABINETS DESIGN. STORAGE CABINETS, DRAWERS, AND KITS SHALL BE EASILY OPENED BUT SHALL NOT COME OPEN IN TRANSIT. FOR RAPID IDENTIFICATION OF CONTENTS, MEDICAL SUPPLY CABINETS ABOVE THE LITTER PATIENTS SHALL HAVE SHATTERPROOF TRANSPARENT SLIDING DOORS PROVIDED WITH A FINGER PULL OPENING OR RECESSED METAL CUPS OR EQUAL. STORAGE COMPARTMENTS SHALL BE DIVIDED INTO SECTIONS, SHELVES SHALL BE ADJUSTABLE, DRAWERS SHALL BE MARINE STYLE SLIDE OR TILT, AND ALL SHALL BE REMOVABLE. CABINET COMPARTMENT DOORS AND DRAWERS, SLIDING OR HINGED, SHALL AUTOMATICALLY LATCH OR BE FITTED WITH FRICTION HOLDING DEVICES WHEN IN A CLOSED POSITION. SIDE CABINET SHELVES SHALL BE NO MORE THAN 12 INCHES IN DEPTH WHEN LOCATED ABOVE THE VEHICLE BELT LEVEL. STORAGE COMPARTMENTS, CABINETS, AND SUPPORT EQUIPMENT AREA INTERIOR SURFACES SHALL BE FINISHED IN ACCORDANCE WITH 3.10.17. CABINETS SHALL BE FIRMLY ANCHORED (BOLTED OR WELDED) TO TAPPING PLATES OF

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the currentversion before use.

THE BODY STRUCTURE (3.10.6). TOPS OF THE CABINETS AND SHELVES SHALL BE BORDERED OR SURROUNDED BY A LIP OF NOT LESS THAN 1/2 INCH IN HEIGHT. STORAGE FOR THE MAIN OXYGEN CYLINDER (SEE 3.12.1) SHALL BE ACCESSIBLE FOR REPLACEMENT FROM AN OUTSIDE POSITION. THE OXYGEN COMPARTMENT SHALL BE PROVIDED WITH AT LEAST A NINE (9) SQUARE INCH LOUVERED DEVICE LOCATED NEAR OR AT THE TOP OF THE COMPARTMENT, PERMITTING ANY LEAKING OXYGEN GAS TO DISSIPATE/VENT TO THE OUTSIDE OF THE AMBULANCE. OXYGEN CYLINDER COMPARTMENT SHALL NOT BE UTILIZED FOR STORAGE OF ANY OTHER EQUIPMENT. ANY WIRING AND ELECTRICAL DEVICES WITHIN THIS COMPARTMENT SHALL COMPLY TO 3.7.2. OXYGEN CYLINDER(S) SHALL BE MOUNTED WITH A RESTRAINING DEVICE(S), AS REQUIRED FOR THE CRASHWORTHINESS TESTS OF AMD STANDARD 003, OXYGEN TANK RETENTION SYSTEM.

PARAGRAPH 3.11.4 DELETE LINES 13, 14, 15, AND SUBSTITUTE:

* "SQUAD BENCH OR WHEELED COT BENCH SHALL BE FURNISHED WITH AT LEAST THREE (3) SETS OF SAFETY BELTS FOR SEATED OCCUPANTS, AND TO RESTRAIN STYLE 3 STRETCHER WHEN POSITIONED ON THE BENCH. SEATBELTS SHALL COMPLY TO FMVSS 209. THE ANCHORAGES FOR THE SIDE FACING SEATBELT ASSEMBLY SHALL WITHSTAND A MINIMUM OF 2,500 POUND FORCE WHEN TESTED IN ACCORDANCE WITH FMVSS 210-S5.2."

PAGE 27

PARAGRAPH 3.11.9 DELETE ENTIRELY AND SUBSTITUTE:

3.11.9 IV HOLDERS FOR INTRAVENOUS FLUID CONTAINERS. TWO NEAR FLUSH STYLE, IV CEILING HOLDERS OR HOOKS WITH STRAPPING DEVICE TO TIE AND CONTROL IV BAGS/BOTTLES SHALL BE PROVIDED. THE CEILING HOLDERS SHALL BE LOCATED ADJACENT TO THE SIDE WALL, AT THE HEAD OF THE PRIMARY PATIENT AND ONE AT THE HEAD OF THE SECONDARY PATIENT'S COT (SQUAD BENCH). WHEN SPECIFIED IN 3.15.4, CODE M2, A DETACHABLE TYPE, RIGID TELESCOPING IV POLE AND HOLDER, WITH A 52 INCH MINIMUM HEIGHT, WHEN EXTENDED, SHALL BE PROVIDED THE STYLE 1 COT. IT SHALL BE MOUNTED ON THE LEFT SIDE AT THE FRONT END OF THE COT.

PAGE 28

PARAGRAPH 3.12.1.1 LINE 6, DELETE THE FOLLOWING:

* "A MAXIMUM FLOW RATE OF 300 LITERS PER MINUTE (LPM) WITH A FULL TANK AND"

PAGE 30

PARAGRAPH 3.13.1 AFTER THE LAST SENTENCE, ADD:

"CONNECTING HOSES FOR THE HEATING AND AIR CONDITIONING SYSTEMS SHALL BE SUPPORTED AT LEAST EVERY 12 INCHES BY RUBBER INSULATED METAL CLAMPING DEVICES."

PARAGRAPH 3.13.4 AND 3.13.5 FOURTH LINE DOWN, DELETE "(FLOOR TO CEILING)".

PAGE 36

PARAGRAPH 3.17 DELETE ENTIRELY AND SUBSTITUTE:

* 3.17 UNDERCOATING. UNLESS THE AMBULANCE IS RUSTPROOFED, THE VEHICLE SHALL BE UNDERCOATED FOR SOUND DEADENING, CORROSION, AND STONE DAMAGE PROTECTION. A COMMERCIAL, SANDLESS PETROLEUM BASE UNDERCOATING MATERIAL SHALL BE APPLIED TO THE UNDERBODY AND UNDER CHASSIS SHEET METAL SURFACES TO A THICKNESS OF 1/16 TO 1/8 INCH - EXCEPT TO THE DRIVE SHAFTS, DRAIN HOLES, LUBRICATION POINTS, ENGINE CRANKCASE, HEAVY CASTINGS, SUSPENSION COMPONENTS, HEAT SHIELDS, HEAT DIFFUSING DEVICES, CATALYTIC CONVERTERS, AND AREAS 10 INCHES OR LESS FROM THE EXHAUST SYSTEM(S). THESE AREAS SHALL BE KEPT FREE OF COATING MATERIAL. CHASSIS FRAME, UNDERSIDE OF ENGINE COMPARTMENT HOOD, AND UNDERBODY SURFACES IN EXCESS OF 1/8 INCH THICKNESS, OR THAT ARE INACCESSIBLE WITHOUT REMOVING VEHICLE FUEL TANK(S) OR OTHER MAJOR COMPONENTS SHALL NOT REQUIRE UNDERCOATING.

PARAGRAPH 3.18, SECOND LINE, DELETE "MIL-STD-1223," AND SUBSTITUTE "FED. STD. NO. 297."

Source: https://assist.dla.mil -- Downloaded: 20260-26T12:46Z
Check the source to verify that this is the current version before use.

PAGE 40

PARAGRAPH 4.3.1 SECOND LINE, CHANGE "JANUARY 1, 1981" TO "JULY 1, 1981".

PAGE 41

PARAGRAPH 4.4.2 LINE "H" - CHANGE TO READ:

"ELECTROMAGNETIC RADIATION TESTS. TYPE APPROVAL ACCEPTABLE, (SEE 3.7.12)"

PAGE 43

PARAGRAPH 6.2 ORDERING DATA, ITEM (G) WHEELS, AFTER: "DESIRED", DELETE: "IF TYPE I".

PAGE 47

PARAGRAPH 6.9 DELETE ENTIRELY AND SUBSTITUTE:

* 6.9 CHANGES AND AMENDMENTS. WHEN A USING AGENCY AND PURCHASER CONSIDER THAT THIS SPECIFICATION REQUIRES REVISION, A WRITTEN REQUEST FOR CHANGE OR ADDITIONS TO THE DOCUMENT SUPPORTED BY ADEQUATE JUSTIFICATION SHALL BE SENT TO THE GENERAL SERVICES ADMINISTRATION, OFFICE OF FEDERAL SUPPLY AND SERVICES, AUTOMOTIVE COMMODITY CENTER (FAE), WASHINGTON, DC 20406, FOR APPROPRIATE ACTION. THE AGENCY WILL BE INFORMED OF ACTION TAKEN. NEW AND REVISED INFORMATION REGARDING THIS SPECIFICATION MAY BE ISSUED FROM TIME TO TIME UNDER AN AMENDMENT TO THE FEDERAL SPECIFICATION. THESE AMENDMENTS ARE IDENTIFIED BY THE SAME NUMBER AND TITLE AS THE DOCUMENT AND ARE ON GREEN PAPER. AMENDMENTS SHOULD BE RETAINED UNTIL SUCH TIME AS THE ENTIRE DOCUMENT IS REVISED.

* DELETE COORDINATION ACTIVITIES AND SUBSTITUTE THE FOLLOWING:

MILITARY COORDINATION ACTIVITY:
ARMY - AT

ACTIVITIES:

AIR FORCE - 84-99
ARMY - AT-EL-CR-ER-MD
NAVY - YD-MC

CUSTODIAN & PREPARING ACTIVITY:
GSA-FSS-FAE

CIVIL AGENCY ACTIVITIES:

USDA - APHIS
INTERIOR - BIA
STATE DEPARTMENT - AID
DOT - NHTSA-EMS
DOE
HEW-EMS
VA-DM-S
DC GOVERNMENT

PAGE 58

* AFTER PAGE 58, ADD: APPENDIX, PAGES NUMBERED 59 THROUGH 75.

NOTE: THE MARGINS OF THIS AMENDMENT ARE MARKED WITH AN ASTERISK (*) TO INDICATE WHERE CHANGES FROM THE PREVIOUS AMENDMENT WERE MADE. THIS WAS DONE AS A CONVENIENCE ONLY AND THE GOVERNMENT ASSUMES NO LIABILITY WHATSOEVER FOR ANY INACCURACIES IN THESE NOTATIONS. BIDDERS AND CONTRACTORS ARE CAUTIONED TO EVALUATE THE REQUIREMENTS OF THIS DOCUMENT BASED ON THE ENTIRE CONTENT IRRESPECTIVE OF THE MARGINAL NOTATIONS AND RELATIONSHIP TO THE LAST PREVIOUS AMENDMENT.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:46Z
Check the source to verify that this is the currentversion before use.

APPENDIX

SPECIFICATION FOR MILITARY AMBULANCE

EMERGENCY MEDICAL CARE SURFACE VEHICLE

10. SCOPE AND CLASSIFICATION

10.1 SCOPE. THIS APPENDIX IS AN EXTENSION OF THE REFERENCED DOCUMENT, INCLUDING AMENDMENTS IF ANY, AND DETAILS THE MILITARY REQUIREMENTS FOR THE EMERGENCY AMBULANCE. TO SPECIFY, FOLLOW THE "ORDERING DATA" 60.2 (PAGE 71).

10.2 CLASSIFICATION. THIS APPENDIX COVERS THE FOLLOWING CLASSIFICATION AND SELECTION OF MILITARY AMBULANCES (TO SPECIFY, SEE 60.2).

TYPE II M - STANDARD VAN, FORWARD CONTROL (FC) INTEGRAL CAB-BODY, MILITARY EMERGENCY AMBULANCE (3.1.3 AND FIGURE 2).

CLASS 1 - TWO REAR WHEEL DRIVEN (4X2).

CLASS 2 - FOUR WHEEL DRIVEN (4X4).

FLOOR PLAN AA - (ARMY USAGE 30.1.2).

FLOOR PLAN AN - (NAVY USAGE 30.1.2).

20. APPLICABLE DOCUMENTS

20.1 UNLESS OTHERWISE SPECIFIED, THE REFERENCED DOCUMENTS OF SECTION 2 OF THE SPECIFICATION SHALL APPLY.

30. REQUIREMENTS

30.1 GENERAL REQUIREMENT. WHEN THIS APPENDIX IS SPECIFIED, IT SHALL AMEND SOME OF THE REQUIREMENTS OF THE REFERENCE DOCUMENT. IT CONTAINS DETAILED DESCRIPTION OF DEVIATIONS, ADDITIONS, SUBSTITUTIONS AND SERVICES WHICH SHALL BE PROVIDED AS SPECIFIED. IN THE EVENT OF A CONFLICT BETWEEN SPECIFICATIONS, THOSE HEREIN (APPENDIX) SHALL TAKE PRECEDENCE. THE AMBULANCE AND COMPONENT ITEMS AUTHENTICALLY CERTIFIED FOR TYPE II AMBULANCE, NEED NOT BE RECERTIFIED IF MODIFIED TO COMPLY TO THE (APPENDIX) MILITARY REQUIREMENTS IN ORDER TO DISPLAY THE CERTIFICATION "STAR OF LIFE" SYMBOL.

30.1.1 TYPE II M AMBULANCE. EXCEPT AS OTHERWISE SPECIFIED HEREIN, THIS AMBULANCE SHALL CONFORM TO 3.1.3 FOR THE CLASS SELECTED.

THE CABINETS, BENCH STORAGE COMPARTMENTS, AND PARTITION SHALL BE CONSTRUCTED OF MARINE GRADE PLYWOOD CONFORMING TO CLASS 1 OF MIL-P-18066, OR MEDIUM DENSITY PRESSED WOOD, WITH PRESSURE BONDED LAMINATE ON BOTH FACES, WITH MATERIAL THICKNESS OF NOT LESS THAN 5/8 INCHES, EXCEPT FOR BACKS AND SHELVES. THE INTERIOR OF THE BODY SIDES AND DOORS SHALL BE LINED WITH WASHABLE HIGH STRENGTH FORMICA OR MARLITE PANELS OR AN APPROVED EQUIVALENT. ALL EXPOSED EDGES OF CABINETS, BENCH STORAGE COMPARTMENTS, AND PARTITIONS THAT ARE ROUGH OR HAVE GAPS SHALL BE PROVIDED WITH BRIGHT FINISH, CORROSION-RESISTANT METAL TRIM. CABINETS AND BENCH COMPARTMENTS WITH LITTER AND COT HOLDER ATTACHMENTS SHALL BE REINFORCED TO WITHSTAND SUDDEN STRESSES IMPOSED BY THE LOADED COTS AND LITTERS DURING SUDDEN STOPS. REINFORCEMENTS SHALL INCLUDE METAL ANGLE BRACKETS BETWEEN THE SIDES OF THE CABINETS AND COMPARTMENTS AND THE FLOOR. THE PARTITION OR BULKHEAD SHALL BE WITHOUT WALK-THRU OPENING, BUT SHALL BE FURNISHED IN THE CENTER SECTION A SLIDING LAMINATED GREEN TINTED SAFETY GLASS OR 1/4 INCH PLEXIGLASS TO ALLOW THE DRIVER TO VIEW THE PATIENT'S COMPARTMENT AND PERMIT VOICE COMMUNICATION BETWEEN COMPARTMENTS. THE SLIDING PANEL SHALL BE NOT LESS THAN 40 INCHES IN LENGTH AND 12 INCHES IN HEIGHT. THE SLIDING WINDOW PANEL SHALL BE PROVIDED WITH A FINGER PULL OPENING WITH RECESSED METAL CUPS. THE PARTITION WINDOW FRAME SHALL BE APPROXIMATELY FLUSH WITH THE PARTITION TO PRECLUDE HEAD INJURY.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

30.1.2 Floor Plans for Type II M. The ambulance shall be provided with the following patient and EMT (attendant) loading accommodations (modifies 3.1.5, Plan A):

Plan AA - Squad bench, storage cabinets and equipment arrangement for ARMY usage (see appendix figures 1, 2, 5, 6, and 7) loading (A) through (D) below, and one (1) seated attendant.

Plan AN - Squad bench, storage cabinets and equipment arrangement for NAVY usage (see appendix figures 3 and 4) loading (A) through (D) (below), and two (2) seated attendants.

(A) One patient in a Navy stokes litter (style 4) on the floor and one patient in a Navy stokes litter (style 4) on the curbside bench
(B) One patient on an elevating cot (style 1) on the floor and one patient in a Navy stokes litter (style 4) on the curbside bench
(C) One patient on an elevating cot (style 1) on the floor and four seated patients on the curbside bench
(D) One patient on an elevating cot on the floor and one patient in a NATO litter (style 5) on the curbside bench

(Dimensions of Army and NATO litter: L 90 (+0, -1/4) in; W 23 (+6/10, -3/4) in; Height 6 3/4 (+0) in.

(Patient weight is computed at 175 pounds each.)

30.2 Vehicle Operation, Performance and Physical Characteristics.

30.2.1 Vehicle Performance. Except as otherwise specified, the basic specification requirements of part 3.4 and 3.5 shall be provided.

30.2.2 Speed. The ambulance shall be capable of 70 mph speed, when tested in accordance to 3.4.6.

30.2.3 Payload Allowance. Minimum payload of 1400 pounds, in lieu of 1000 pounds specified in 3.5.2 shall be provided. (Compute occupant weight at 175 pounds each.)

30.3 Chassis, Power Unit and Components.

30.3.1 Chassis Components. Except as otherwise specified shall comply to 3.6 to 3.7 of the specification.

For the purposes of establishing minimum component capacities, the capacity of axles, springs, and tires shall be at least equal to the load imposed at the ground, with the complete vehicle with a full compliment of fuel and lubricants and loaded with full specified payload.

30.3.2 Power Plant Heaters. When specified (see 60.2) in lieu of power plant heaters of 3.6.3.2.1, the supplier shall provide the following coolant and battery heaters. Heaters shall operate on 115-volt alternating current (ac), unless otherwise specified, these 115 VAC power plant heater(s) shall be switched and connected to the vehicle's 115 VAC system (see 3.7.8 and figure 6) so that it can only be energized from utility power. When 115 VAC utility power is not furnished the heaters shall be wired through a junction block to a single, three-pronged (male), weatherproof, slave receptacle for receiving external power and grounding the vehicle. A three-wire connecting cable, 25 feet long and of adequate line capacity to supply power for all heater units simultaneously, shall be furnished. The connecting cable shall include a matching female connector at the vehicle end and a standard three-pronged (two power plus one ground) male connector at the other end. Electrical apparatus shall conform to Federal Motor Carrier Safety Regulation 393.77 (c)(7). Electrical insulation of the connecting cable shall withstand normal operating stresses in low ambient air temperatures (down to minus 60 F) without cracking or loss of dielectric capacity. All heater lead wires shall be installed without interfering with vehicle component operation, and without loose, excess wire. A carrier for the connecting cable shall be mounted within the vehicle and shall provide positive cable retention during vehicle operation. Heaters shall be furnished as follows:

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

(A) COOLANT HEATER, 1,500-WATT MINIMUM RATING, SHALL BE INSTALLED IN THE ENGINE BLOCK OR LOWER, COOLANT, INLET HOSE. AN ENGINE THERMOSTAT WITH AN OPERATING RANGE OF 170 F TO 195 F SHALL BE INSTALLED.

(B) BATTERY HEATER SHALL HAVE A CAPACITY ADEQUATE TO MAINTAIN THE BATTERY ELECTROLYTE AT A TEMPERATURE OF NOT LESS THAN 10 F DURING VEHICLE EXPOSURE IN AMBIENT AIR TEMPERATURES AS LOW AS MINUS 60 F, AND SHALL EMBODY A THERMOSTAT TO LIMIT THE TEMPERATURE OF ELECTROLYTE TO NOT MORE THAN 80 F.

30.3.3 GASOLINE ENGINE. TYPE II M AMBULANCE SHALL BE V8 TYPE PER 3.6.3.3.

30.4 ELECTRICAL SYSTEM AND COMPONENTS.

30.4.1 ELECTRICAL SYSTEMS. UNLESS OTHERWISE SPECIFIED THE ELECTRICAL SYSTEMS SHALL COMPLY TO 3.7 THRU 3.8 OF THE SPECIFICATION, EXCEPT 3.7.8 TO 3.7.8.3 (115VAC) IF FLOOR PLAN AN (NAVY AMBULANCE UNIT NOT REQUIRED).

30.5 LIGHTING, AMBULANCE EXTERIOR AND INTERIOR.

30.5.1 LIGHTING SYSTEMS AND COMPONENTS. EXCEPT AS MODIFIED HEREIN OR ELSEWHERE SHALL COMPLY TO 3.8.

30.5.2 AMBULANCE LOW MOUNT WARNING LIGHTS (3.8.2). THESE WARNING LIGHTS SHALL BE MOUNTED BEHIND THE OVERRIDE BUMPER (SEE 30.6.2) IN THE VICINITY OF THE VEHICLE FRONT GRILLE. THE LIGHTS SHALL BE RED, EXCEPT FOR VEHICLES DESTINED FOR EUROPE THE LIGHTS SHALL BE BLUE. THE WARNING LIGHTS SHALL BE INSTALLED WITH THE CENTERLINE OF THE LIGHTS, AS CLOSE AS PRACTICAL, ON A HORIZONTAL PLANE THROUGH THE CENTERLINE OF THE VEHICLE FRONT HEADLIGHTS.

30.5.3 AMBULANCE EMERGENCY WARNING LIGHTS. WHEN SPECIFIED (SEE 60.2) THE AMBULANCE(S) DESTINED FOR EUROPE SHALL HAVE ALL THE RED (COLOR) WARNING LIGHTS OF 3.8.2, IN BLUE COLOR.

30.5.4 REMOVAL OF LIGHTS FOR SHIPMENT. AT THE OPTION OF THE MANUFACTURER OR WHEN SPECIFIED (SEE 60.2), THE WARNING LIGHT, SPOTLIGHT(S), AND FLOODLIGHT(S) SHALL BE REMOVED FOR SHIPMENT WHERE IT WILL RESULT IN A REDUCTION IN OVERALL VEHICLE SHIPPING CUBAGE. WHEN REMOVED, THE LIGHT(S) SHALL BE STOWED WITHIN THE VEHICLE AND THE ROOF OPENING SHALL BE PROVIDED WITH WEATHERTIGHT COVER(S). PROVISIONS FOR REINSTALLING THE LIGHT(S), INCLUDING ACCESS TO THE LIGHT WIRING AND MOUNTING DEVICES FROM INSIDE THE VEHICLE, SHALL BE PROVIDED.

30.5.5 LIGHTING SWITCH CONTROLS. ADDITIONAL SWITCHES TO CONTROL THE FLOODLIGHTS SHALL BE PROVIDED AT THE REAR DOOR.

30.5.6 TWO SPOTLIGHTS (3.8.4). WHEN SPECIFIED (SEE 60.2), TWO SPOTLIGHTS SHALL BE FURNISHED IN LIEU OF A SINGLE SPOTLIGHT, MOUNTED SO THAT ONE IS LOCATED FOR CONVENIENT ACCESS BY THE DRIVER, THE OTHER FOR USE BY THE ASSISTANT DRIVER/ATTENDANT. SPOTLIGHTS SHALL HAVE INSIDE CONTROLS, AND SHALL BE MOUNTED THROUGH THE WINDSHIELD HEADER SECTION. INTERIOR CONTROLS SHALL BE LOCATED TO MINIMIZE POSSIBLE SAFETY HAZARD. SPOTLIGHTS SHALL BE MOUNTED SO THAT THEY WILL NOT RESTRICT THE VISIBILITY OF THE WARNING LIGHT.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:46Z
Check the source to verify that this is the current version before use.

30.5.7 PATIENTS; COMPARTMENT LIGHTS FOR PLAN AA. (MODIFYING 3.8.5.1). LIGHTING SHALL INCLUDE TWO 120-VOLT, 40-WATT FLUORESCENT LIGHTS WITH INSTANT START AND NOT LESS THAN 48-INCH TUBE LENGTHS. INVERTER BALLAST DEVICES TO PERMIT OPERATION FROM THE 12-VOLT ELECTRICAL SYSTEM SHALL BE FURNISHED. THE FLUORESCENT FIXTURES SHALL HAVE TRANSLUCENT POLYCARBONATE BOTTOM COVERS, READILY REMOVABLE FOR REPLACEMENT OF THE FLUORESCENT TUBES. END CAPS SHALL BE PADDED TO REDUCE THE POSSIBILITY OF INJURY TO PERSONNEL. THE FIXTURES SHALL BE MOUNTED TO PRECLUDE DAMAGE FROM VEHICLE MOTION AND VIBRATION AND SHALL PROJECT NO MORE THAN THREE INCHES BELOW THE CEILING. ONE FLUORESCENT LIGHT SHALL BE MOUNTED SO THAT THE FORWARD END OF THE FIXTURE SHALL BE OVER THE FORWARD END OF THE STYLE 1 AMBULANCE COT WHEN THE COT IS CLAMPED IN THE TRANSPORT POSITION. LATERALLY, IT SHALL BE TO THE STREET (LEFT) SIDE OF THE VEHICLE CENTERLINE, LOCATED TO PROVIDE CLEARANCE FROM THE STREET CABINET TOP TO THE LIGHT OF NINE INCHES, TO PERMIT PLACEMENT AND STORAGE OF ARMY LITTER(S), STYLE 5 ON THE TOP OF THE STREETSIDE CABINET (SEE FIGURES 6 AND 7). THE SECOND FLUORESCENT LIGHT SHALL BE MOUNTED LATERALLY TO THE CURB (RIGHT) SIDE OF THE VEHICLE CENTERLINE OVER THE CURB SIDE BENCH, DIRECTLY IN LINE WITH THE STREET SIDE FLUORESCENT LIGHT. ADDITIONALLY, TWO DOMELIGHTS SHALL BE CEILING MOUNTED, ONE OVER THE CURB SIDE BENCH, APPROXIMATELY TWELVE INCHES TO THE REAR OF THE BENCH FRONT, AND THE SECOND OVER THE STREET SIDE COT, APPROXIMATELY TWELVE INCHES TO THE REAR OF THE COT FRONT. THE DOMELIGHTS SHALL PROTRUDE FROM THE CEILING NOT MORE THAN 1 INCH AND SHALL PROVIDE NOT LESS THAN 40 FOOT-CANDLES AT THE LEVEL OF THE PATIENT(S) HEAD ON A STYLE 5 LITTER ON THE CURBSIDE BENCH AND A STYLE 1 COT ON THE STREETSIDE. SEPARATE SWITCHES SHALL BE PROVIDED FOR THE FLUORESCENT LIGHTS AND THE DOMELIGHTS AT BOTH THE FORWARD AND REAR COMPARTMENT PANELS. THE SWITCHES FOR THE DOMELIGHTS SHALL BE OF THE DIMMER TYPE.

30.5.7.1 PATIENT COMPARTMENT LIGHTING FOR PLAN AN (MODIFYING 3.8.5.1). AT LEAST EIGHT (8) DOME LIGHTS SHALL BE INSTALLED IN THE CEILING OF THE PATIENTS' COMPARTMENT. EACH LAMP SHALL BE OF THE HIGH-LOW INTENSITY TYPE AND SHALL PROVIDE LIGHTING OF NOT LESS THAN 40-FOOT CANDLES AT THE LEVEL OF THE LITTER PATIENT WHEN ON HIGH INTENSITY MODE. DOME LIGHTS SHALL BE RECESSED INTO THE CEILING AND THE LENS SHALL NOT PROTRUDE BELOW CEILING LEVEL MORE THAN ONE INCH. THE DOME LIGHTS SHALL BE INSTALLED IN TWO ROWS OF FOUR EACH WITH THE LEFT ROW DIRECTLY OVER THE STYLE 1 COT AND THE RIGHT ROW AN EQUAL DISTANCE FROM THE ROOF CENTERLINE AS THE LEFT ROW. THE TWO FRONT DOME LIGHTS SHALL BE LOCATED NOT MORE THAN 36 INCHES FROM THE PARTITION AND THE TWO REAR DOME LIGHTS SHALL BE LOCATED APPROXIMATELY 18 INCHES FROM THE REAR DOOR WITH THE TWO REMAINING LIGHTS IN EACH ROW SPACED EVENLY BETWEEN THE FORWARD AND REAR LIGHTS. THE DOME LIGHTS SHALL BE OPERATED BY FOUR SWITCHES LOCATED ON THE PATIENTS' COMPARTMENT SWITCH PANEL AND SHALL BE WIRED AS FOLLOWS (LIGHT NUMBERING SYSTEM IS FROM FRONT TO REAR 1,2,3 AND 4 IN EACH ROW:

(A) ONE SWITCH TO OPERATE LIGHTS 1 AND 2 LEFT.
(B) ONE SWITCH TO OPERATE LIGHTS 1 AND 2 RIGHT.
(C) ONE SWITCH TO OPERATE LIGHTS 3 LEFT AND 3 RIGHT.
(D) ONE SWITCH TO OPERATE LIGHTS 4 LEFT AND 4 RIGHT.

TWO ADDITIONAL SWITCHES SHALL BE PROVIDED ON THE SWITCH PANEL AT THE REAR DOOR:

(A) ONE SWITCH TO OPERATE LIGHTS 1 AND 2 LEFT.
(B) ONE SWITCH TO OPERATE LIGHTS 4 LEFT AND 4 RIGHT.

30.5.7.2 REAR FLOODLIGHT AND STEP LIGHT FOR PLAN AA & AN, (MODIFYING 3.8.3 AND 3.8.5). SIDE FLOODLIGHTS ARE NOT REQUIRED ON THE TYPE IIM AMBULANCE. A FLOODLIGHT SHALL BE MOUNTED TO THE REAR ROOF OF THE BODY, OVER THE REAR DOORS, WHICH PROVIDES LIGHTING AT GROUND LEVEL TO ALL POINTS AT THE REAR OF THE VEHICLE, TWO FEET OR MORE. THE FLOODLIGHT SHALL BE SWIVEL MOUNTED WHICH PROVIDES FOR VERTICAL AND HORIZONTAL ADJUSTMENT. A SWITCH SHALL BE LOCATED AT THE REAR DOOR WHICH ACTIVATES THE LIGHT WHEN DOORS ARE OPENED. A DASH MOUNTED SWITCH SHALL BE PROVIDED TO OVERRIDE THE DOOR SWITCH. TWO REAR BUMPER STEP LIGHTS SHALL BE FURNISHED TO ILLUMINATE THE REAR STEP. A SWITCH WHICH AUTOMATICALLY TURNS ON THE LIGHTS WHEN THE DOORS ARE OPENED SHALL BE FURNISHED.

30.6 CAB-BODY DRIVER COMPARTMENT AND EQUIPMENT.

30.6.1 CAB-BODY PROVISIONS. UNLESS OTHERWISE SPECIFIED, SHALL CONFORM TO 3.9.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

30.6.2 Heavy Duty Grille Guard Plans AA and AN (Unless Deleted). A heavy duty grille guard shall be furnished to protect the vehicle grille, radiator, and air conditioner condenser. The heavy duty grille guard shall be custom fit to the front bumper and bolted to the vehicle frame. The grille guard shall be of all welded steel construction with not less than 3/8-inch thick side plates and two horizontal two-inch diameter tube crossmembers. The grille guard shall be of a height to extend from the bottom edge of the front bumper to not less than eight inches above the top edge. The grille guard shall be chrome plated or painted to match the vehicle exterior colors. Guard must not block low mount warning lights. Grill warning lights shall be rearward of the front edge of the bumper guards for the protection of the lights.

30.7 Ambulance Body and Patient Area.

30.7.1 Body Accommodations. Except as modified herein, and unless otherwise specified shall be furnished in accordance to 3.10 to 3.11. In addition, The ambulance body proper and patient compartment shall be sufficient in size to transport occupants as specified in plan AA or AN (see 30.1.2), and accommodate and store all the stretchers, cots, and litters through the range of dimensions specified in table II. The patients' compartment shall accommodate two seated EMT (attendants) for plan AN, and one seated attendant for plan AA, modifying 3.10.3.

30.7.2 Doors (3.10.8). The side door shall be the manufacturer's standard sliding door with safety glass window in upper section.

30.7.3 Door Latches (3.10.9). The rear door shall be furnished with a latch operable from inside and out and with a lock mechanism key type on outside and plunger/button type inside similar to those furnished on forward driver/passenger doors. The door shall at no time be locked in such a manner that it cannot be unlocked from inside patients' compartment.

30.7.4 Floor Covering (3.10.11). No wax vinyl or linoleum shall be provided.

30.7.5 Partition (3.10.15). Shall not have a door opening, in the partition (see 30.1.1).

30.7.6 Interior Surfaces (3.10.17). Patient compartment ceiling inner shell of the roof shall serve as a ceiling of the patients' compartment. The inner shell shall be molded, reinforced fiberglass or acrylonitrile butadiene styrene (ABS) material. The shell shall include built-in, molded recesses for ceiling mounted equipment including lights, vents, support eyes, and IV solution hooks, enabling all items to be retained within the ceiling when not in use, except ceiling lights and IV solution hooks may extend not more than 1/2-inch below vehicle ceiling.

30.8 Storage Compartments and Facilitations.

30.8.1 Patient Compartment Facilities (3.11). Unless otherwise specified (see 60.2) the patient compartment facilities shall comply to that specified below in lieu of 3.11 through 3.11.9, with the exception of applicable requirements of 3.11.1.1; 3.11.3, and 3.11.7.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

30.8.2 Bench and Storage Compartment (Plan AA and AN). The longitudinal bench with upholstered seat and separate back shall be mounted on the right (curbside) of the vehicle. The bench shall be capable of accommodating four passengers with a minimum of 19 inches provided for each passenger. The bench seat shall provide support for the style 4 and 5 litters specified in Table II (page 21), and shall have storage space underneath. The bench seat shall be hinged at the back with a full length piano hinge or butt hinges and shall serve as a top for the storage compartment. Bench seat hinges shall be adequate to allow the seat to support not less than 800-pound passenger weight and to support the seat in the upright position with the vehicle stationary or in transit. The hinged seat shall be provided with stay(s) to support the seat when in the raised position. The storage compartment shall run the full length of the bench and interior dimensions shall be not less than 76 inches long, 18 inches wide, and 14 inches high. The width of the bench seat shall be not less than 23 and not more than 24 inches. The storage compartment shall be provided with two clear 1/4-inch plexiglass sliding doors in the side of the compartment to provide maximum accessibility to the compartment. A center support at the front of the compartment, between the doors is acceptable. Doors shall be provided with recessed finger pulls, opening with recessed cups, and shall be positive locking or equipped with friction holding devices. Hardware, catches, brackets, and hinges shall be heavy duty.

30.8.2.1 Bench Seat. The bench seat shall be padded with flexible, polyester urethane foam. The foam shall be non-allergenic, flame retardant, non-toxic, and shall reject moisture and body odors. The density shall be 2.0 pounds per cubic foot to 2.4 pounds per cubic foot. The firmness of the foam shall be 35 pounds to 70 pounds at a 25 percent deflection over an area of 50 square inches. The foam padding shall be capable of withstanding 100 percent humidity and an ambient temperature from minus 65 F to plus 125 F with no evidence of deformation or cell breakdown. Flexible latex polyester foam padding is unacceptable. Thickness of the padding shall be two inches. The padding shall be covered with a washable non-absorbent artificial leather or vinyl having a nylon backing of not less than 32 ounces per square yard. The seat and backrest shall be designed so as to not require removal or shall not hamper the effectiveness of the vehicle when utilized to transport cot or litter patients.

30.8.3 Stretchers, Cots, and Litters. The vehicle shall be capable of accommodating the stretchers, cots, and litters through the range of dimensions specified in 3.10.1, table II. When specified (see 60.2), a style 3 stretcher conforming to Ferno Washington Number 11 or equivalent shall be furnished. Stretcher shall be of the folding type with two castered wheels, two legs, and straps for holding the patient in the stretcher. When specified (see 60.2), a style 1 cot conforming to Ferno Washington Model 30 All-Level or equivalent shall be furnished. Cot shall include foot pulls, head pull handles, a three-inch thick polyester mattress with a vinyl coated nylon fabric cover and straps for holding a patient in the cot. The mattress pad and cover and the stretcher bottom shall be of fire retardant material.

30.8.3.1 Stretcher and cot holders. A quick detachable and adjustable cot holder of the one piece plunger type, Ferno Washington Model 175.5, or equivalent, operable with the style 1 cot (see 30.8.3) shall be installed on the street side lower cabinet of section three. When a style 3 stretcher is specified (see 30.8.3), post cups and wheel cups for holding the stretcher on the right-hand side of the floor shall be installed.

30.8.4 Safety Straps. Three two-inch wide nylon safety straps with proper anchors shall be provided to strap in a litter patient at the chest, waist, and knees when an Army litter is placed on the bench seat or bench litter support. Litters are loaded head forward. Each strap shall be not less than 72 inches in length. Two additional straps shall be provided to preclude movement of the litter. It is intended that the straps be applied to the exposed litter pole, nearest the vehicle curbside, at litter head and foot. All of the safety straps and buckles shall be of the automotive seat belt type and quality. Safety strap attachment hardware shall preclude undue wear of the strap webbing at the point of attachment. All safety straps shall be of sufficient length for the stipulated intended usage, and shall be provided with means for rapid adjustment.

30.8.5 Backrest (plan AN). For vehicles furnished in accordance with plan AN, the seat backrest shall be (permanently) mounted to the curbside wall above the seat from the curbside door opening to the curve at the rear of the body. The backrest shall be not less than 12 inches in height. The top edge of the backrest shall be not less than 18 inches above the unloaded seat cushion. The backrest foam padding shall be in accordance with 30.8.2.1.

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:46Z
Check the source to verify that this is the current version before use.

30.8.6 Combination Backrest/Litter Support Panel (plan AA). For vehicles furnished in accordance with plan AA, a combination backrest/litter support panel shall be furnished, and shall be designed to adequately support a patient on a standard Army litter (see table II) in the "DOWN" position and to provide a bench backrest in the "UP" position. The panel shall be of the hinged type, shall be not less than 63 inches in length, and shall be mounted behind the bench seat on the curbside wall (see appendix figure 1). Two latches shall be furnished to secure the panel in the "UP" position (see appendix figure 2). When in the "UP" position, the panel shall become part of the curbside wall. When in the "DOWN" position, the top section of the panel shall serve as a litter support and shall be furnished with litter skid strips (see 30.8.6.1), and shall extend minimally into the aisle. When in the "UP" position, the outside surface of the panel shall provide a foam-padded backrest conforming to 30.8.2.1. When in the "DOWN" position, the backrest shall lie flush with the top of the bench seat. The backrest shall be centered along the support panel, shall run the full length of the panel, and shall extend not less than 3 inches beyond the rear (back door) end of the panel. The panel shall be designed so as to not require removal or shall not hamper the effectiveness of the vehicle when utilized to transport litter patients.

30.8.6.1 Litter Skid Strips (plan AA). For vehicles furnished in accordance with plan AA, litter skid strips shall be furnished. Two parallel 2 3/4 inch (inside) x 1/2 inch x 1/8 inch stainless steel channels shall be fixed to the top (when in the folded down position) of the combination backrest/litter support panel (see 30.8.6) on 21 1/4 inch ± 1/8 inch centers. The channels shall have a litter stop at the forward end of each channel to prevent movement of the litter stop at the forward end of each channel to prevent movement of the litter during sudden deceleration. Skid strips shall run the length of the bench seat. Channels are for sliding standardized (Army and NATO-STANAG 2040) litters along the litter support. The channel toward the center of the vehicle shall locate the aisle side edge of the litter support legs. The channel toward the curbside of the vehicle shall be located so that its centerline is not less than 2 3/8 inches from the wall.

30.8.7 Back Board Stowage (plan AA and AN). For type II M vehicles, provisions for stowing a long and short back board shall be furnished within the vehicle. For plan AN vehicles, quick release type retaining devices for the back boards shall be so located so that the stowed back boards will not interfere with the function or operation of the ambulance in any manner. The long back board shall be stowed on the curbside under bench top for plan AN and as specified in 30.8.8.2 for plan AA vehicles. The stowage facility for plan AA shall hold the spine boards without rattling or vibration and shall allow ready removal of the spine boards. The long back board maximum size measures 18 inches by 72 inches overall and is fabricated of 3/4-inch plywood with 3/4-inch runners. The short back board maximum size shall measure 18 inches by 34 inches overall, and shall be of 3/4-inch thick plywood and shall be provided when code M12 in 3.15.4 is specified. For plan AA vehicles, the back boards shall be furnished with pull handles at the head end to facilitate removal from the stowage area.

30.8.8 Plan AA. Type II M ambulances furnished in accordance with plan AA shall be further provided with bench, storage cabinets, and equipment as specified in 30.8.8 through 30.8.8.7. Equipment arrangement shall conform generally to appendix figures 5, 6, and 7.

30.8.8.1 Attendant's Seat and Oxygen Storage Cabinet. A rear facing attendant's seat, with hinged seat lid, shall be provided over the streetside end of a compartment for "H" oxygen cylinder storage at the front of the patient compartment. The piano hinged seat shall be approximately 16 inches deep, 22 inches wide, and 18 inches high, and shall be equipped with a seat belt. It shall be located (laterally) so that it can be raised without interference with the streetside cabinets. A backrest, comparable to that for the curbside bench (30.8.4), of appropriate length shall be provided. Stays to support the seat in the raised position shall be provided. The seat and backrest shall be upholstered as specified for the bench (see appendix figure 6).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

30.8.8.2 FRONT STORAGE COMPARTMENT ARRANGEMENT. THE STORAGE COMPARTMENT UNDER THE ATTENDANT'S SEAT SHALL RUN THE WIDTH OF THE VEHICLE (TO THE INBOARD EDGE OF THE STEP-WELL, IF ONE IS PROVIDED) AT THE REAR OF THE PARTITION. IT SHALL PROVIDE FOR STORAGE AND CRASHWORTHY RETENTION OF AN "H" OXYGEN CYLINDER AND SHALL PROVIDE SPACE FOR A REGULATOR, INCLUDING GAGE(S), AT THE CURBSIDE END. PROVISION SHALL BE MADE FOR VIEWING OF AND ACCESS TO THE REGULATOR FROM INSIDE THE PATIENT COMPARTMENT WHEN THE SIDE VEHICLE DOOR IS CLOSED, BY MEANS OF A TRANSPARENT PLEXIGLASS SLIDING OR HINGED DOOR IN THE CURBSIDE END OF THE REAR FACE OF THE COMPARTMENT. A PIANO HINGED DOOR SHALL BE PROVIDED IN THE RIGHT (CURBSIDE) END OF THE COMPARTMENT TO FACILITATE THE OXYGEN CYLINDER EXCHANGE AND SERVICING. THE DESIGN SHALL PROVIDE FOR PROTECTION OF THE COMPARTMENT FROM DAMAGE DURING CYLINDER EXCHANGE, AND FOR EASY ACCESS TO THE RESTRAINTS FOR THE CYLINDER. THE OXYGEN TANK RETENTION SYSTEM SHALL CONFORM TO AMD STANDARD 003. A WRENCH FOR CONNECTING AND DISCONNECTING THE REGULATOR AND CYLINDER SHALL BE PROVIDED AND SECURELY STOWED IN A CONVENIENT LOCATION. THE SPACE ABOVE THE CYLINDER AND UNDER THE ATTENDANT'S SEAT SHALL BE CONSTRUCTED TO PROVIDE ADDITIONAL STORAGE. ALONGSIDE THE ATTENDANT'S SEAT, ABOVE THE CYLINDER COMPARTMENT, SHALL BE A STORAGE CABINET WITH SLIDING PLEXIGLASS DOORS (WITH 1 1/4-INCH DIAMETER FINGER HOLES) AND A ONE-INCH LIP TO PREVENT THE CONTENTS FROM SLIDING OUT WHEN DOORS ARE OPEN. THE TOP OF THIS CABINET SHALL BE PROVIDED WITH A 2 1/2-INCH LIP ON THE ENDS AND REARWARD FACING EDGE (OVER THE CABINET DOORS) TO PREVENT EQUIPMENT PLACED ON THE SHELF FROM SLIDING OFF. THE FORWARD EDGE SHALL BE AGAINST THE PARTITION. THIS SHELF SHALL BE NOT LESS THAN THREE INCHES BELOW THE BOTTOM EDGE OF THE PARTITION WINDOW, AND COVERED OR FINISHED FOR EASE OF CLEANING AND FOR RESISTING DAMAGE FROM STORED EQUIPMENT. THE PREFERRED MEANS FOR STOWING TWO SPINE BOARDS (SEE 30.8.7) SHALL BE A COMPARTMENT WHICH WILL PERMIT STANDING THEM ON EDGE, WITH THEIR LONG DIMENSION CROSSWISE OF THE VEHICLE, TO BE PROVIDED BETWEEN THE PARTITION AND THE OXYGEN CYLINDER STORAGE COMPARTMENT, OR IN THE FRONT OF THE PARTITION. ACCESS SHALL BE BY MEANS OF A PIANO HINGED DOOR AT THE CURBSIDE END OF THE COMPARTMENT, TO PERMIT REMOVAL OF THE SPINE BOARDS THROUGH THE PATIENT COMPARTMENT CURBSIDE DOOR. IF THE VEHICLE WIDTH IS INADEQUATE FOR THE PREFERRED CROSSWISE STORAGE OF THE LONG SPINE BOARD OR IF THE PATIENT COMPARTMENT CURBSIDE SLIDING DOOR LOCATION WILL NOT PERMIT CURBSIDE ACCESS, AN ALTERNATIVE LOCATION UNDER THE CURBSIDE BENCH SEAT OR IN A WEATHERPROOF AND SPLASHPROOF FLOOR COMPARTMENT MAY BE USED.

30.8.8.3 STREETSIDE STORAGE CABINETRY AND EQUIPMENT. STORAGE CABINETRY AND EQUIPMENT SHALL BE FURNISHED ON THE STREETSIDE (LEFT SIDE) OF THE PATIENTS' COMPARTMENT, AS DESCRIBED HEREIN. THE CABINETS SHALL CONFORM GENERALLY TO APPENDIX FIGURES 5, 6, AND 7. STORAGE CABINETRY SHALL RUN THE LENGTH OF THE PATIENTS' COMPARTMENT. THE DEPTH OF THE CABINETRY SHALL BE NOT LESS THAN EIGHT INCHES NOR MORE THAN 12 INCHES AS REQUIRED TO ENCASE THE WHEELWELL MEASURED AT FLOOR LEVEL AND SHALL EXTEND VERTICALLY TO A HEIGHT ADEQUATE TO INCORPORATE ALL THE CABINETRY SHOWN IN APPENDIX FIGURES 5, 6, AND 7. ALL SLIDING DOORS SHALL BE 1 1/4-INCH DIAMETER TO PERMIT EASE OF OPENING. ALL SHELVES SHALL BE PROVIDED WITH A 3/4 TO ONE INCH LIP TO PREVENT MATERIAL FROM SLIDING OFF WHILE THE VEHICLE IS IN MOTION AND THE DOORS ARE OPEN. THE CABINET COMPARTMENT DOORS (SLIDING AND HINGED) SHALL BE POSITIVE LOCKING OR FITTED WITH FRICTION HOLDING DEVICES. CHANNELS FOR SLIDING DOORS SHALL BE LINED WITH MATERIAL TO REDUCE RATTLES. THE SPARE WHEEL ASSEMBLY SHALL BE LOCATED IN A SUITABLE LOCATION ON THE EXTERIOR OF THE VEHICLE (SEE 3,6,10).

30.8.8.4 STREETSIDE SECTION 1. THE UPPER PART OF THE FIRST SECTION BEHIND THE PARTITION SHALL BECOME PART OF THE SECTION 2 ACTION WALL. THIS SECTION SHALL PROVIDE A SUITABLE STORAGE SPACE AND SHALL BE FURNISHED WITH MOUNTING BRACKET(S) AND AN ELECTRICAL RECEPTACLE OF THE QUICK-DISCONNECT (NOT SCREW-IN) TYPE FOR THE PORTABLE BATTERY POWERED SUCTION UNIT DESCRIBED IN 30.9.3. BELOW THE TOP OF THE ATTENDANT'S SEAT, THIS SECTION WILL PROVIDE SPACE FOR THE BOTTOM OF THE "H" OXYGEN CYLINDER AND THE END OF THE LONG SPINE BOARD.

30.8.8.5 STREETSIDE SECTION 2. THE SECOND SECTION SHALL BE APPROXIMATELY 24 INCHES WIDE. THE UPPER PORTION OF THIS SECTION SHALL HAVE A BACKING RECESSED SIX TO EIGHT INCHES FROM THE FACE OF SECTION 1 AND SHALL EXTEND FROM A FLOOR LEVEL SHELF OF THE LOWEST CABINET OF SECTION 1 TO THE SAME HEIGHT AS SECTION 1. THE SHELF AT THE BOTTOM OF THIS RECESSED AREA SHALL HAVE A 1 1/2 INCH LIP AT THE OUTER EDGE. A WELL FOUR INCHES IN DIAMETER AND APPROXIMATELY THREE INCHES DEEP SHALL BE PROVIDED IN THE SHELF TO HOLD A SCREW CAP JAR (FSN 6530-00-985-7241). THE WELL SHALL BE LOCATED SO THAT THE JAR IS READILY ACCESSIBLE FOR OXYGEN OUTLETS FREE FOR A PREASSEMBLED OXYGEN BAG, VALVE MASK UNIT (SEE APPENDIX FIGURES 5 AND 7). THE OXYGEN AND SUCTION CONNECTORS (SEE 30.9.1.1 AND 30.9.2.1) SHALL BE MOUNTED ON THE VERTICAL BACK WALL (TOWARD THE STREETSIDE OF THE BODY) OF THIS UPPER PORTION. THE INSTALLATION SHALL BE DESIGNED TO PERMIT ACCESS FOR SERVICING THE VACCUM AND OXYGEN SYSTEMS. THE BOTTOM OF SECTION 2 SHALL HAVE ACCESS DOOR(S) TO PERMIT STORAGE OF EQUIPMENT AND SUPPLIES. DOOR(S) SHALL NOT INTERFERE WITH THE COT HOLDER.

Source: https://assist.dla.mil -- Downloaded: 2026l0-26T12:46Z
Check the source to verify that this is the currentversion before use.

30.8.8.6 STREETSIDE SECTION 3. THE THIRD SECTION SHALL INCLUDE A COMPARTMENT TO THE REAR OF THE WHEELWELL FOR FUTURE STORAGE OF A (STYLE 3) STAIR CHAIR, FERNO WASHINGTON MODEL 40 OR EQUAL, SO DESIGNED THAT THE STAIR CHAIR CAN BE REMOVED WITHOUT REMOVING THE PATIENT ON THE COT FROM THE VEHICLE. CLAMP(S) OR STRAP(S) SHALL BE PROVIDED TO SECURE THE STAIR CHAIR POSITIVELY WHEN NOT IN USE. THIS COMPARTMENT SHALL BE COVERED WITH A SOLID DOOR HINGED FORWARD WITH FULL LENGTH PIANO HINGE, IN A MANNER TO PERMIT SIDE OPENING AND EASY ACCESS TO THE STAIR CHAIR. STORAGE CABINETS, WITH SLIDING PLEXIGLASS DOORS, SHALL BE PROVIDED IN SECTION 3 AS SHOWN IN APPENDIX FIGURE 7. THE BOTTOM OF THE LOWER CABINET(S) SHALL BE AT THE LEVEL OF THE SHELF AT THE BOTTOM OF THE RECESSED AREA OF SECTION 2. BELOW THE SLIDING DOOR CABINETS, A DOOR, HINGED AT THE BOTTOM, SHALL BE PROVIDED TO GIVE ACCESS TO THE SPACE AROUND THE WHEELWELL FOR ADDED STORAGE. BETWEEN THE CABINETRY AND THE ROOF, THERE SHALL BE PROVIDED STORAGE SPACE FOR ONE ARMY LITTER (STYLE 5, TABLE II) EXTENDING FROM THE REAR OF THE VEHICLE FORWARD 95 INCHES, AND EQUIPPED WITH MEANS TO RETAIN THE STYLE 5 LITTER SECURELY DURING VEHICLE MOVEMENT. THE SPACE FORWARD OF THE LITTER STORAGE AREA BETWEEN THE CABINETS OF SECTION 1 AND SECTION 2 AND THE ROOF SHALL BE ENCLOSED AS A CEILING CABINET AND PROVIDED WITH TRANSPARENT SLIDING OR HINGED DOOR(S) AND LIP AS IN OTHER CABINETS (APPENDIX FIGURE 5).

30.8.8.7 I V HOLDERS FOR INTRAVENOUS FLUID CONTAINERS (PLAN AA). IN LIEU OF THE I V HOLDERS IN 3.11.9, THE FOLLOWING SHALL BE FURNISHED: A CEILING MOUNTED TRACK WITH THREE TROLLEY HOOKS FOR SUPPORTING INTRAVENOUS BOTTLES OR BAGS SHALL BE PROVIDED. PROVISIONS FOR LOCKING THE HOOKS IN POSITION ALONG THE TRACK SHALL BE PROVIDED. THE TRACK SHALL BE NOT LESS THAN FIVE FEET LONG, AND SHALL BE ATTACHED TO THE CEILING SO THAT IT IS CENTERED LONGITUDINALLY OVER THE COT WHEN THE COT IS IN THE COT HOLDER. LATERALLY, THE TRACK SHALL BE MOUNTED OVER THE COT, BETWEEN THE LIGHT(S) AND THE GRAB RAIL. TRACK AND ADJUSTABLE HOOKS SHALL BE ARNCO NC100 WITH THREE-INCH HOOKS CEILING MOUNTED CUBICLE TRACK (EXTRUDED ALUMINUM BOX CHANNEL 1 3/8 INCH X 3/4 INCH), NO. 12 ROLLER CARRIERS AND END STOPS, OR EQUAL.

30.8.9 PLAN AN. TYPE II M AMBULANCES FURNISHED IN ACCORDANCE WITH PLAN AN SHALL BE FURTHER PROVIDED WITH THE BENCH, STORAGE CABINETS, AND EQUIPMENT AS SPECIFIED IN 30.8.9 THROUGH 30.8.9.8. EQUIPMENT ARRANGEMENT SHALL CONFORM GENERALLY TO APPENDIX FIGURES 3 AND 4.

30.8.9.1 ATTENDANT'S BENCH. A REAR FACING ATTENDANT'S BENCH WITH A HINGED SEAT LID AND STORAGE COMPARTMENT SHALL BE INSTALLED IN FRONT OF THE PATIENTS' COMPARTMENT AT THE PARTITION. HINGES SHALL BE OF THE HEAVY-DUTY TYPE. THE STORAGE COMPARTMENT SHALL BE APPROXIMATELY 55 INCHES LONG BY 14 INCHES WIDE BY 14 INCHES HIGH. THE HINGED SEAT SHALL BE 16 INCHES DEEP AND OF A LENGTH TO PERMIT RAISING THE SEAT WITHOUT INTERFERENCE WITH THE STORAGE COMPARTMENTS DESCRIBED IN 30.8.9.3. THE COMPARTMENT SHALL BE PROVIDED WITH A SLIDING PLEXIGLASS WINDOW OR HINGED PLEXIGLASS DOOR TO VIEW THE PRESSURE GAGE ON OXYGEN BOTTLES STORED WITHIN AND SHALL BE LARGE ENOUGH TO PERMIT ADJUSTMENT BY THE ATTENDANT. STAYS SHALL BE PROVIDED TO SUPPORT THE SEAT WHEN IN THE RAISED POSITION. THE BACKREST SHALL BE NOT LESS THAN 12 INCHES IN HEIGHT WITH THE TOP EDGE LOCATED DIRECTLY BELOW THE PARTITION WINDOW. THE SEAT AND BACK SHALL BE UPHOLSTERED AS SPECIFIED IN 30.8.2.1.

30.8.9.2 STORAGE COMPARTMENT ARRANGEMENT. THE STORAGE COMPARTMENT UNDER THE ATTENDANT'S BENCH SHALL HAVE PROVISIONS TO FACILITATE THE LOADING, UNLOADING, AND SECURING OF AN "H" SIZE OXYGEN TANK COMPLETE WITH VALVE, PRESSURE REGULATOR, AND ASSOCIATED PIPING. THE MOUNTING AND RESTRAINTS FOR THE OXYGEN CYLINDER SHALL BE CRASHWORTHY UNDER ALL CONDITIONS. THE OXYGEN TANK RETENTION SYSTEM SHALL CONFORM TO AMD STANDARD 003. A HINGED OPENING SHALL BE PROVIDED AT THE RIGHT END (CURBSIDE) OF THE STORAGE COMPARTMENT TO FACILITATE OXYGEN TANK EXCHANGE AND SERVICING. THE STORAGE COMPARTMENT SHALL BE PROVIDED WITH MEANS TO PROTECT THE COMPARTMENT FROM DAMAGE DURING CYLINDER EXCHANGE OPERATIONS.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

30.8.9.3 STREETSIDE STORAGE CABINETRY AND EQUIPMENT. STORAGE CABINETRY AND EQUIPMENT SHALL BE FURNISHED ON THE STREETSIDE (LEFT SIDE) OF THE PATIENTS' COMPARTMENT, AS DESCRIBED HEREIN. THE CABINETS SHALL CONFORM GENERALLY TO APPENDIX FIGURES 3 AND 4. MATERIALS, CONSTRUCTION, AND TRIM SHALL CONFORM TO 3.10.17 AND 3.11.3. STORAGE CABINETRY SHALL RUN THE LENGTH OF THE PATIENTS' COMPARTMENT. THE DEPTH OF THE CABINETRY, MEASURED AT THE FLOOR LEVEL, SHALL BE NOT LESS THAN EIGHT INCHES AND NOT MORE THAN THE DEPTH REQUIRED TO ENCASE THE WHEEL WELL. THE CABINET FACING SHALL EXTEND VERTICALLY TO A HEIGHT ADEQUATE TO INCORPORATE ALL THE CABINETRY SHOWN IN APPENDIX FIGURES 3 AND 4. ALL SLIDING DOORS SHALL BE 1/4 INCH PLEXIGLASS AND SHALL HAVE FINGER-TIP OPENINGS WITH RECESSED METAL CUPS TO PERMIT EASE OF OPENING. ALL SHELVES SHALL BE PROVIDED WITH A 3/4 TO ONE INCH LIP TO PREVENT MATERIAL FROM SLIDING OFF WHILE THE VEHICLE IS IN MOTION AND THE DOORS ARE OPEN. CABINET COMPARTMENT DOORS (SLIDING AND HINGED) SHALL BE POSITIVE LOCKING OR FITTED WITH FRICTION HOLDING DEVICES. CHANNELS FOR ALL SLIDING DOORS SHALL BE LINED WITH MATERIAL TO REDUCE RATTLES.

30.8.9.4 STREETSIDE CABINET SECTION 1. THE FIRST SECTION BEHIND THE PARTITION SHALL BE APPROXIMATELY 30 INCHES WIDE. THE LOWER PORTION OF SECTION 1 SHALL BE AN ENCLOSED COMPARTMENT HAVING A VERTICAL HEIGHT LEVEL WITH THE TOP OF THE ATTENDANT'S SEAT. ACCESS TO THIS COMPARTMENT SHALL BE THROUGH A 10 INCH SQUARE, SOLID, DROP-HINGED DOOR LOCATED THREE INCHES ABOVE THE FLOOR AND ONE INCH IN FRONT OF THE ATTENDANT'S BENCH. IMMEDIATELY ABOVE THIS COMPARTMENT, A SLIDING DOOR CABINET SHALL BE PROVIDED. THIS CABINET SHALL BE APPROXIMATELY 14 TO 15 INCHES HIGH AND SHALL HAVE TWO ADJUSTABLE SHELVES. THE BOTTOM OF THIS CABINET SHALL BE EVEN WITH THE TOP OF THE ATTENDANT'S SEAT. A SLIDING DOOR CABINET, WITH ONE FIXED SHELF SHALL BE PROVIDED IN THE AREA REMAINING IN SECTION 1.

30.8.9.5 STREETSIDE CABINET SECTION 2. THE SECOND SECTION SHALL BE 18 INCHES WIDE. THE TOP AND BOTTOM PORTION OF THIS SECTION SHALL BE FLUSH WITH SECTIONS 1 AND 3. THE TOP PORTION SHALL BE 18 INCHES WIDE AND APPROXIMATELY 20 INCHES HIGH. THE LOWER PORTION SHALL BE 18 INCHES WIDE AND 18 INCHES HIGH. THE CENTER PORTION SHALL BE RECESSED NOT LESS THAN SIX INCHES AND SHALL HAVE A WIDTH OF 18 INCHES. A DUAL OXYGEN OUTLET SHALL BE FLUSH MOUNTED AND CENTERED IN THE UPPER PORTION OF SECTION 2 AT A HEIGHT TO PRECLUDE ANY INTERFERENCE WITH THE RECESSED PORTION, WITH THE OXYGEN FLOW METER AND HUMIDIFIER INSTALLED. THE RECESSED AREA SHALL ACCOMMODATE THE PORTABLE SUCTION UNIT SPECIFIED IN 30.9.3. THE WALL MOUNT BRACKETS FURNISHED WITH THE SUCTION UNIT SHALL BE MOUNTED ON THE REAR FLAT SURFACE OF THE RECESSED AREA FOR THE STORAGE AND IN-VEHICLE OPERATION OF THE SUCTION UNIT. A QUICK DISCONNECT RETAINING STRAP SHALL BE PROVIDED TO SECURE THE SUCTION UNIT WHILE IN TRANSIT. THE 12 VOLT PLUG OF THE SUCTION UNIT (SEE 30.9.3) SHALL BE PROVIDED IN THE RECESSED AREA ON THE TOP OF THE REAR FLAT SURFACE. TO FACILITATE INSPECTION, REPAIR, AND REPLACEMENT, THE OXYGEN OUTLETS AND ELECTRICAL RECEPTACLE SHALL BE MOUNTED ON REMOVABLE PANELS.

30.8.9.6 STREETSIDE CABINET SECTION 3. THE THIRD SECTION SHALL CONSIST OF A COMPARTMENT TO THE REAR OF THE WHEEL WELL TO ACCOMMODATE STORAGE OF THE SPARE WHEEL ASSEMBLY AND TOOLS. IF TOOLS ARE STORED WITH THE SPARE WHEEL ASSEMBLY, DEVICES TO PREVENT RATTLING SHALL BE FURNISHED. THIS COMPARTMENT SHALL BE COVERED WITH A SOLID PANEL WHICH CAN BE REMOVED VERTICALLY OR A SOLID PANEL DOOR HINGED FORWARD TO PERMIT EASY ACCESS TO THE SPARE WHEEL ASSEMBLY AND TOOLS WITHOUT MOVING THE PATIENT COT. A SLIDING DOOR CABINET 8 TO 12 INCHES HIGH SHALL BE INSTALLED OVER THE SPARE WHEEL COMPARTMENT EXTENDING FROM THE RECESSED AREA TO THE BACK DOOR. TWO MORE CABINETS OF EQUAL HEIGHT SHALL BE INSTALLED HORIZONTALLY FROM THE RECESSED AREA TO THE FORWARD WALL OF THE SPARE WHEEL STORAGE. THE BOTTOM OF THE LOWER CABINET IS TO BE 18 INCHES FROM THE FLOOR OVER THE WHEELWELL. BOTH CABINETS SHALL HAVE SLIDING DOORS. THE DESIGN OF THESE CABINETS SHALL BE COMPATIBLE WITH THE VEHICLE CONFIGURATION.

30.8.9.7 EMERGENCY OXYGEN SUPPLY HOLDER. A FLOOR-MOUNTED TYPE DUAL-OXYGEN BOTTLE BASE, FERNO WASHINGTON MODEL 516 OR EQUAL, SHALL BE MOUNTED IN THE SIDE LOADING DOOR STEPWELL. THE UNIT SHALL BE MOUNTED AS FAR FORWARD AS POSSIBLE WITHOUT INTERFERING WITH THE SIDE DOOR MECHANISM.

30.8.9.8 IRRIGATOR HOOK, (I V). TWO DYNA MED INC. MODEL 1063-CA, OR EQUIVALENT CEILING ATTACHMENT HOLDERS SHALL BE INSTALLED FOR SUSPENDING INTRAVENOUS SOLUTION CONTAINERS. THE HOLDERS SHALL BE INSTALLED 36 INCHES TO 48 INCHES FROM THE PARTITION AT THE REAR OF THE DRIVER'S COMPARTMENT AND EIGHT INCHES ± ONE INCH FROM THE VEHICLE LONGITUDINAL CENTERLINE ON BOTH SIDES. THE HOLDERS SHALL BE CIRCULAR AND FITTED WITH A SPRING SNAP CLOSURE TO PROVIDE POSITIVE BOTTLE RETENTION WHEN THE VEHICLE IS IN MOTION.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

30.8.10 ATTENDANT STRAP HANGERS OR GRAB RAIL (PLAN AA AND AN).

30.8.10.1 STRAP HANGERS (PLAN AN). FOUR REMOVABLE STRAP HANGERS FOR ATTENDANT SUPPORT SHALL BE PROVIDED IN THE CEILING. GRAB RAILS NOT REQUIRED.

30.8.10.2 GRAB RAIL (PLAN AA). AN OVERHEAD GRAB RAIL SHALL BE PROVIDED. THE RAIL SHALL HAVE NOT LESS THAN A ONE-INCH OUTSIDE DIAMETER, STAINLESS STEEL TUBING, WITH A TWO-INCH CLEARANCE BETWEEN THE TOP OF THE RAIL AND THE CEILING. THE RAIL SHALL BE APPROXIMATELY SIX FEET LONG, CENTERED LONGITUDINALLY OVER THE COT WHEN IT IS IN PLACE ON THE STREET SIDE OF THE VEHICLE. THE RAIL SHALL BE POSITIONED (LATERALLY) ON THE VEHICLE CENTER LINE. THE ENDS OF THE GRAB RAIL SHALL BE CURVED UPWARD, TOWARD THE CEILING. THE ASSEMBLY SHALL BE BRADLEY GRAB BAR 857-002-72-2, OR EQUIVALENT.

30.9 OXYGEN AND SUCTION SYSTEMS AND EQUIPMENT.

30.9.1 OXYGEN SYSTEM (PLAN AA AND AN). UNLESS OTHERWISE SPECIFIED, THE OXYGEN SYSTEM SHALL CONFORM TO 3.12.1 AND 3.12.1.1, AND CONSIST OF ONE "H" SIZE OXYGEN CYLINDER, PRESSURE REDUCTION VALVE, FLOW METER, PRESSURE GAGE, HUMIDIFIER, TWO WALL OUTLETS AND NECESSARY HIGH PRESSURE OXYGEN HOSE, AND ACCESSORIES FOR A PIPED OXYGEN SYSTEM. THE VEHICLE USER WILL FURNISH AND INSTALL THE OXYGEN CYLINDER AT THE TIME THE VEHICLE IS PLACED IN SERVICE. THE OXYGEN CYLINDER WILL BE LOCATED IN THE STORAGE COMPARTMENT AS SPECIFIED IN 30.8.9.2 AND 30.8.8.2. SUFFICIENT CLEARANCE SHALL BE PROVIDED BETWEEN THE OXYGEN STATION AND THE VACUUM OUTLET TO PERMIT REMOVAL AND INSTALLATION OF THE FLOW METER AND OTHER DEVICES. THE OXYGEN HOSE FURNISHED SHALL BE TEFLON, WIRE BRAIDED TYPE. THE H OXYGEN TANK SHALL CONFORM TO DOT SPECIFICATION 3AA2015: OUTSIDE DIAMETER 9 INCHES (1/2 - 0); OVERALL HEIGHT W/VALVE 55 INCHES; CAPACITY 221 CUBIC FEET; WEIGHT EMPTY 135 POUNDS AND WEIGHT FULL 145 POUNDS.

30.9.1.1 OXYGEN STATION (PLUG-IN CONNECTIONS), PLAN AA AND AN. PLUG-IN CONNECTIONS SHALL BE FURNISHED FOR THE OXYGEN OUTLET STATION. THE OXYGEN OUTLET SHALL BE A DOUBLE OUTLET, CHEMETRON 400 SERIES PART EQUIVALENT TO 376 SERIES, PART NO. 700100-64 (OXYGEN-BLANK-BLANK-OXYGEN) OR EQUAL, WITH BOTTOM INLET. THE OXYGEN OUTLET SHALL BE MOUNTED IN THE STREETSIDE CABINET AS SHOWN IN APPENDIX FIGURES. THE OXYGEN OUTLET SHALL BE EQUIPPED WITH FLOWMETER/REGULATOR, OXYGEN 15 LITERS PER MINUTE (LPM) WITH QUICK DISCONNECT ADAPTER INLET CHEMETRON PART NO. 34-01-0003 OR EQUAL, AND A HUMIDIFIER BUBBLER TYPE WITH PLASTIC BOTTLE CHEMETRON PART NO. 34-10-0001 OR EQUAL. THE SECOND OUTLET SHALL BE USED FOR OTHER DEVICES AND A MATING OUTLET FITTING SHALL BE PROVIDED.

30.9.2 SUCTION ASPIRATOR, PRIMARY SYSTEM (PLAN AA). THE REQUIREMENTS OF 3.12.3 APPLY, EXCEPT AS MODIFIED BELOW.

30.9.2.1 PLUG-IN OUTLET FOR ASPIRATION SYSTEM FOR PLAN AA. THE VACUUM OUTLET OF 3.12.3 SHALL BE A CHEMETRON 400 SERIES PART NO. 64-50-0009 OR EQUAL, SINGLE PLUG-IN, SELF-SEALING VALVE CONNECTION WITH A BOTTOM INLET. THE PLUG-IN UNIT SHALL PREVENT THE ENTRY OF DUST WITHOUT THE USE OF A DUST CAP OR COVER AND ALLOW THE ATTACHMENT AND RELEASE OF SECONDARY EQUIPMENT WITH ONE HAND. THE FOLLOWING ITEMS SHALL BE FURNISHED: ONE EACH REGULATOR WITH FULL LINE CAPABILITY, CHEMETRON PART NO. 22-01-0012 OR EQUAL; ADAPTER, DISS MALE TO SERRATED STEM FOR HOSE, CHEMETRON PART NO. 15-90-0002 OR EQUAL; HOSE, PLASTIC, VACUUM, 18 INCHES IN LENGTH, CHEMETRON PART NO. 15-21-0001 OR EQUAL; TWO EACH COLLECTION BOTTLE ASSEMBLIES, CHEMETRON PART NO. 22-10-0002 INCLUDING ADAPTER HOSE TO DISS FEMALE, CHEMETRON PART NO. 22-93-0005, OR EQUAL; BOTTLE HOLDER WITH LOCK, CHEMETRON PART NO. 22-11-0007 OR EQUAL; BRACKET (FOR WALL MOUNT TO ACCEPT BOTTLE HOLDER), CHEMETRON PART NO. 22-11-0006 OR EQUAL. OUTLET AND BRACKETS SHALL BE MOUNTED AS SHOWN IN APPENDIX FIGURE 7.

30.9.3 PORTABLE SUCTION ASPIRATOR (VACUUM SYSTEM, PLAN AA AND AN). A PORTABLE BATTERY POWERED UNIT LAERDAL CATALOG NO. 79 00 00, COMPLYING TO 3.12.4 PERFORMANCE SHALL BE FURNISHED TO INCLUDE:

(A) A POWER PACK COMPLETE WITH BATTERY CHARGER RECHARGEABLE BATTERIES.

(B) WIRED TO VEHICLE 12 VDC SYSTEM (3.7.7.3) AND INSTALLED IN APPLICABLE CABINETS AS SPECIFIED. THE PLUG AND RECEPTACLE SHALL BE OF THE COMMERCIAL QUICK-DISCONNECT (NOT SCREW-IN) TYPE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

30.10 Environmental: Climatic and Noise Parameters.

30.10.1 Environmental Systems (3.13). Heating, air conditioning, ventilation and sound level requirements shall comply to section 3.13.

30.11 Communications.

30.11.1 Communications Equipment (3.14). Unless otherwise specified (see 60.2) shall comply to section 3.14. The amplifier and its controls shall be mounted on the driver's compartment ceiling, centered between the driver and the assistant with controls accessible to both.

30.11.2 Siren speaker location and mounting (Plan AA and AN). An external speaker, designed for roof mounting, with a weatherproof driver shall be installed on the centerline of the cab roof in a location that will not obstruct light from or movement of the roof mounted spotlight or rotating warning light. The speaker shall be metal with a chrome finish, aluminum, or fiberglass painted to match the vehicle exterior color. A gasket of not less than 1/16 inch thick shall be furnished between the speaker mounting bracket and the vehicle roof to minimize drumming. When necessary to prevent deflection and drumming, reinforcements shall be provided on the vehicle at the point of attachment of the speaker. The speaker location shall permit servicing of the vehicle without removing the speaker.

30.12 Additional Systems, Equipment, Accessories and Supplies.

30.12.1 Additional and Optional Equipment (3.15). Shall be furnished as specified in section 3.15, and as selected by the purchasing agency (see 60.2).

30.13 Preparation for Painting, Color and Markings.

30.13.1 Preparation for Painting, Color, and Markings (3.16). As specified by the procuring activity for the appropriate service (see 60.2) treatment and painting shall be in accordance with the specification. The exterior color of the vehicle shall be nearest gloss white, matching color chip No. 17886 of Fed. Std. No. 595. The grill and mirrors shall be furnished in bright finish metal as OEM standard or option. Unless otherwise specified (see 60.2) ambulance markings and data plates shall be in accordance with MIL-STD-1223, and 3.19.

40. QUALITY ASSURANCE

40.1 Quality Assurance Provisions, Tests, and Certifications. Except as specified in 30.1, quality assurance provisions shall comply to section 4 of the specification.

50. PREPARATION FOR DELIVERY

50.1 Preparation. Unless otherwise specified, preparation for delivery shall comply to 5.1.

Source: https://assist.dla.mil -- Downloaded: 202610-26T12:46Z
Check the source to verify that this is the current version before use.

60. NOTES

60.1 Intended Use of Appendix. The intended use of this appendix is to procure a standardized certified "Star of Life" ambulance for military services use. Military agencies desiring an ambulance (type II M) must use the "Ordering Data," 60.2 following. (Use the ordering data 6.2 of the specification for other types of ambulances.) All purchasers should read the entire document (including any amendments) before requisitioning an ambulance, to be aware of just what equipment and requirements are standard and which options need to be excised.

60.2 Ordering Data. Procurement document should specify the following:

(a) Title, number, and date of this specification, appendix, and amendment number if any.

(b) Type, class, and floor plan of ambulance required (see 10.2) identify appropriate service.

(c) Engine, (V8 gasoline is standard) specify if 6 cylinder or OEM diesel engine is desired (see 30.3).

(d) Power plant heaters (engine/battery) in lieu of 3.15.3-15) state if required (see 30.3.2).

(e) Air pollution controls, cite where ambulance will operate, county and state, or if it is for export, name country (see 3.6.4.3 and 3.22.1 and 3.22.2).

(f) Drive train and transmission (automatic and special traction rear-end is standard) if class 2 (4x4) specify requirements; if other than that specified (3.6.5 through 3.6.5.9), check chassis manufacturer's data.

(g) Wheels and tires, highway tread is standard for all classes of ambulances. Mud and snow or all purpose type tires should be specified if 4x4 vehicle. Specify radial tires if desired (see 3.6.8 to 3.6.9).

(h) Spare tire assembly, specify if not required (see 3.6.10).

(i) Electrical wiring and generating systems, suppliers are required to provide necessary generating capacity (see 30.4). If additional capacity is desired for purchaser's installed electrical devices, specify the minimum reserve amperes needed (see 3.7 to 3.7.12).

(j) Warning and exterior lighting, red and clear warning lights are Federal standard, specify other color(s) only if export vehicle, or required by state or local regulations. Specify if strobe type lights are desired (see 30.5 to 30.5.7.1, and 3.8 to 3.8.4).

(k) Removal of exterior lights for shipment, if required (see 30.5.4).

(l) Storage compartments and facilitations, cite any changes (see 30.8 to 30.8.9.8) cite paragraph which is being modified.

(m) Stretchers, cots, and litters, specify any cots needed (see 30.8.3, table II and 3.11.5 to 3.11.7).

(n) Oxygen system and equipment, cite any changes necessary (see 30.9 to 30.9.1.1, and 3.12 to 3.12.1.1).

(o) Suction aspirator system, for plan AA select engine vacuum and/or electrically powered type (see 30.9.2 to 30.9.3 and 3.12.3 to 3.12.4).

(p) Painting, color, and marking, (see 30.13.1) specify any changes.

(q) Rustproofing, if required (see 3.18).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

(R) SPECIAL REQUIREMENTS, STATE ANY OTHER ADDITIONS, CHANGES, OR DELETIONS TO THE SPECIFICATION (SEE 3.22).

(S) OVERSEAS VEHICLE REQUIREMENTS, SELECT (A) THROUGH (D) (SEE 3.22.1 THROUGH 3.22.3.1), INCLUDE TIEDOWN POINT AND LIFTPOINT REQUIREMENTS ONLY IF ABSOLUTELY NECESSARY.

(T) QUALITY ASSURANCE PROVISIONS, SPECIFY CLASSIFICATION OF INSPECTION DESIRED (SEE 4 THROUGH 4.2.7 AND 40).


1. SOURCE INSPECTION (SEE 4.2.1) OR

2. DESTINATION EXAMINATION (SEE 4.2.2).

(U) FIRST PRODUCTION AMBULANCE INSPECTION, STATE IF REQUIRED (SEE 4.2.5).


(V) PROCUREMENT REQUIREMENTS, (SEE 6.3) SPECIFY OTHER PURCHASER'S CONTRACTUAL REQUIREMENTS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

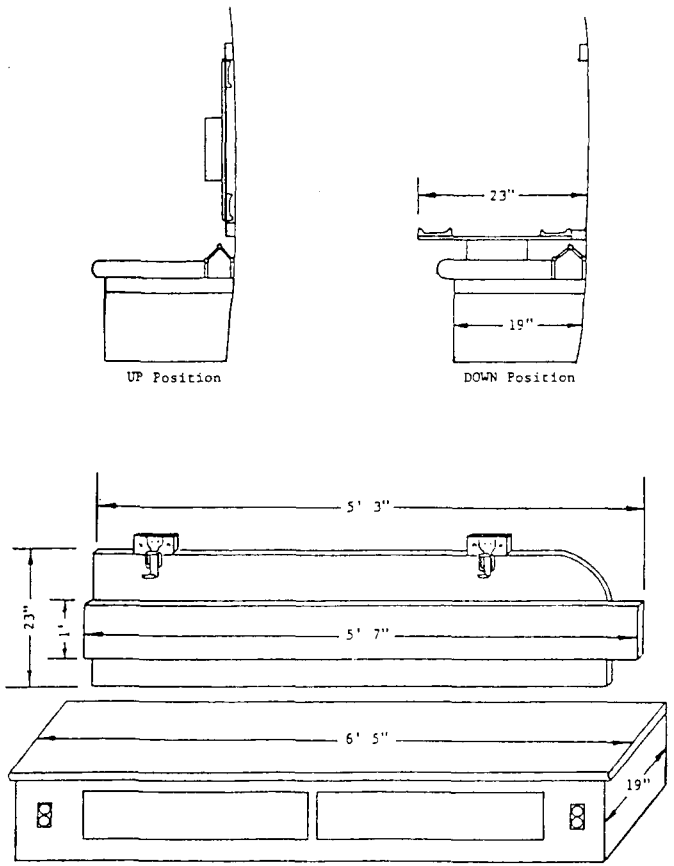


NOTE: Unless otherwise specified herein, all dimensions are approximate.

APPENDIX FIGURE 1 COMBINATION BACKREST/LITTER SUPPORT PANEL - PLAN AA

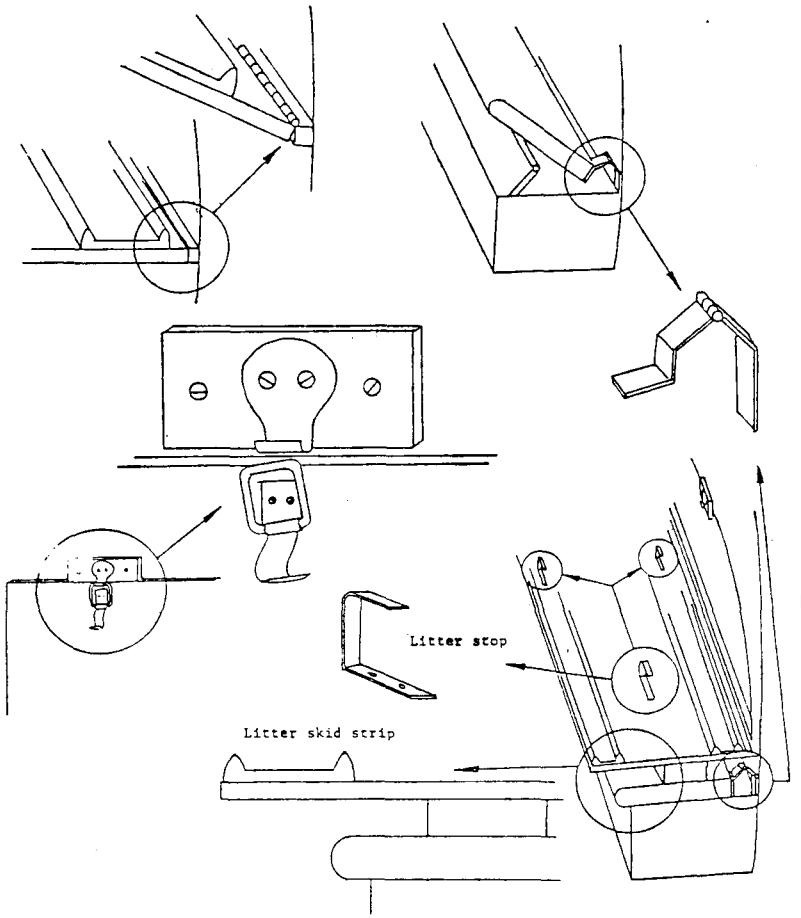


APPENDIX FIGURE 2 DETAIL COMBINATION BACKREST/LITTER SUPPORT PANEL - PLAN AA


Source: https://assist.dla.mil -- Downloaded: 2026-10-26T12:46Z
Check the source to verify that this is the current version before use.

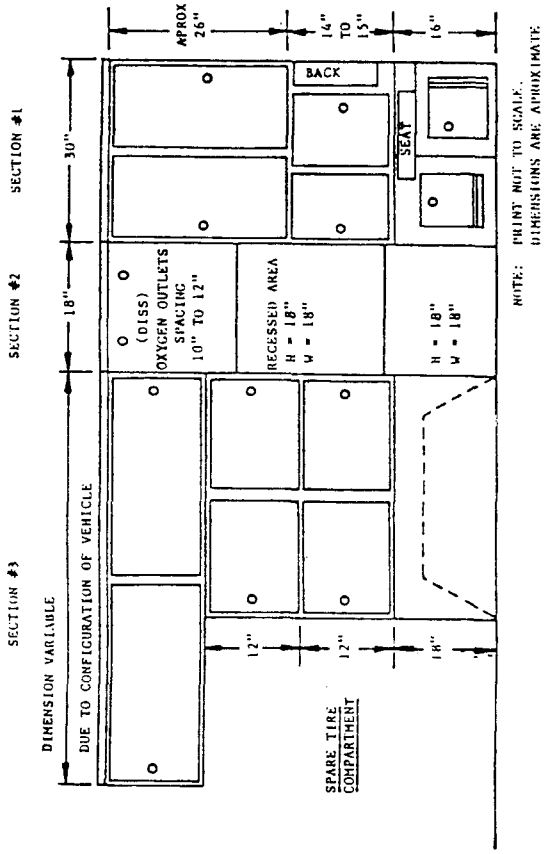

APPENDIX FIGURE 3 STREETSIDE CABINETRY - PLAN AN

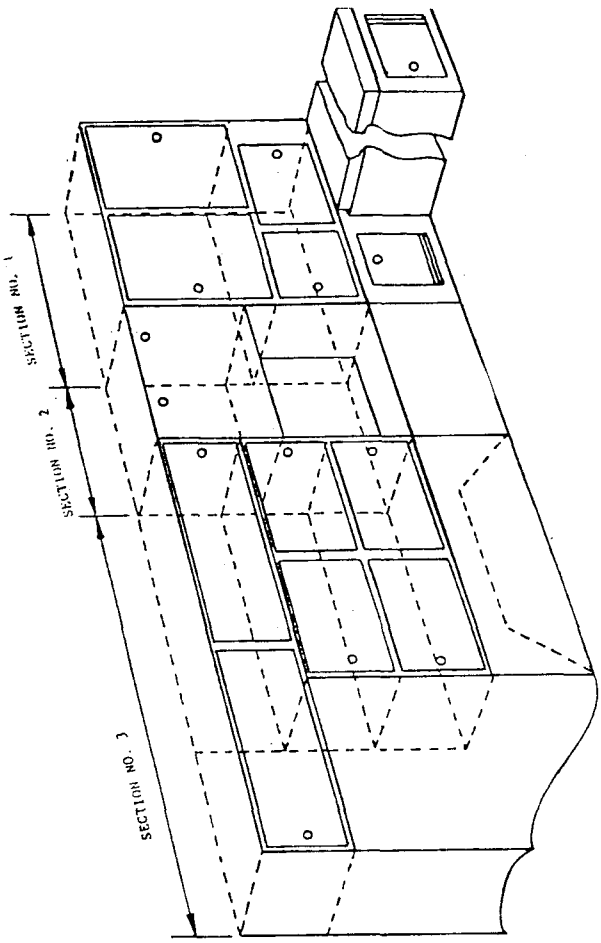


APPENDIX FIGURE 4 STREETSIDE CABINETRY - PLAN AN

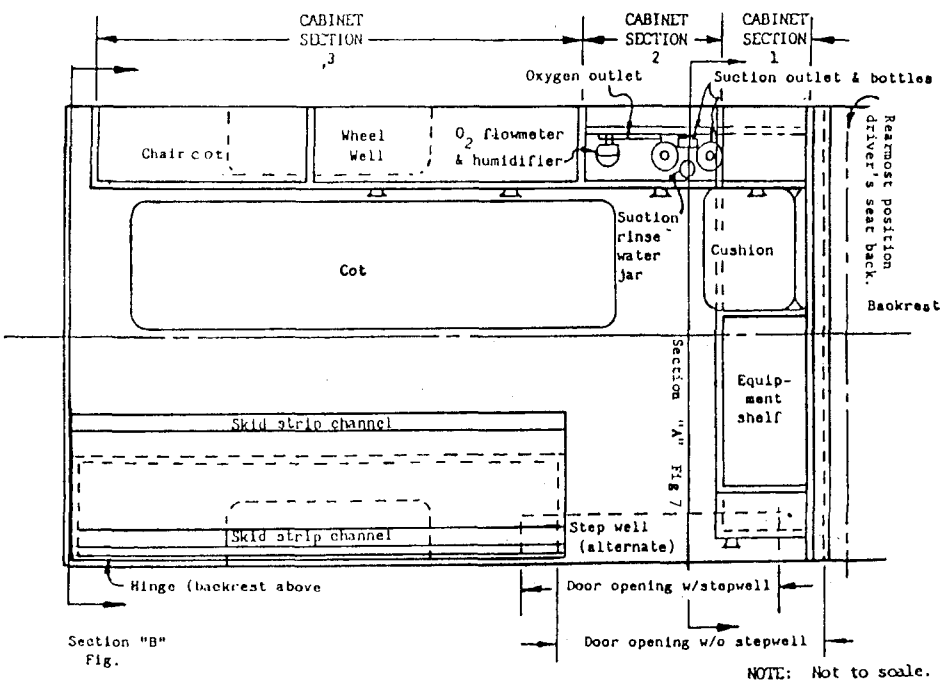


APPENDIX FIGURE 5 PLAN VIEW - PATIENTS' COMPARTMENT - PLAN AA

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:46Z
Check the source to verify that this is the current version before use.

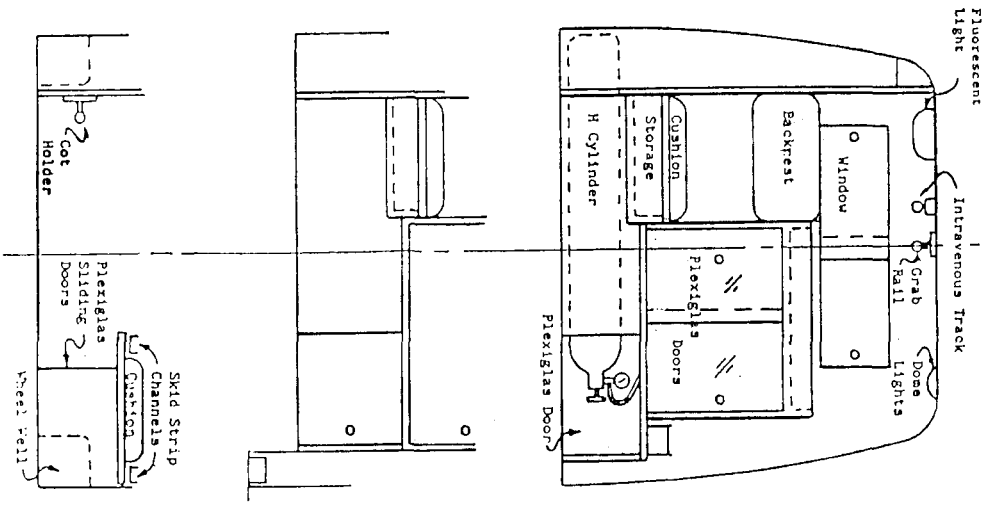

NOTE: Not to scale.

APPENDIX FIGURE 6 SECTIONAL VIEWS - PATIENTS' COMPARTMENT - PLAN AA

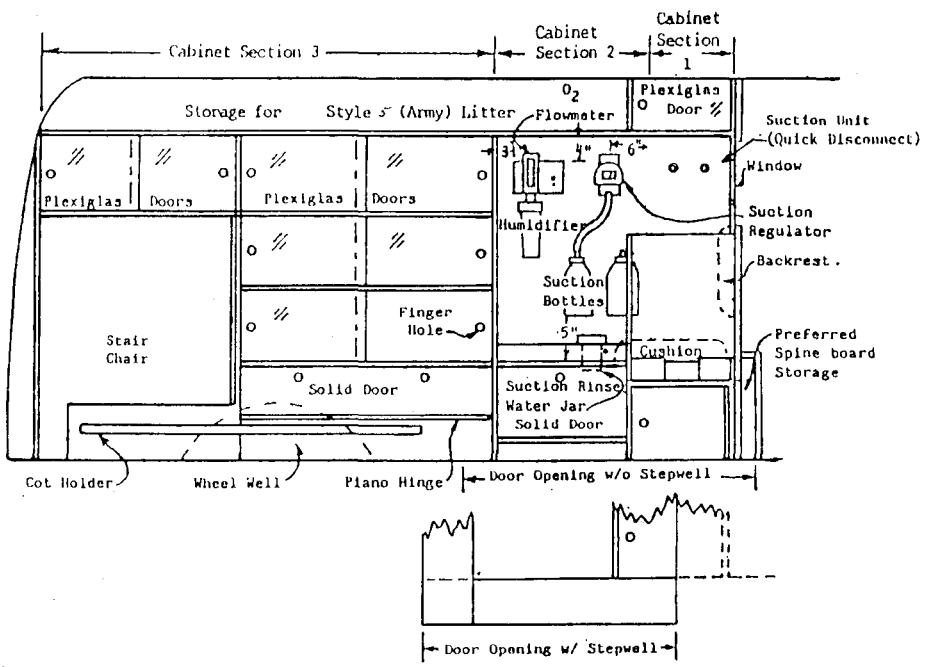

NOTE: Not to scale.

APPENDIX FIGURE 7 STREETSIDE CABINETRY AND EQUIPMENT - PLAN AA

Source: https://assistdata.mil - Downloaded: 2026-04-26T12:46Z
Check the source to verify that this is the current version before use.

GENERAL SERVICES ADMINISTRATION - FEDERAL SUPPLY SERVICE

SPECIFICATION COMMENT SHEET

BUDGET BUREAU NO. 29-R0175

INSTRUCTIONS

This form provides a way for users of this specification to inform the originator of problems encountered in its use. It is not to be used to request changes to accommodate proprietary features. All comments will be considered and appreciated, but please do not expect a reply. To comment: detach, complete, fold, staple, and mail. to GSA-FSS-FAE, CMBg. #4, Rm. 420, Wash., DC 20406.

NOTE: Comments on this form do not constitute or imply authorization to waive any part of the document or serve to amend contractual requirements.

1. SPECIFICATION

KKK-A-1822A

AMBULANCE
Emergency Medical Care Surface Vehicle

2. CONTRACT NO. *(If any)*	3. QUANTITY ON CONTRACT *(Optional)*	4. DOLLAR VALUE *(Optional)*

5. GENERAL NATURE OF PROBLEM *(e.g., inspection difficulties, manufacturers unable to meet tolerances, containers collapse under normal warehousing conditions, etc.)*

6. SPECIFIC REQUIREMENTS AFFECTED *(Include paragraph number and lines of wording)*

7. SPECIFIC PROBLEMS *(e.g. tests in 4.2.2 will not assure that the battery will last required time; temperature ranges in table 2 do not conform to commercially available items.)*

8. RECOMMENDATIONS

9. NAME OF MANUFACTURER, ASSOCIATION, GOVT., AGENCY, ETC.	10. ADDRESS *(Number, Street, City, State and Zip Code)*

11. NAME AND TITLE OF SUBMITTER	12. DATE

GSA DC 69-9761

FORM GSA FEB 69 2200

Source: https://assist.dla.mil -- Downloaded: 202640-26T12:46Z
Check the source to verify that this is the current version before use.