MILITARY SPECIFICATION

FORCEPS, DRESSING, STRAIGHT, CUSHING, 7 INCH

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a dressing forceps of the Cushing design, suitable for use in surgical procedures of the brain.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Set-up.

Military

MIL-P-116	Preservation, Methods of
MIL-L-10547	Liners, Case and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions shall be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The dressing forceps shall be in accordance with the applicable requirements of GG-I-526, and as specified herein.

3.2 Material. The forceps shall be fabricated from class 4, type 410 or 420 material.

3.3 Hardness. After proper stress relieving, Rockwell hardness shall be C40 to C45.

3.4 Style, design and dimensions. Shall be a straight dressing forceps, of the Cushing design, suitable for lifting tissues in deep cavity procedures during brain surgery. Forceps shall be of slender design with serrated tips. Serrations shall be of consistent depth and well defined. Forceps shall be in accordance with Figure 1.

3.5 Finish. Finish shall be mirror.

3.5.1 Passivation. The forceps shall be properly passivated.


3.6 Identification marking. In addition to the requirements specified in GG-I-526, forceps of foreign manufacture shall be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

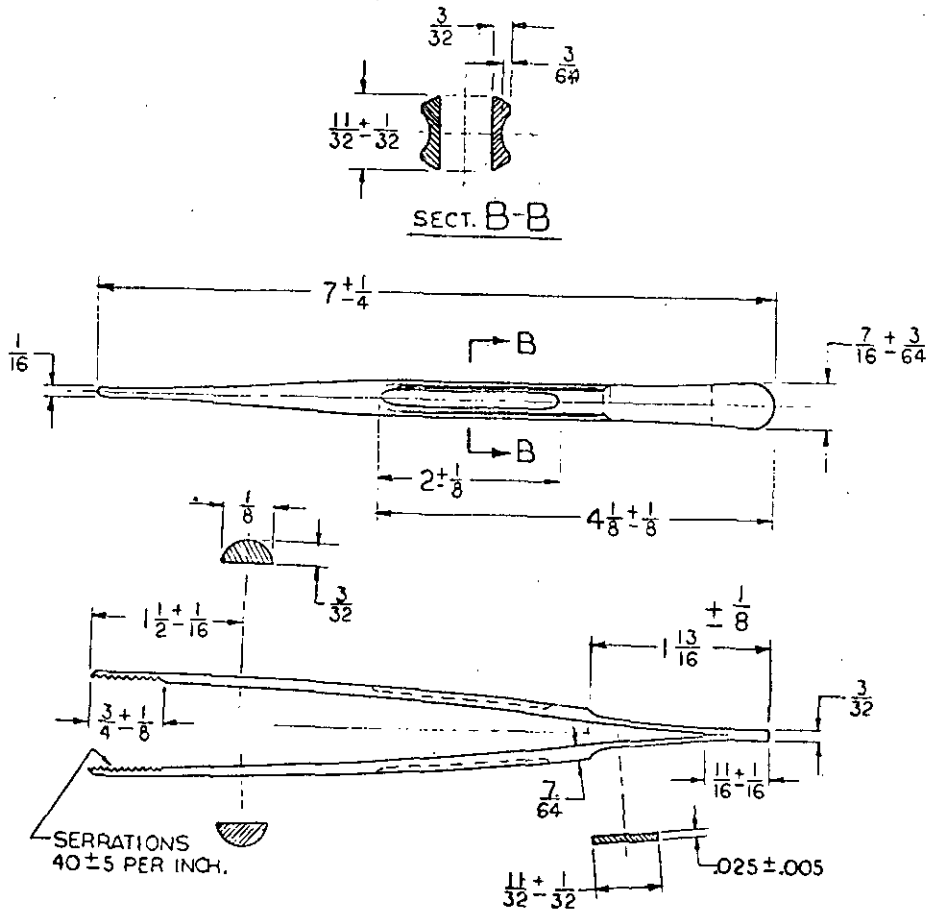

NSN 6515-00-333-3100

NOTE

TOLERANCES INDICATED DELINEATE ACCEPTABLE EXTREME DIMENSIONS, AND ARE NOT INTENDED TO PERMIT VARIATIONS WITHIN A SINGLE INSTRUMENT WHICH WILL SACRIFICE UNIFORMITY, SYMMETRY AND FIRST QUALITY WORKMANSHIP.

ALL DIMENSIONS IN INCHES
UNLESS OTHERWISE SPECIFIED
TOLERANCES SHALL BE ± 1/64

MIL-E-3709

FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the corrosion-resistant steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in Table I. The unit of product for examination purposes shall be one forceps.

Table I. Sampling Criteria for Examination

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics. The unit of product for test purposes shall be one forceps.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL
Forceps	Hardness test	3.3 & GG-I-526	GG-I-526	S-2	1.5
	Dimensions	3.4	--------	S-2	2.5
	Copper sulfate test	GG-I-526	GG-I-526	S-2	1.0
	Boil test	GG-I-526	GG-I-526	S-2	1.0

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

4.3 Examination. The forceps shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to defects listed in Table III. Any forceps in the sample containing one or more defects shall be rejected and if the number of defective forceps in any sample exceeds the acceptance number for the sample, the lot represented by that sample shall be rejected.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Forceps not of the specified design.
102	Serrations not of uniform depth and not well defined.
103	Forceps not free from cracks, pits, burrs, sharp edges, rough areas and tool marks.
104	Finish of forceps not uniform.
Minor	
201	Forceps not identified as specified in 3.6.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.5 Examination of preparation for delivery. An examination shall be made to determine whether the packaging, packing and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 2.5 expressed in terms of defects per hundred units.

Table IV. Examination of Preparation for Delivery

Examine	Defect
Containers	Not as specified.
Contents	Not as specified.
Markings	Omitted; incorrect; illegible; improper size, location, sequence, or method of application.
Materials	Component missing or damaged.
Workmanship	Bulging or distortion of containers.
	Cushioning inadequate, improper or missing.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

4.5.1 Examination of closure and reinforcement for containers. When shipping containers are required to comply with PPP-B-636, examination for defects in closure and reinforcement shall be in accordance with the appendix to that specification.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A, or C, as specified (see 6.1).

5.1.1 Unit of issue. Each forceps as specified constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Unit package. Each forceps shall be cleaned and dried in accordance with the applicable method specified in MIL-P-116. The forceps shall be wrapped in neutral tissue or other suitable anticorrosive material and packaged in accordance with MIL-P-116, method IC-1 except that a preservative shall not be utilized.

5.1.2.2 Intermediate package. Six unit packages shall be packed in a snug fitting box constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure of the box shall be secured to prevent spilling of contents under normal handling.

5.1.3 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.1).

5.2.1 Level A. Forty eight intermediate packages (288 units) shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification. Special requirements as specified in PPP-B-636 shall apply for fiberboard boxes.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraph of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed in accordance with 30.4 of PPP-B-636.

5.2.2 Level B. Forty eight intermediate packaged (288 units) shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636. Special requirements as specified in PPP-B-636 shall apply for fiberboard boxes.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.2.4 Packing variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable box is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification covers NSN 6515-00-333-3100 FORCEPS, DRESSING, Straight, Cushing 7 inch listed in the Federal Supply Catalog.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

6.3 Supersession data. This specification includes includes requirements of Purchase Description No. 2, dated 1 April 1967, for FSN 6515-333-3100 FORCEPS,DRESSING, Straight, Cushing, 7 inch.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Review activities:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1891

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-F-37109

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:59Z
Check the source to verify that this is the current version before use.