MIL-R-37103B
20 December 1985
SUPERSEDING
MIL-R-37103A(DLA-DM)
28 April 1977

MILITARY SPECIFICATION

RETRACTOR, HEMILAMINECTOMY, HAVERFIELD-SCOVILLE AND BLADES, RETRACTOR, INTERCHANGEABLE

This specification is approved for use by Defense Logistics Agency-DM, Department of Defense, and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a hemilaminectomy retractor body of the Haverfield-Scoville design and selected styles and sizes of interchangeable blades.

1.2 Classification.

1.2.1 Styles and sizes. The blades shall be of the following styles and sizes (see 6.2).

Style I - Scoville hook
Size 1 - Blunt hook, 2 inches deep
Size 2 - Blunt hook, 3 inches deep

Style II - Taylor laminectomy
Size 1 - Small, 3 prongs, 1-3/4 inches deep, 1-1/2 inches wide
Size 2 - Medium, 4 prongs, 1-7/8 inches deep, 2 inches wide
Size 3 - Large, 4 prongs, 2-1/2 inches deep, 2-1/4 inches wide

Beneficial comments (recommendations, additions, deletions) and any pertinent data which may be of use in improving this document should be addressed to: Headquarters, Defense Personnel Support Center, ATTN: Directorate of Medical Materiel, DPSC-ATT, 2800 South 20th Street, Philadelphia, PA 19101, by using the self-addressed Standardization Document Improvement Proposal (DD Form 1426) appearing at the end of this document or by letter.

FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

AMSC N/A

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

Style III - Scoville laminectomy
Size 1 - 4 prongs, 1-5/8 inches deep, 1-1/2 inches wide
Size 2 - 4 prongs, 2-5/8 inches deep, 1-3/4 inches wide

Style IV - Epstein hemilaminectomy, 2-1/4 inches deep, 1 inch wide

Style V - Hibbs
Size 1 - 2 inches deep, 1 inch wide
Size 2 - 2 inches deep, 2 inches wide
Size 3 - 3 inches deep, 1 inch wide
Size 4 - 3 inches deep, 2 inches wide
Size 5 - 4 inches deep, 2 inches wide

Style VI - Meyerding laminectomy
Size 1 - 2-1/4 inches deep, 1 inch wide
Size 2 - 3 inches deep, 1 inch wide
Size 3 - 3-1/2 inches deep, 2 inches wide

2. APPLICABLE DOCUMENTS

2.1 Issues of documents. The following documents of the issue in effect on date of invitation for bids or request for proposals form a part of this specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

GG-I-526 - Instruments, Dental and Surgical; General Specifications.
PPP-B-566 - Boxes, Folding, Paperboard.
PPP-B-601 - Boxes, Wood, Cleated-Plywood.
PPP-B-621 - Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636 - Boxes, Shipping, Fiberboard.

MILITARY

MIL-P-116 - Preservation-Packaging, Methods Of.
MIL-L-10547 - Liners, Case and Sheet, Overwrap, Water-Vaporproof, or Waterproof, Flexible.

STANDARDS

MILITARY

MIL-STD-105 - Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129 - Marking for Shipment and Storage.
MIL-STD-147 - Palletized Unit Loads.
MIL-STD-794 - Part and Equipment, Procedures for Packaging and Packing Of.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

(Copies of specifications, standards, and publications required by contractors in connection with specific procurement functions should be obtained from procuring activity or as directed by the contracting office.)

3.2 Other publications. The following documents form a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

American Society for Testing and Materials (ASTM) Standards

E 10 - Method of Test for Brinell Hardness of Metallic Materials.
E 18 - Rockwell Hardness and Rockwell Superficial Hardness of Metallic Materials.
E 92 - Method of Test for Vickers Hardness of Metallic Materials.

E 140 - Standard Hardness Conversion Tables for Metals (Relationship between Brinell Hardness, Vickers Hardness, Rockwell Hardness, Rockwell Superficial Hardness and Knoop Hardness).

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103).

American Iron and Steel Institute (AISI).

Steel Products Manual.

(Application for copies should be addressed to the American Iron and Steel Institute, 1000 16th Street, NW, Washington, DC 20036).

(Technical society and technical association specifications and standards are generally available for reference from libraries. They are also distributed among technical groups and using Federal agencies).

3. REQUIREMENTS

3.1 General requirements. The individual part requirements shall be as specified herein and in accordance with the applicable requirements of GG-I-526. In the event of any conflict between the requirements of GG-I-526 and those of this specification, the latter shall govern.

3.2 Materials. All metal parts shall be as specified herein and in accordance with the applicable requirements of GG-I-526. The component parts of the retractor body assembly shall be fabricated from corrosion resistant steel as specified in table I. Blades shall be fabricated from material specified in table II.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

TABLE I. Retractor body materials.

Component Part	Quantity	AISI Type	Hardness
Arms	2	416 or 410	Rc 35-40 Rc 38-43
Arm screws	2	410	Rc 38-43
Carriage	1	304	Rb 85 min
Carriage spring	1	304	Rb 85 min
Pawl	1	304	Rb 85 min
Pawl screws	1	304	Rb 85 min
Rack	1	17-4 PH or 410	Rc 38-43 Rc 38-43
Rack screws	1	304	Rb 85 min
Carriage screws	1	304	Rb 85 min
Thumb piece	1	304	Rb 85 min
Pinion gear	1	304 or 410	Rb 85 min Rc 38-43

TABLE II. Blade materials.

Blade Style	AISI Type	Thickness	Boss/Flange	AISI Type	Diameter	Hardness
I	304	1/4"	Flange	304	1/2"	Rb 85 min
II, III, IV, V, & VI	410	1/8"	Boss	410	1/2"	Rc 38-43
Wing Nut (1)	410	1/16"	Boss	410	1/2"	Rc 38-43
	304	-	-	-	-	Rb 85 min

3.3 Design and construction.

3.3.1 Retractor assembly and blades.

3.3.1.1 Retractor. The hemilaminectomy retractor body assembly shall be fabricated from the materials specified in 3.2, table I and shall be of the Haverfield-Scoville design with ratchet action and hinged arms. It shall be designed for use with selected, detachable blades specified in 3.3.1.2.

3.3.1.2 Blades. The laminectomy blades shall be fabricated from the materials specified in 3.2, table II for the appropriate style and size. The blades shall be of the design specified in 1.2.1 and shall be detachable. The blade attachment design shall permit easy assembly and disassembly with the retractor assembly.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

3.3.1.3 Physical dimensions. The physical dimensions of the retractor assembly shall be in accordance with figure 1. Figures 2 through 7 delineate the blade dimensions and configuration for the appropriate style and size.

3.3.1.4 Hardness. When tested as specified in 4.5.1, the component parts shall have a Rockwell hardness as specified in table I. Hardness of the finished blades shall be as specified in table II.

3.3.1.5 Corrosion resistance. When tested as specified in 4.5.2.1, the retractor body component parts and the blade including attachment device shall be corrosion resistant conforming to the requirements of GG-I-526. Parts fabricated from AISI Type 400 series material shall also be subjected to the test specified in 4.5.2.2.

3.4 Finish. The finished retractor assembly and detachable blades shall have a satin finish except for the carriage which shall be smooth. Carriage finish may be produced by sandblast.

3.4.1 Passivation. As a final finish operation, all parts shall be passivated.

3.5 Identification marking. Identification marking of finished instruments shall be in accordance with GG-I-526. In addition to the requirements specified, instruments of foreign manufacture shall also be marked "stainless".


3.6 Interchangeability and substitutability. Interchangeable parts having the same manufacturer's part number will be functionally and dimensionally interchangeable. Components parts except for blades need not be interchangeable between manufacturers and may not be interchangeable with different models produced by the same manufacturer. All blades regardless of source of manufacture shall be capable of being attached to any manufacturers retractor.

3.7 Workmanship. Workmanship shall be first class throughout. The instrument shall be processed in such a manner as to be uniform in quality and shall be free from surface roughness, burrs, pits, scale, corrosion, or any other defects that will affect life, serviceability or appearance.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspection set forth in the specification where such inspections are deemed necessary to assure supplied and services of the supplies to which such records relate.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

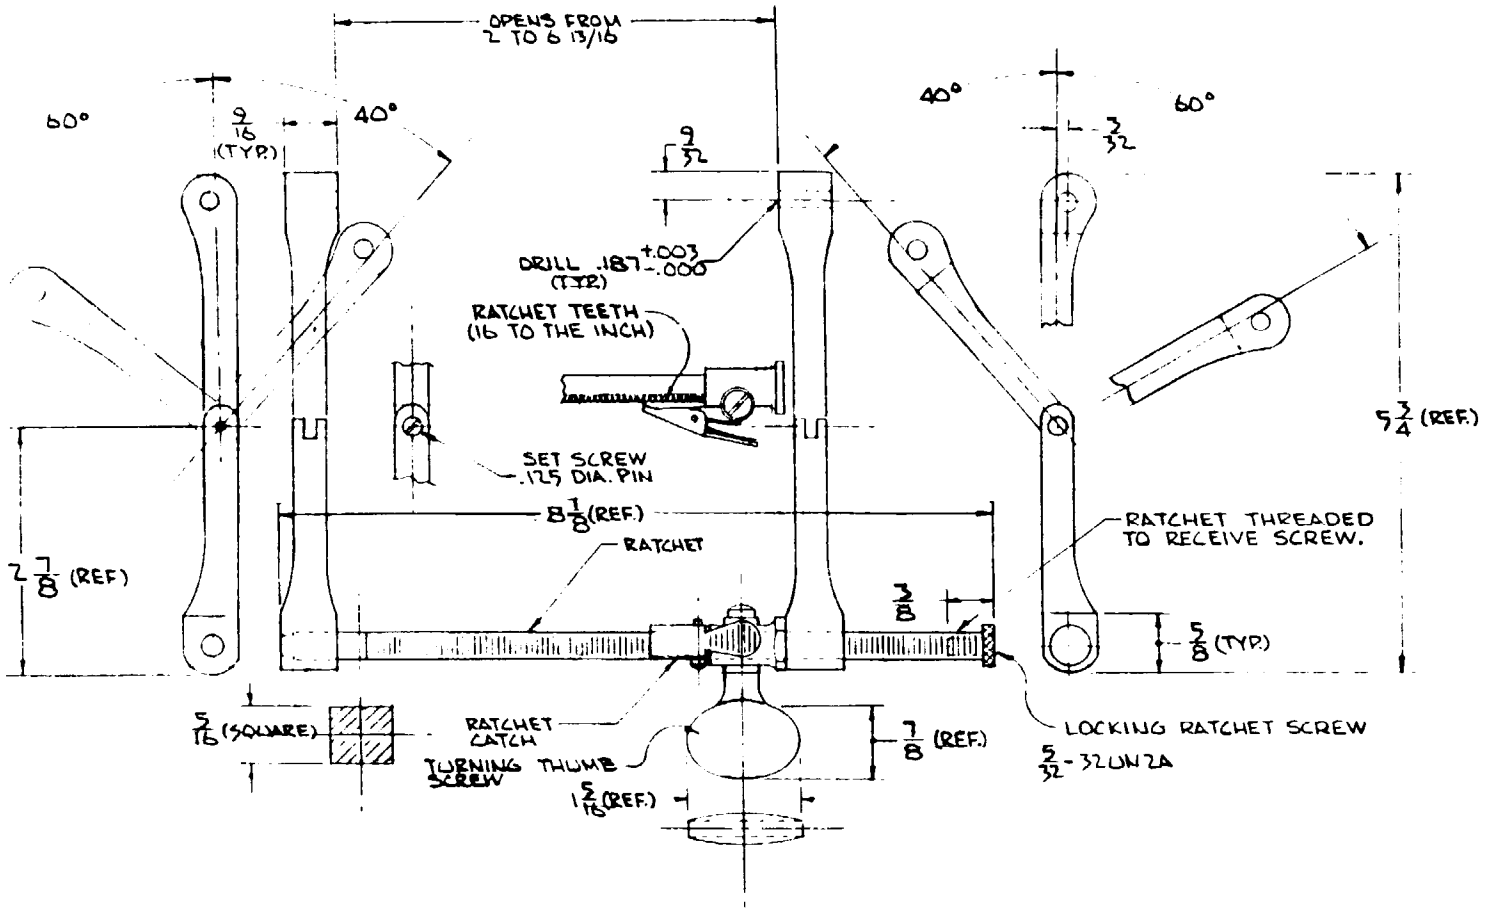

NSN 6515-00-385-3685


RETRACTOR, LAMINECTOMY, HAVERFIELD-SCOVILLE

FIGURE 1

TOLERANCE NOTES:
REMOVE BURRS AND BREAK ALL SHARP EDGES, UNLESS OTHERWISE SPECIFIED.
UNLESS OTHERWISE SPECIFIED, DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED, TOLERANCES ON
FRACTIONS ± 1/32
DECIMALS ± .03
ANGLES ± 3°


Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

MIL-S-27035

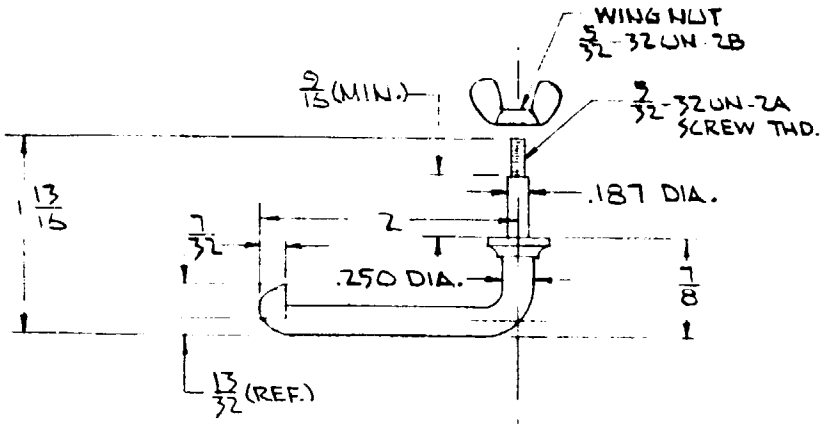

NSN 6515-00-392-0722

BLADE, LAMINECTOMY RETRACTOR, SCOVILLE, SINGLE HOOK, TYPE I, SIZE 1

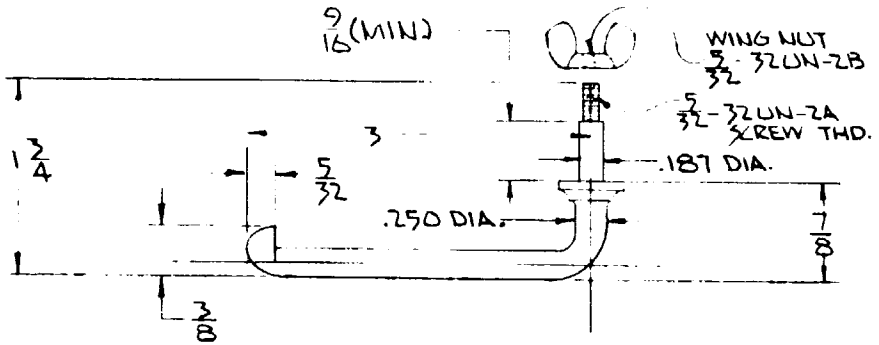


NSN 6515-00-392-0723

BLADE, LAMINECTOMY RETRACTOR, SCOVILLE, SINGLE HOOK, TYPE I, SIZE 2


FIGURE 2

TOLERANCE NOTES:
REMOVE BURRS AND BREAK ALL SHARP EDGES, UNLESS OTHERWISE SPECIFIED.
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES
UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 2°


Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

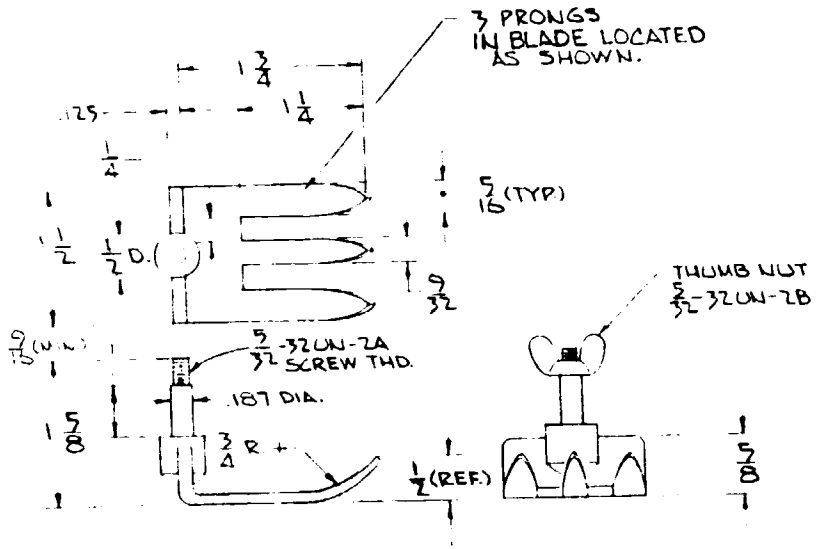

NSN 6515 00 379 4389
BLADE, LAMINECTOMY RETRACTOR, TAYLOR, TYPE II, SIZE 1

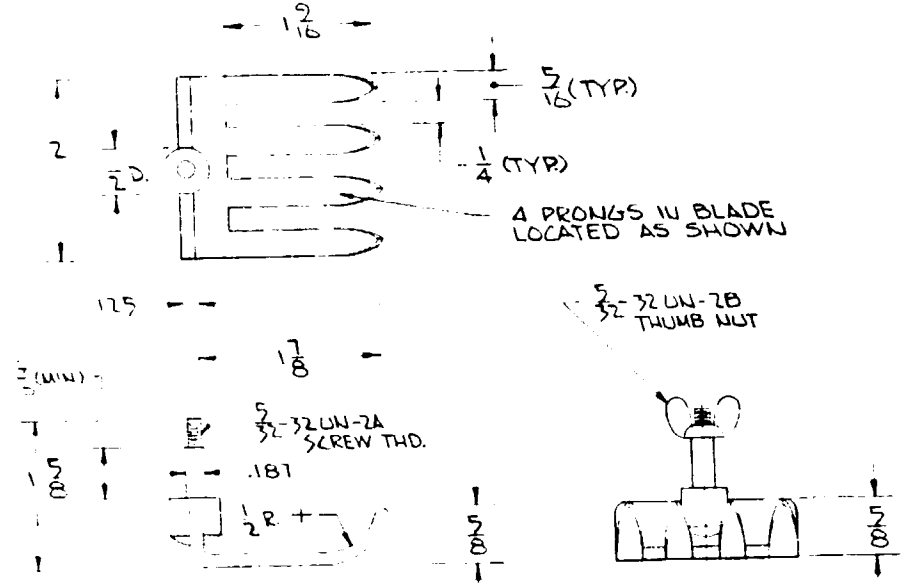

NSN 6515-00-376-7776
BLADE, LAMINECTOMY RETRACTOR, TAYLOR, TYPE II, SIZE 2

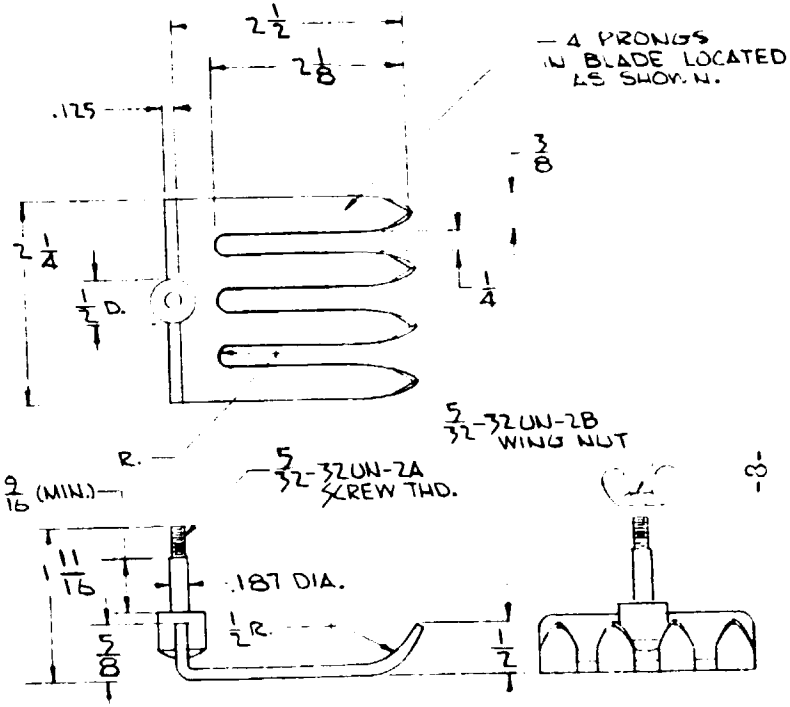


NSN 6515-00-376 7784
BLADE, LAMINECTOMY RETRACTOR, TAYLOR, TYPE II, SIZE 3

TOLERANCE NOTES:
REMOVE BURRS AND BREAK ALL SHARP EDGES UNLESS OTHERWISE SPECIFIED.
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 1°


FIGURE 3

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

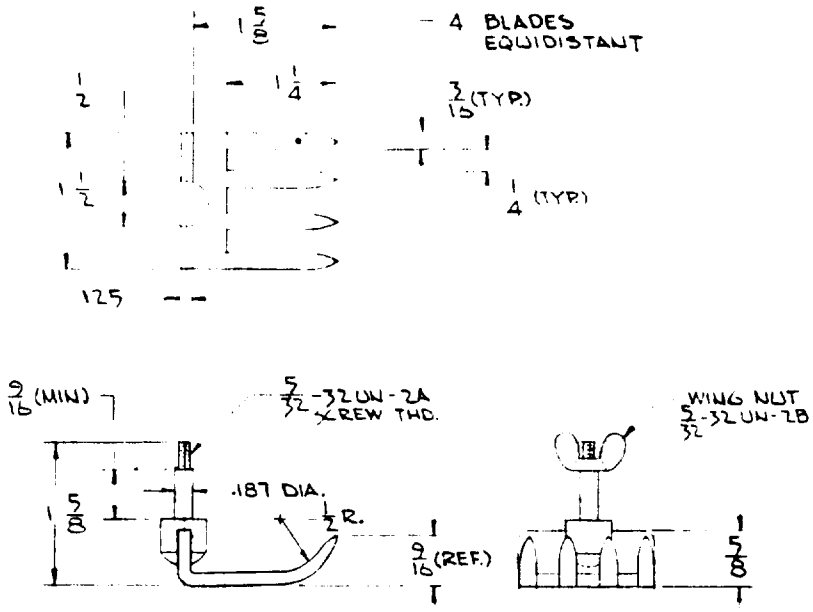

NSN 6515-00-376-7789

BLADE, LAMINECTOMY RETRACTOR, SCOVILLE, 4 PRONG, TYPE III, SIZE 1

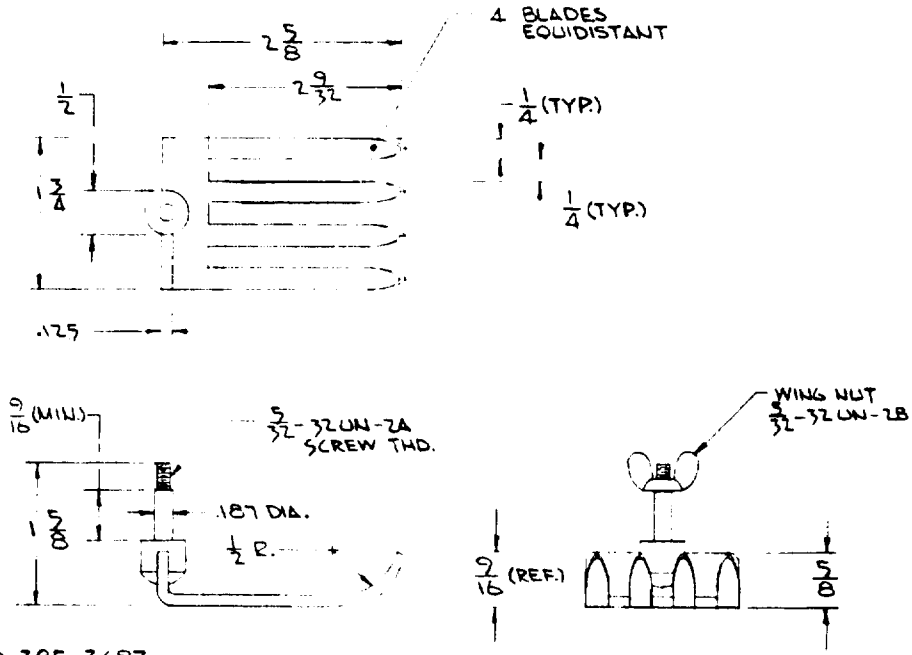


NSN 6515-00-385-3687

BLADE, LAMINECTOMY RETRACTOR, SCOVILLE, 4 PRONG, TYPE III, SIZE 2

FIGURE 4

TOLERANCE NOTES:
REMOVE BURRS AND BREAK ALL SHARP EDGES UNLESS OTHERWISE SPECIFIED.
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± ~

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

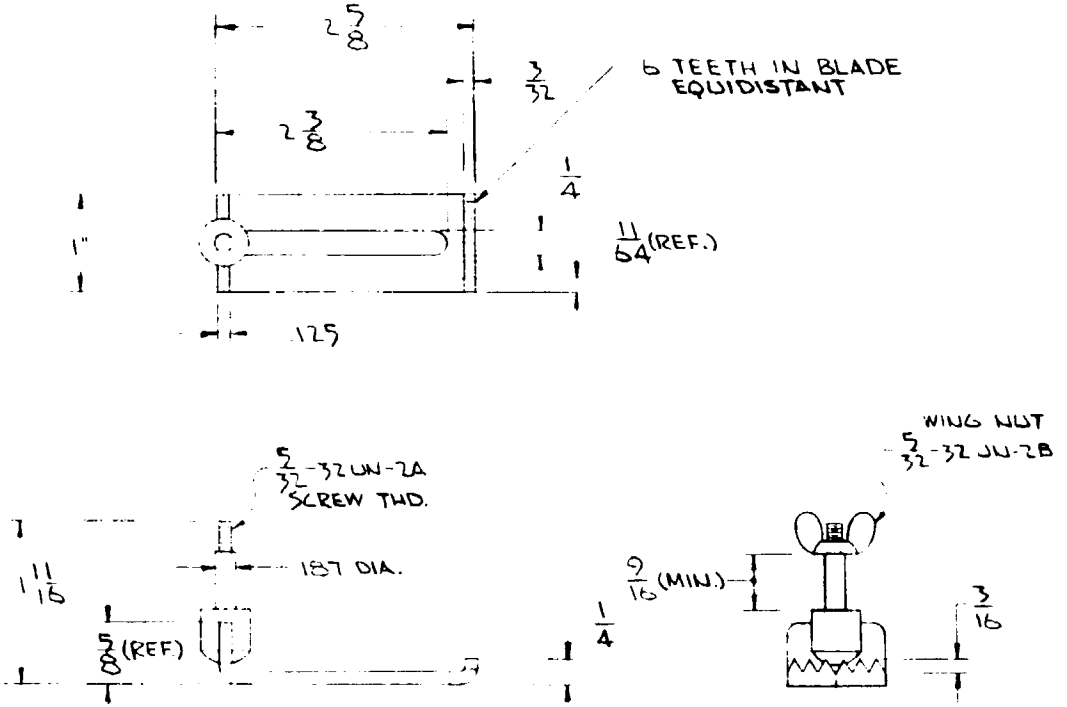


BLADE, LAMINECTOMY RETRACTOR, EPSTEIN, SINGLE PRONG, TYPE IV

FIGURE 5

NSN 6515-00-385-3710

TOLERANCE NOTES
REMOVE BURRS AND BREAK ALL SHARP EDGES UNLESS OTHERWISE SPECIFIED.
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 1°

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

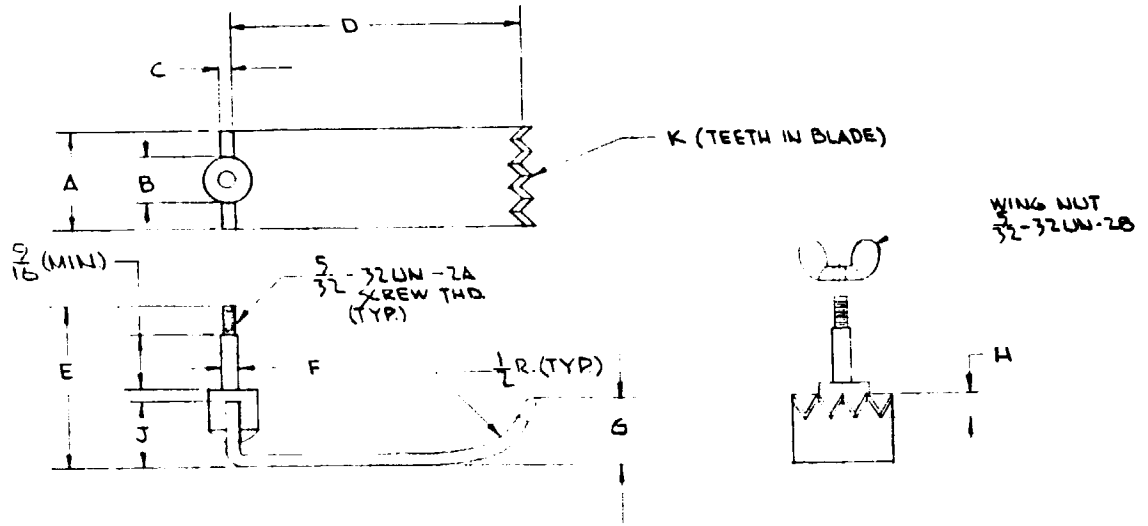


BLADE, LAMINECTOMY RETRACTOR, HIBBS, SINGLE PRONG, TYPE V

SIZE	NSN	DIMENSIONS A	B	C	D	E	F	G	H	J	K
1	6515-00-385-3711	1"	1/2 D.	.125	2	1 5/8	.187 DIA.	1/2	3/16	5/8	5
2	6515-00-385-3739	2"	1/2 D.	.125	2	1 11/16	.187 DIA.	1/2	3/16	5/8	9
3	6515-00-385-3740	1"	1/2 D.	.125	3	1 13/16	.187 DIA.	5/8	3/16	5/8	5
4	6515-00-385-3751	2"	1/2 D.	.125	3	1 7/8	.187 DIA.	1/2	3/16	5/8	8
5	6515-00-111-6383	2"	1/2 D.	.125	4	1 11/16	.187 DIA.	19/32	3/16	5/8	8

TOLERANCE NOTES:
REMOVE BURRS AND BREAK ALL SHARP EDGES UNLESS OTHERWISE SPECIFIED.
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 5°

FIGURE 6

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

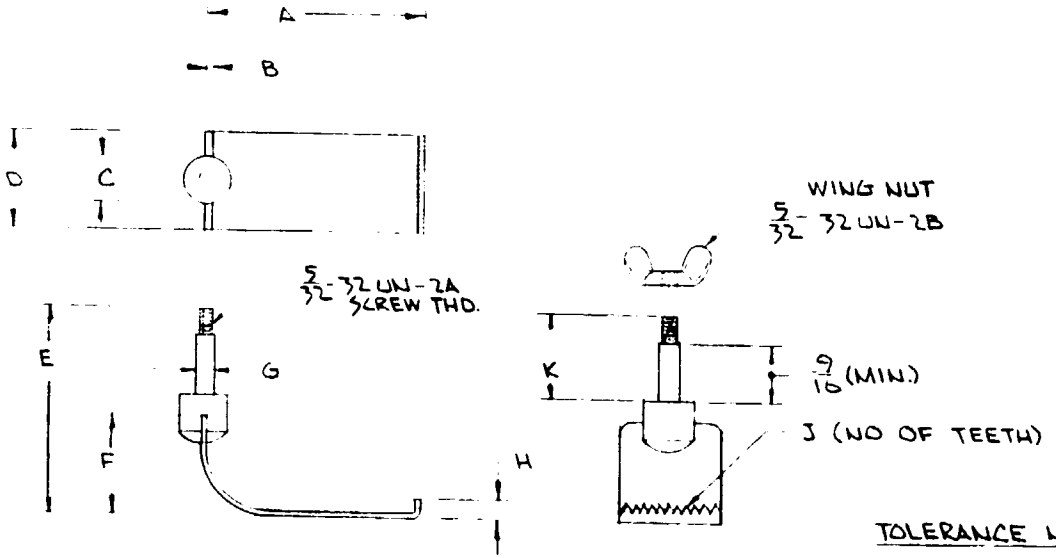

SIZE	NSN	DIMENSIONS									
		A	B	C	D	E	F	G	H	J	K
1	6515-00-389-9289	2¼	.062	½ D.	1"	2⅛	1 1/16	3/16 D.	3/16	11	⅞
2	6515-00-389-9291	3	.062	½ D.	1"	2⅛	1 1/16	3/16 D.	3/16	11	⅞
3	6515-00-392-0724	3½	.062	½ D.	2"	2⅛	1 1/16	3/16 D.	3/16	22	⅞

TOLERANCE NOTES:

REMOVE BURRS AND BREAK ALL SHARP EDGES UNLESS OTHERWISE SPECIFIED.
UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES.
UNLESS OTHERWISE SPECIFIED TOLERANCES ON FRACTIONS ± 1/32
DECIMALS ± .002
ANGLES ± 1°

BLADE, LAMINECTOMY RETRACTOR, MEYERDING, SINGLE PRONG, TYPE VI

FIGURE 7

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number (NSN), the Item Identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Inspection lot. The inspection lot shall be determined in accordance with MIL-STD-105.

4.2.2 Sampling for visual and dimensional examination. Sampling for examination shall be in accordance with MIL-STD-105 and as indicated in table I. The unit of product for examination purposes shall be one retractor body assembly or one blade.

TABLE III. Sampling criteria for visual and dimensional examination.

Type of defect	Inspection level	AQL (percent defective)
Major A	II	1.0
Major B	S-4	1.0
Minor A	II	4.0
Minor B	S-2	4.0

4.2.3 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in table II. Unless otherwise specified, the unit of product for tests shall be one component part of the retractor body or one blade and attachment device. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

TABLE IV. Sampling criteria for tests.

Item	Characteristics	Requirements	Test Procedure	Inspection level	AQL (percent defective)
Component part & Retractor body assembly and blade with nut	Hardness	3.3.1.4	4.5.1	S-2	1.5
	Corrosion	3.3.1.5	4.5.2.1	S-2	1.5
Component part 1 /	Corrosion	3.3.1.5	4.5.2.2	S-2	1.5

1 / Component parts fabricated from AISI Type 400 series material only.

4.2.4 Raw materials. A sufficient amount from each lot of each metal used in the construction of the instrument shall be selected for chemical analysis.

4.3 Examination for visual and dimensional defects. The retractor or blade shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in tables III and V. Examination however, shall not be restricted to defects listed in table V. Any retractor or blade in the sample containing one or more defects shall be rejected and if the number of defective retractors or blades in any sample exceeds the acceptance number for that sample, the lot represented by that sample shall be rejected.

TABLE V. Classification of defects.

Categories	Defects
Critical	None defined.
Major	
101	Retractor body design not as specified.
102	Blade style and size not as specified for appropriate NSN.
103	Any component part missing.
104	Not free from sharp edges, rough areas, burrs, cracks, grind marks or overlaps.
105	Blade not capable of being attached to retractor.
Minor	
201	Finish not as specified.
202	Not permanently and legibly marked with either the name or trademark of the contractor.
203	Physical dimensions not as specified.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

4.5 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.5.1 Hardness. Rockwell hardness shall be determined in accordance with ASTM test methods E-10, E-18, or E-92. A minimum of 5 hardness reading shall be made on test specimens representative of the material used in the fabrication of the blades including attachment and on the component parts of the retractor body. Conversion of Vickers or Brinell hardness values to Rockwell values shall be in accordance with ASTM Hardness Conversion Tables E-140.

4.5.2 Corrosion tests.

4.5.2.1 Boil test. The blade and attachment device and the retractor body assembly or component parts shall be subjected to the boil test as specified in GG-I-526.

4.5.2.2 Copper sulfate test. Parts fabricated of AISI Type 400 series material shall be subjected to the copper sulfate test as specified in GG-I-526.

4.6 Inspection of packaging. The sampling and inspection of the preservation and interior package marking shall be in accordance with groups A and B quality conformance inspection requirements of MIL-P-116. The sampling and inspection of the packing and marking for shipment and storage shall be in accordance with the quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

5. PACKAGING

5.1 Preservation. Preservation shall be level A or C as specified (see 6.2).

5.1.1 Level A.

5.1.1.1 Cleaning. Retractors and blades shall be cleaned in accordance with MIL-P-116, process C-1.

5.1.1.2 Drying. Retractors and blades shall be dried in accordance with MIL-P-116.

5.1.1.3 Preservative application. Preservatives shall not be used.

5.1.1.4 Unit package.

5.1.1.4.1 Retractors. Each retractor shall be packaged conforming to MIL-P-116, method IC-2.

5.1.1.4.2 Blades. Each blade shall be wrapped in neutral tissue or other suitable anti-corrosive material. Each protected blade shall be packaged in accordance with MIL-P-116, method IC-1.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

5.1.1.5 Intermediate package. Twelve unit packages containing retractors or twelve unit packages containing blades of one style and size only shall be packaged in a box conforming to PPP-B-566; PPP-B-636, class domestic, or PPP-B-676. Closure shall be as specified in the applicable box specification.

5.1.2 Level C. The level C preservation for retractors and blades shall conform to MIL-STD-794 requirements for this level.

5.2 Packing. Packing shall be level A, B or C, as specified (see 6.2).

5.2.1 Level A. Three intermediate packages containing retractors or six intermediate packages containing blades of one style and size only shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, overseas type; PPP-B-621, class 2, or PPP-B-636, class weather-resistant. Fiberboard boxes shall be waterproofed as specified in PPP-B-636. Closure and strapping shall conform to the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof liner conforming to MIL-L-10547. Closure and sealing shall be as specified in the liner specification.

5.2.2 Level B. Three intermediate packages containing retractors or six intermediate packages containing blades of one style and size only shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-601, domestic type; PPP-B-621, class 1, or PPP-B-636, class domestic. Closure shall be as specified in the applicable box specification.

5.2.3 Level C. The level C packing for retractors and blades shall conform to MIL-STD-794 requirements for this level.

5.2.4 Unitized loads. Unitized loads, commensurate with the level of packing specified in the contract or order, shall be used whenever total quantities for shipment to one destination equal 40 cubic feet or more. Quantities less than 40 cubic feet need not be unitized. Unitized loads shall be uniform in size and quantities to the greatest extent practicable.

5.2.4.1 Levels A and B. Retractors and blades packed as specified in 5.2.1 and 5.2.2, shall be unitized on pallets conforming to MIL-STD-147.

5.2.4.2 Level C. Retractors and blades packed as specified in 5.2.3, shall be unitized as specified in MIL-STD-794.

5.3 Marking.

5.3.1 Levels A, B, and C. Each unit pack, intermediate pack, exterior container and unitized load shall be marked as specified in MIL-STD-129.

5.4 General.

5.4.1 Exterior container. Exterior container (see 5.2.1, 5.2.2, and 5.2.3) shall be of minimum tare and cube consistent with the protection required and shall contain equal quantities of identical stock numbered items to the greatest practicable.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

5.4.2 Packaging inspection. The inspection of these packaging requirements shall be in accordance with 4.6.

6. NOTES

6.1 Intended use. The hemilaminectomy retractor shall be suitable for use with selected, interchangeable and detachable blades for laminectomy procedures.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number and date of this specification.
(b) Blade style and size (see 1.2.1).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).
(d) NSN.

6.3 This specification is intended to cover the following item appearing in the Federal Supply Catalog:

NSN	Item Identification	Specification designation	
		Style	Size
6515-00-385-3685	RETRACTOR, LAMINECTOMY, Haverfield-Scoville	-	-
6515-00-392-0722	BLADE, LAMINECTOMY RETRACTOR, Scoville, Single Hook, 2 inches Long	I	1
6515-00-392-0723	BLADE, LAMINECTOMY RETRACTOR, Scoville, Single Hook, 3 inches Long	I	2
6515-00-379-4389	BLADE, LAMINECTOMY RETRACTOR, Taylor, 3 Prong, 1-3/4 inches Long, 1-1/2 inches Wide	II	1
6515-00-376-7776	BLADE, LAMINECTOMY RETRACTOR, Taylor, 4 Prong, 1-7/8 inches Long, 2 inches Wide	II	2
6515-00-376-7784	BLADE, LAMINECTOMY RETRACTOR, Taylor, 4 Prong, 2-1/2 inches Long, 2-1/4 inches Wide	II	3
6515-00-376-7789	BLADE, LAMINECTOMY RETRACTOR, Scoville, 4 Prong, 1-5/8 inches Long, 1-1/2 inches Wide	III	1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

6515-00-385-3687	BLADE, LAMINECTOMY RETRACTOR, Scoville, 4 Prong, 2-5/8 inches Long, 1-3/4 inches Wide	III	2
6515-00-385-3710	BLADE, LAMINECTOMY RETRACTOR, Epstein, Single Prong, 2-1/4 inches Long, 1 inch Wide	IV	-
6515-00-385-3711	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 2 inches Long, 1 inch Wide	V	1
6515-00-385-3739	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 2 inches Long, 2 inches Wide	V	2
6515-00-385-3740	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 3 inches Long, 1 inch Wide	V	3
6515-00-385-3751	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 3 inches Long, 2 inches Wide	V	4
6515-00-111-6383	BLADE, LAMINECTOMY RETRACTOR, Hibbs, Single Prong, 4 inches Long, 2 inches Wide	V	5
6515-00-389-9289	BLADE, LAMINECTOMY RETRACTOR, Meyerding, Single Prong, 2-1/4 inches Long, 1 inch Wide	VI	1
6515-00-389-9291	BLADE, LAMINECTOMY RETRACTOR, Meyerding, Single Prong, 3 inches Long, 1 inch Wide	VI	2
6515-00-392-0724	BLADE, LAMINECTOMY RETRACTOR, Meyerding, Single Prong, 3-1/2 inches Long, 2 inches Wide	VI	3

6.5 Cross-reference of classifications. This specification revises end item classification to conform to industry practice. Classes, types and sizes are changed to styles and sizes. The new classification, styles and sizes (see 1.2) of end items are functionally and dimensionally interchangeable with items specified under the prior classification (see table VI), and are substitutable, one for the other.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

TABLE VI. Prior classification.

Classes, style and sizes
Class A - Retractor
Class B - Blades
Type I - Scoville, Single Hook
Size 1 - 2 inches long (deep)
Size 2 - 3 inches long (deep)
Type II - Taylor
Size 1 - small (1-3/4 inches long (deep) x 1-1/2 inches wide)
Size 2 - medium (1-7/8 inches long (deep) x 2 inches wide)
Size 3 - large (2-1/2 inches long (deep) x 2-1/4 inches wide)
Type III - Scoville, Laminectomy
Size 1 - 1-5/8 inches x 1-1/2 inches
Size 2 - 2-5/8 inches x 1-3/4 inches
Type IV - Epstein
Type V - Hibbs
Size 1 - 2 inches long (deep) x 1 inch wide
Size 2 - 2 inches long (deep) x 2 inches wide
Size 3 - 3 inches long (deep) x 1 inch wide
Size 4 - 3 inches long (deep) x 2 inches wide
Size 5 - 4 inches long (deep) x 2 inches wide
Type VI - Meyerding
Size 1 - 2-1/4 inches long (deep) x 1 inch wide
Size 2 - 3-1/2 inches long (deep) x 1 inch wide
Size 3 - 3-1/2 inches long (deep) x 2 inches wide

6.6 Changes from previous issue. Asterisks are not used in this revision to identify changes with respect to the previous issue, due to the extensiveness of the changes.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing Activity:
DoD-MB

Agent:
DLA-DM
Project No. 6515-3226

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS: In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE: This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-ATT
2800 South 20th St.
Philadelphia, PA 19101

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
MIL-R-37103B	RETRACTOR, HEMILAMINECTOMY, HAVERFIELD-SCOVILLE AND BLADES, RETRACTOR, INTERCHANGEABLE

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)*: _____

5. PROBLEM AREAS

a. Paragraph Number and Wording:

b. Recommended Wording:

c. Reason/Rationale for Recommendation:

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T09:58Z
Check the source to verify that this is the current version before use.