MIL-S-37118A(DSA-DM)
27 April 1976
SUPERSEDING
MIL-S-37118
30 April 1975 and
MIL-W-37152
23 April 1975

MILITARY SPECIFICATION

SNARE, RECTAL, FRANKFELDT

This specification is approved for use by Defense Personnel Support Center, Defense Supply Agency, and is available for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a rectal snare, of the Frankfeldt design, suitable for use in surgical proctology procedures.

2. APPLICABLE DOCUMENTS

2.1 The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of the specification to the extent specified herein:

SPECIFICATIONS

FEDERAL

GG-I-526	-	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	-	Boxes, Folding, Paperboard.
PPP-B-636	-	Box, Shipping, Fiberboard.
PPP-B-676	-	Boxes, Set-up.

MILITARY

MIL-P-116	-	Preservation, Methods of.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

STANDARDS

MILITARY

MIL-STD-105	-	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	-	Marking for Shipment and Storage.

DRAWING

Defense Personnel Support Center (DPSC)
20423 Wire, Snare, Hinged Loop

(Copies of specifications, standards and drawing required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

2.2 Other publications. The following document forms a part of this specification to the extent specified herein. Unless otherwise indicated, the issue in effect on date of invitation for bids or request for proposals shall apply.

AMERICAN SOCIETY FOR TESTING AND MATERIALS (ASTM)

ASTM E-8 Tension Testing of Metallic Materials.

(Application for copies should be addressed to the American Society for Testing and Materials, 1916 Race Street, Philadelphia, PA 19103.)

3. REQUIREMENTS

3.1 Material.

3.1.1 Handle assembly. The handle assembly shall be fabricated from durable, corrosion-resistant material, of the highest quality throughout, suitable in all respects for the purpose intended.

3.1.2 Insulated stem assembly. The stem assembly shall be fabricated from class 3, type 304 material in accordance with GG-I-526, or from nickel-copper alloy (Copper content: 54.5 to 64.5 percent; Nickel content: 28.0 to 31.5 percent). The stem assembly shall be permanently insulated throughout its length. As an alternate, the stem shall be fabricated from a durable plastic, such as acetal copolymer or acetal homopolymer (Delrin), suitable for the purpose intended.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

3.1.3 Wire snare. The loop portion of the wire snare proper shall be fabricated from cold drawn, spring temper, wire having a minimum tensile strength of 304,000 pounds per square inch. The material shall be class 3, type 302 or 304 in accordance with GG-I-526. The stem proper, of the wire snare assembly, shall be fabricated from class 3, type 304 material in accordance with GG-I-526; or as an alternate, chromium plated nickel copper alloy (nominal composition 66.0 percent nickel and 31.5 percent copper). The rivet shall be fabricated from class 3, type 302, 303 or 304 material in accordance with GG-I-526. The loop material of the wire snare shall be treated and processed as to result in finished wire snares in full compliance with the requirements of this specification. The wire loop portion shall not be plated.

3.2 Style, design and dimensions. Shall be a rectal snare assembly of the Frankfeldt design, suitable for use in proctology procedures involving surgical procedures of the bowel terminus, while simultaneously providing coagulation by electrical supply. The assembly shall include a hinged loop wire snare assembly fabricated from materials specified in 3.1.3. The assembled pivoting member of the hinged loop shall be constructed so as to permit free motion between loops without perceptible axial or radial play. The wire shall be uniform in diameter, quality and temper. The snare wire assembly shall be in accordance with DPSC Drawing No. 20423. The insulated stem, that encloses the wire portion of the snare assembly, shall be fabricated from materials specified in 3.1.2. The insulated stem (outer tube) shall be 13-3/4 to 14-1/4 inches in length and shall be secured to an angulated handle assembly by means of a retaining screw. The handle shall possess finger grips, thumb ring, retaining screw to secure the hinged loop wire snare assembly proper, and a terminal post for electrical connection to an electrosurgical apparatus. The terminal post shall be electrically insulated from the handle. The outer insulated stem shall be of uniform size for suitable entrance into proctosigmoidoscopes. Style and design of the complete rectal snare assembly shall be as shown in Figure 1.

3.3 Finish. The wire loop of the snare assembly proper shall have a smooth, bright (highly polished) finish except for the stem and pivoting point which may have a satin finish. The insulated outer stem shall have a smooth uniform finish.

3.4 Passivation. All components fabricated from class 3 material shall be properly passivated.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

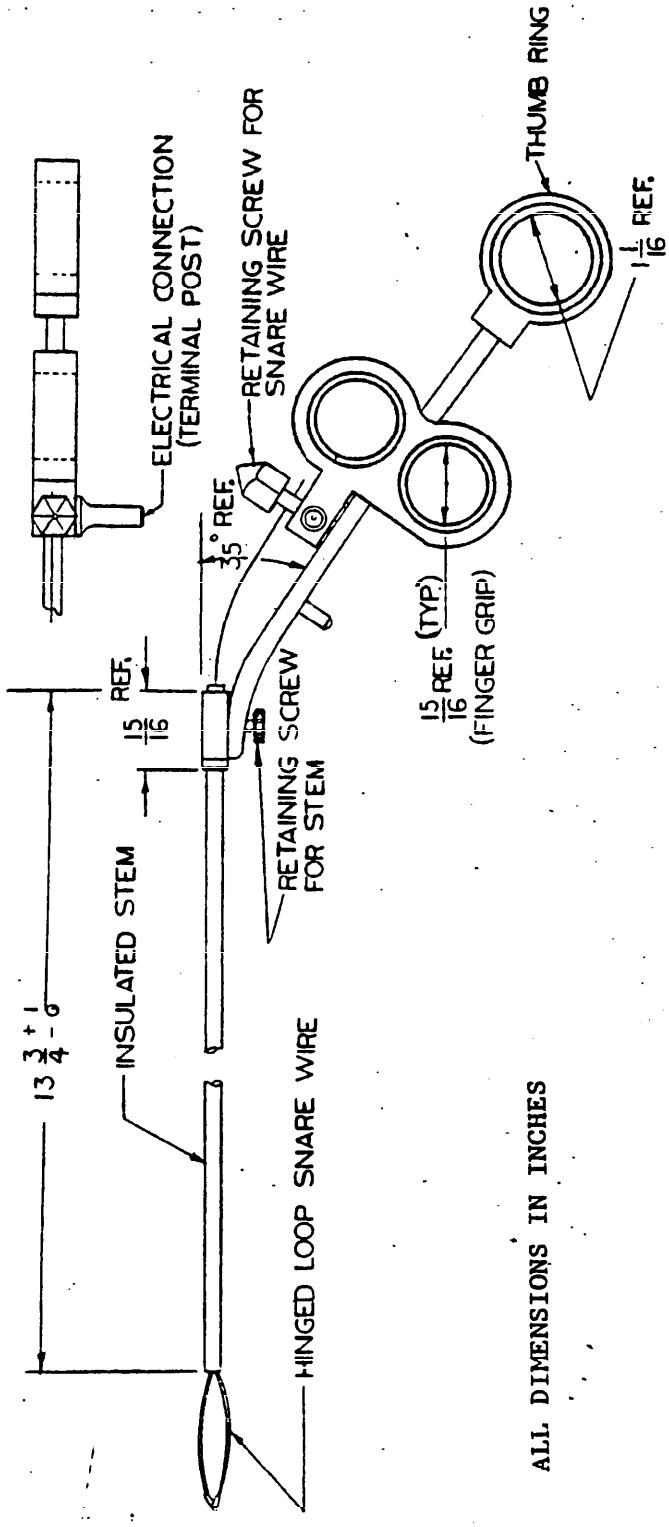


FIGURE 1. Snare, rectal, Frankfeldt

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

3.5 Boil test. The materials used in the fabrication of the wire snare assembly, specified in 3.1.3, shall show no evidence of corrosion when tested as specified in 4.4.1.

3.6 Tensile strength. The wire used in the fabrication of the loop portion of the snare shall exhibit a minimum tensile strength of 304,000 pounds per square inch when tested as specified in 4.4.2.

3.7 Snare operation. The rectal snare assembly shall exhibit free motion when tested as specified in 4.4.3. In addition, the hinged loop of the snare shall not break, or exhibit perceptible axial or radial movement.

3.8 Identification marking. The rectal snare assembly shall be legibly and permanently marked with the contractor's name or registered trademark.

3.9 Service data. The contractor shall enclose, with each rectal snare assembly, two copies of one or more booklets which contain instructions for safe operation, maintenance and a list of component parts. Each component of the assembly shall be identified in the service data and parts list by the manufacturer's part number. The contractor shall forward 15 copies of the service data to the Contracting Officer. The copies shall be addressed to the Defense Personnel Support Center, Directorate of Medical Materiel, 2800 South 20th Street, Philadelphia, PA 19101.

3.10 Workmanship. Workmanship shall be first class throughout. Rectal snare assemblies shall be free from burrs, cracks, pits, sharp edges, scale, corrosion and other defects which detract from their appearance or impair their serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:00Z
Check the source to verify that this is the currentversion before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the steel alloys, nickel-copper alloys and plastic, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the National Stock Number (NSN), the item identification, the name of the component and material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as indicated in table I. Unit of product for examination purposes shall be one complete rectal snare, or one wire snare, as applicable (see 6.3).

TABLE I. Sampling criteria for examination.

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in table II. Unit of product for test purposes shall be one complete rectal snare, or one wire snare as applicable (see 6.3). Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

TABLE II. Sampling criteria for tests.

Component	Characteristic	Rqmt.	Test procedure	Inspection level	AQL
Rectal snare assembly	Snare operation test	3.7	4.4.3	S-1	1.0
Wire snare assembly	Dimensions	3.2	----	S-1	2.5
	Boil test	3.5	4.4.1	S-2	1.5
	Tensile strength	3.6	4.4.2	S-2	1.5

4.2.3 Raw materials. A sufficient quantity of each lot of each metal used in the construction of the rectal snare assemblies shall be selected for chemical analysis.

4.2.4 Sample unit usage. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics.

4.3 Examination of assemblies. The rectal snare assemblies (or wire snare assemblies when procured separately) shall be examined to determine compliance with all requirements contained in this specification. Examination shall be conducted as specified in tables I and III. Examination, however, shall not be restricted to defects listed in table III. Any items in the sample containing one or more defects shall be rejected and if the number of defective rectal snare assemblies in any sample exceeds the acceptance number for that sample, the lot represented by the sample shall be rejected.

TABLE III. Classification of defects.

Categories	Defects
Critical	None defined.
Major	
101	Rectal snare not furnished completely assembled with all specified components.
102	Handle of snare not electrically insulated from terminal post.
103	Wire snare component not readily removed from, or assembled to, the handle assembly.
104	Snare assembly not free from burrs, cracks, pits, sharp edges, scale, corrosion and rough areas.
105	Outer stem, or tube, not insulated throughout its length when of metallic construction.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

TABLE III. Classification of defects (cont'd)

Categories	Defects
Major	
106	Handle of snare does not possess appropriate terminal post for electrical connection.
107	Loop of snare wire does not possess a smooth, bright finish.
108	Loop of snare wire not properly assembled.
Minor	
201	Service data not furnished.
202	Contractor's name or registered trademark not indicated on snare.

4.3.1 Packaging inspection. The inspection of the unit, intermediate package, packing and marking for shipment and storage shall be in accordance with quality assurance provisions of the applicable container specification and the marking requirements of MIL-STD-129.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Boil test. The wire snare assembly shall be subjected to the boil test in accordance with GG-I-526.

4.4.2 Tensile strength test. The wire shall be subjected to the tensile strength test in accordance with ASTM E-8, Tension Testing of Metallic Materials.

4.4.3 Snare operation test. The handle member of the completely assembled rectal snare shall be actuated at least 10 times without the use of lateral excessive force. The wire snare proper shall be observed for any loop bending, or loop breakage at the hinged point, perceptible axial or radial play, and sluggish or binding action through the insulated stem.

5. PACKAGING

5.1 Preservation-packaging. Preservation-packaging shall be level A or C as specified (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

5.1.1 Unit of issue. One rectal snare or one wire snare, as specified, constitutes one unit of issue.

5.1.2 Level A.

5.1.2.1 Cleaning. Snares shall be cleaned in accordance with MIL-P-116, process C-1.

5.1.2.2 Drying. Snares shall be dried in accordance with MIL-P-116.

5.1.2.3 Preservative application. Preservatives shall not be applied to snares.

5.1.2.4 Unit packaging. Each rectal snare or wire snare shall be packaged in accordance with MIL-P-116, method IA-15 or method IC-2. Each wire snare shall be packaged in accordance with MIL-P-116, method IA-8 or method IC-1.

5.1.2.5 Intermediate package. Six wire snares packaged as specified in 5.1.2.4 shall be packed in a box conforming to PPP-B-566, PPP-B-636, class domestic or PPP-B-676. Closure shall be as specified in the appendix of the applicable box specification. An intermediate package shall not be required for rectal snares.

5.1.3 Level C. Snares shall be clean, dry and individually packaged in a manner that will afford adequate protection against corrosion and physical damage during shipment from the supply source to the first receiving activity.

5.2 Packing. Packing shall be level A, B or C as specified, (see 6.2).

5.2.1 Level A. Twelve unit packages containing rectal snares or sixty intermediate packages containing wire snares shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-636, class weather-resistant. Closure, strapping and waterproofing shall be as specified in the appendix of the box specification.

5.2.2 Level B. Twelve unit packages containing rectal snares or sixty intermediate packages containing wire snares shall be packed in an exterior container designed for a type 2 load and conforming to PPP-B-636, class domestic. Closure shall be as specified in the appendix of the box specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

5.2.3 Level C. The packaged snares shall be packed in shipping containers in a manner that will afford adequate protection against damage during direct shipment from the supply source to the first receiving activity. These packs shall conform to the applicable carrier rules and regulations.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior containers shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Sterilization. The complete rectal snare assembly shall be capable of withstanding cold chemical or gas sterilization procedures presently used in the medical profession. In addition to the above, the wire snare assembly shall also be capable of withstanding steam sterilization.

6.2 Ordering data. Purchasers should exercise any desired options ordered herein, and the procurement document should specify the following:

(a) Title, number, and date of this specification.
(b) National Stock Number of complete rectal snare assembly, or wire snare assembly, as applicable (see 6.3).
(c) Applicable levels of packing and packaging (see 5.1 and 5.2).

6.3 This specification covers the following items appearing in the Federal Supply Catalog:

National Stock Number	Item Identification
6515-00-367-5600	SNARE, RECTAL, Frankfeldt
6515-00-664-9142	WIRE, SNARE, Hinged Loop.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

6.4 Changes from previous issue. Asterisks are not used in this revision to indicate changes, due to the extensiveness of the changes.

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-2011

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-S-37118A(DSA-DM) SNARE, RECTAL, FRANKFELDT

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 68 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S.MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:00Z
Check the source to verify that this is the current version before use.