MIL-S-37125A
21 May 1975
SUPERSEDING
MIL-S-37125
20 November 1974

MILITARY SPECIFICATION

SCISSORS, NASAL, FOMON

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers nasal scissors of the Fomon design.

1.2 Classification. Scissors shall be furnished in the following types as indicated below (see 6.2):

Type I - Angular
Type II - Curved

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical, General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Boxes, Shipping, Fiberboard.
PPP-B-676	Boxes, Set-up.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof or Waterproof, Flexible.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:01Z
Check the source to verify that this is the current version before use.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

(Copies of specifications and standards, required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General Requirements. The scissors shall be in accordance with the applicable requirements of GG-I-526, and as specified herein.

3.2 Material. The scissors shall be fabricated from Class 4, type 420 material, except that the carbon content shall be 0.30 percent, minimum.

3.3 Hardness. After proper stress relieving, the Rockwell hardness of the scissors shall be C-50 to C-55.

3.4 Style, design, and dimensions. Shall be in accordance with Figure 1, for Type I and with Figure 2, for Type II.

3.5 Finish. Shall be mirror, except the inside of the blades which may be crocus.

3.6 Scissors performance. The scissors shall cut a continuous length of at least 3/8 inch of the test material when tested as specified in 4.5.1. Cutting edge shall extend to the end of the tip of scissors.

3.7 Identification marking. In addition to GG-I-526 requirements, scissors of foreign manufacture shall also be marked "stainless."

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.

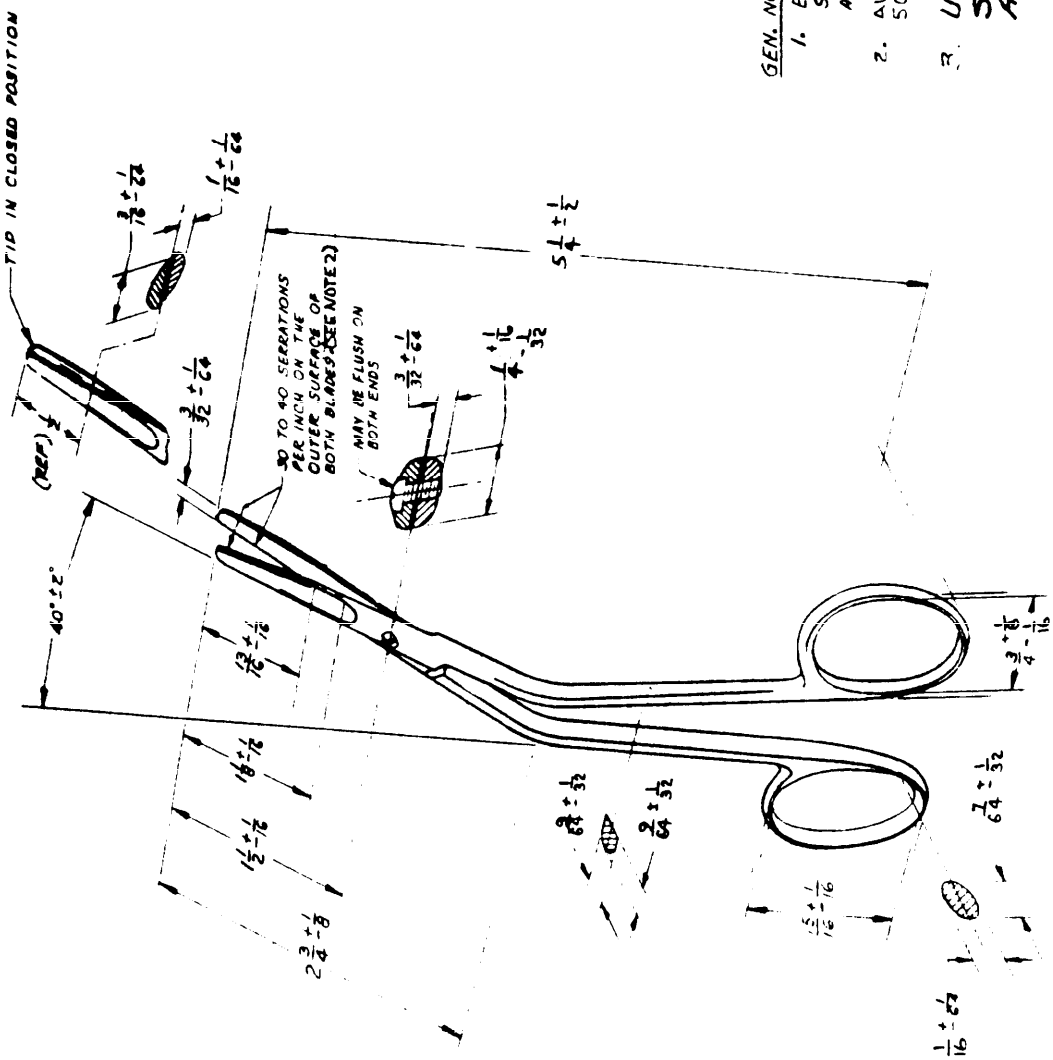


FIGURE 1

SCISSORS, NASAL, ANGULAR, FOMON

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:01Z
Check the source to verify that this is the current version before use.

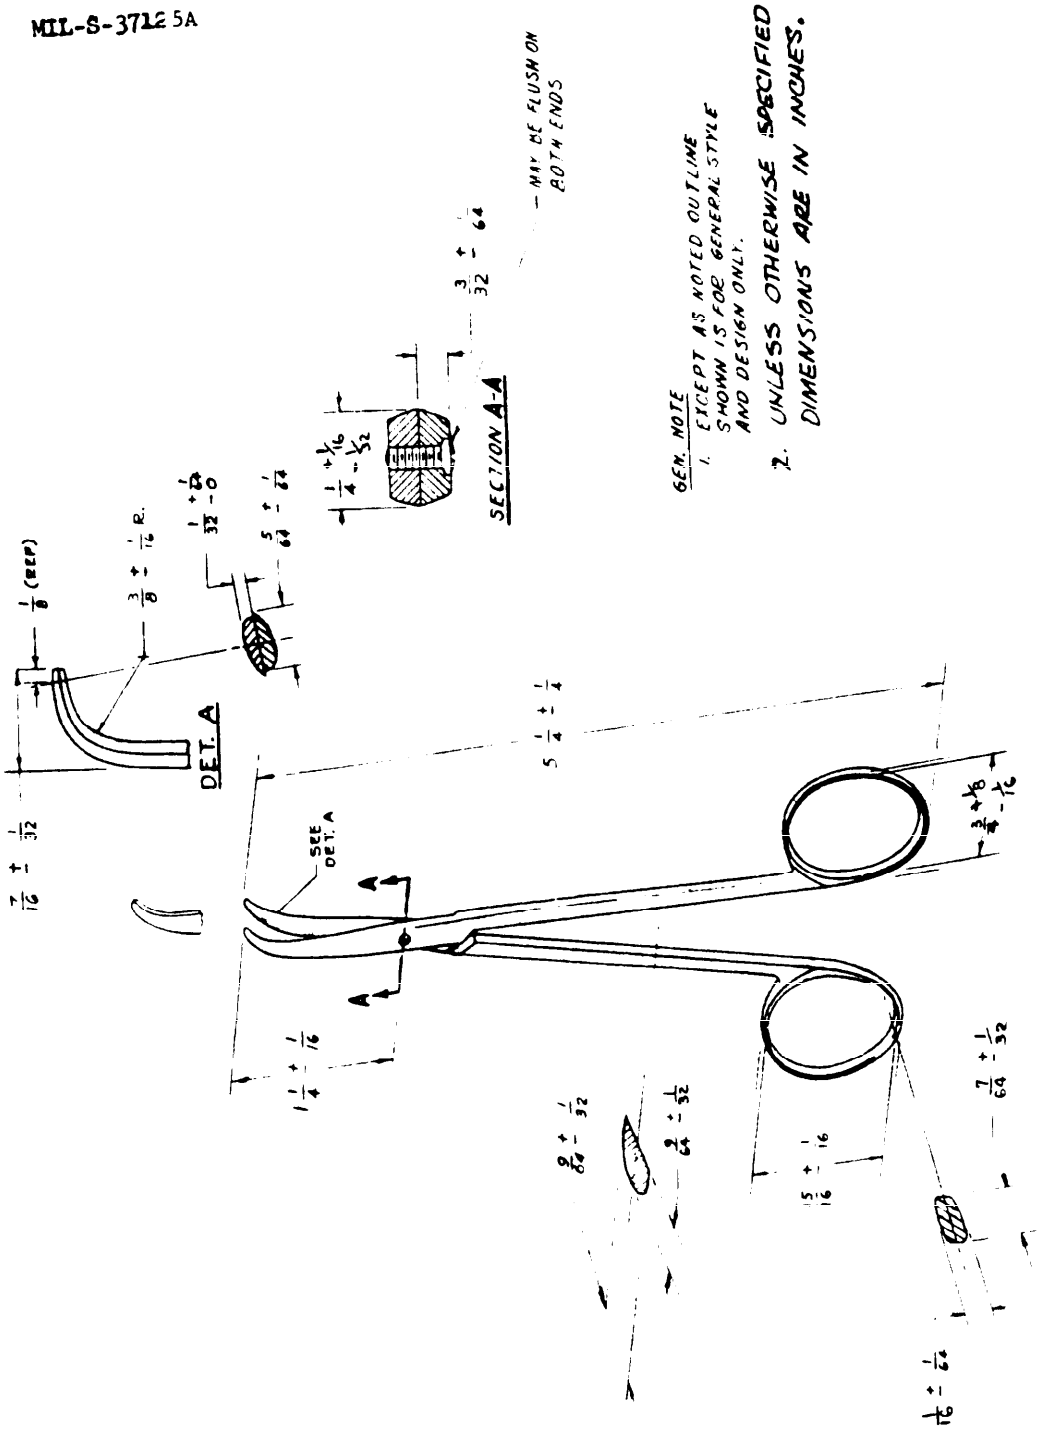


FIGURE 2

SCISSORS, NASAL, CURVED, FOMON, 5-1/4 INCH

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:01Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the stainless steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels shall be as indicated in Table I. The unit of product for examination purposes shall be one scissors.

Table I. Sampling for Examination

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as indicated in Table II. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.

Table II. Sampling for Tests

Component	Characteristics	Req.	Test procedure	Insp. level	AQL
Entire scissors	Composition analysis	3.2 and GG-I-526	GG-I-526	**	*
Entire scissors	Performance test	3.6	4.5.1 and GG-I-526	II	1.5
Entire scissors	Hardness	3.3 and GG-I-526	GG-I-526	S-2	1.5
Entire scissors	Dimensions	3.4	-	S-1	3.5
Entire scissors	Copper sulfate	GG-I-526	GG-I-526	S-2	1.5
Entire scissors	Boil test	GG-I-526	GG-I-526	S-2	1.5

*Acceptance number shall be zero for all sample sizes.
**Sufficient amount from each lot of each metal used in the construction of the scissors shall be selected for composition analysis.

4.3 Examination.

4.3.1 Examination of scissors. The scissors shall be examined to determine compliance with specification requirements. Examination shall be conducted in accordance with MIL-STD-105 and the following classification of defects. Examination shall include, but not be limited to, the defects listed in Table III.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Style and design not as specified.
102	Scissors not constructed as specified.
103	Scissors not free from cracks, pits, dents, nicks or burrs.
104	Scissors not free from excessive play or excessive stiffness during cutting action.
105	Scissors not free from sharp edges except for cutting edge.
Minor	
201	Finish not as specified.
202	Scissors not permanently and legibly marked as required.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.

4.3.2 Examination of preparation for delivery. examination shall be made to determine whether the packaging, packing and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 with an AQL of 4.0 expressed in terms of defects per hundred units.

Table IV. Examination of Preparation for Delivery

Examine	Defect
Containers	Not as specified.
Contents	Not as specified.
Markings	Omitted: incorrect; illegible; improper location, sequence, or method of application.
Packaging and packing materials	Component missing or damaged.
Workmanship	Bulging or distortion of containers. Cushioning inadequate, improper or missing.

4.3.2.1 Examination of closure and reinforcement for containers. When shipping containers are required to comply with PPP-B-636, examination for defects in closure and reinforcement shall be in accordance with the appendix to that specification.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Scissors performance test. The test material shall be rubber dam meeting the requirements of the specification for NSN 6515-00-754-2469 Rubber Dam, Medium, 6 inches square. Three separate, consecutive tests shall be performed for each scissors as specified in GG-I-526.

5. PREPARATION FOR DELIVERY

5.1 Packaging. Packaging shall be level A or C, as specified (see 6.2).

5.1.1 Unit of issue. Each nasal scissors, as specified, constitutes one unit of issue.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.

5.1.2 Level A.

5.1.2.1 Unit package. Each pair of scissors of the type specified shall be thoroughly cleaned, wrapped in neutral tissue or other suitable anticorrosive material, and packaged in accordance with MIL-P-116, method 1C-1 except that a preservative shall not be utilized.

5.1.2.2 Intermediate package. Six unit packages of one type shall be packaged in a snug fitting box constructed in accordance with PPP-B-566 or PPP-B-676 except that commercial colors are acceptable. Closure shall be adequate to prevent accidental opening.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be Level A, B or C as specified (see 6.2).

5.2.1 Level A. Forty eight intermediate packages, containing scissors of one type only, shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2 or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Fiberboard boxes shall be waterproofed in accordance with 30.4 of PPP-B-636.

5.2.2 Level B. Forty eight intermediate packages containing scissors of one type only shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification except that the closure of fiberboard boxes shall conform to method I or II as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Intended use. The scissors are used in rhinoplasty surgery.

6.2 Ordering data. Purchasers should exercise any desired options offered herein, and the procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Type (see 1.2).
(c) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.3 National Stock No. coverage. This specification covers the following items appearing in the Federal Supply Catalog:

National Stock No.	Item Identification
6515-00-619-8914	SCISSORS, NASAL, Angular, Fomon, 5 inch
6515-00-656-0481	SCISSORS, NASAL, Curved, Fomon, 5-1/4 inch

It does not include all types or sizes as indicated by the title nor all types which are commercially available.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1953
is

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:01Z
Check the source to verify that this is the currentversion before use.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22-R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-S-37125A SCISSORS, NASAL, FOMON

NAME OF ORGANIZATION AND ADDRES

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426

REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, PA 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304



OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:01Z
Check the source to verify that this is the current version before use.