MIL-S-37151
30 January 1975

MILITARY SPECIFICATION

SCISSORS, TENOTOMY, CURVED, WESTCOTT, 4-1/2 INCH

This specification is approved for use by all Departments and Agencies of the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a tenotomy scissors, of the Westcott design, suitable for use in surgical procedures involving the eye.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents of the issue in effect on date of invitation for bids or request for proposals, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

GG-I-526	Instruments, Dental and Surgical; General Specifications.
PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Box, Wood, Wirebound.
PPP-B-601	Box, Wood, Cleated-plywood.
PPP-B-621	Box, Wood, Nailed and Lock-corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Set-up.

Military

MIL-P-116	Preservation, Methods of.
MIL-L-10547	Liners, Case and Sheet, Overwrap Water-Vaporproof or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

FSC 6515

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:04Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 General requirements. The scissors shall be in accordance with the applicable requirements of GG-I-526, and as specified herein.

3.2 Material. The scissors shall be fabricated from class 4, type 420 material, except that the carbon content shall be 0.30 percent minimum.

3.3 Hardness. After proper stress relieving, Rockwell hardness shall be C50 to C55.

3.4 Style, design and dimensions. Shall be a tenotomy scissors, of the Westcott design, suitable for use in delicate surgical procedures involving the eye. Scissors shall be of the spring-handle type with both points blunt. Scissors shall be in strict accordance with Figure 1.

3.5 Finish. Finish shall be mirror, except that the inside surfaces of the blades shall have a crocus finish.

3.5.1 Passivation. The scissors shall be properly passivated.

3.6 Cutting edges. Scissors shall cut a continuous length of at least 1/4 inch of the test material, when tested as specified in 4.4.1. This cutting requirement shall also include the tips of the scissors.

3.7 Identification marking. In addition to the requirements specified in GG-I-526, scissors of foreign manufacture shall be marked "stainless".

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:04Z
Check the source to verify that this is the current version before use.

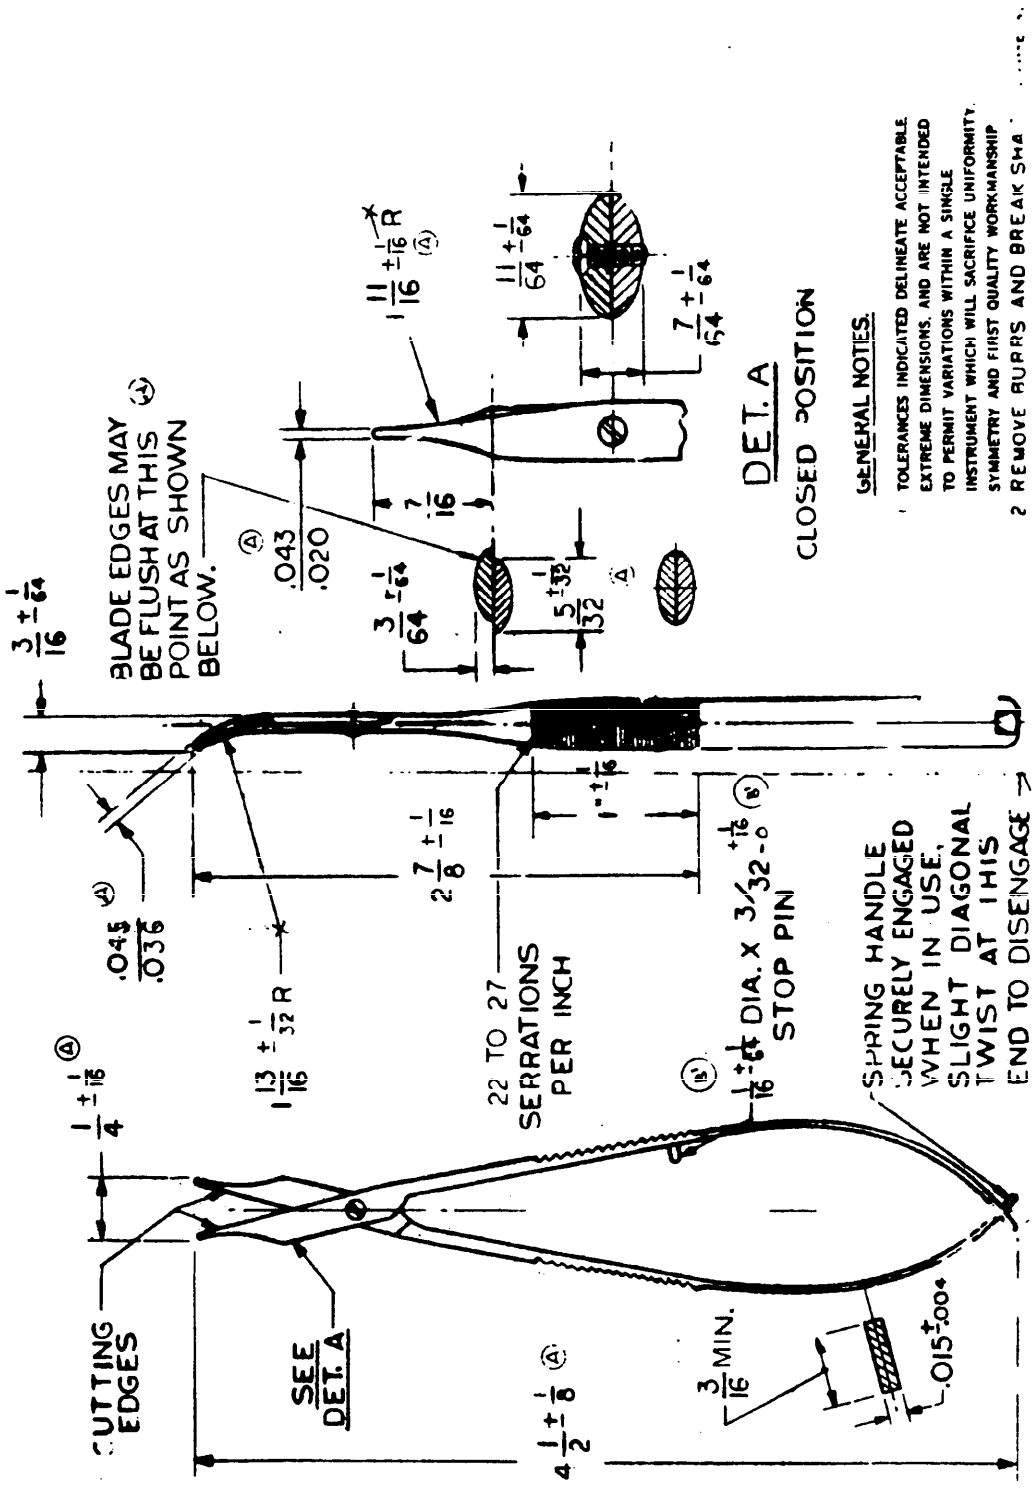


FIG. 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:04Z
Check the source to verify that this is the current version before use.

4.1.1 Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government, upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of 3 years after delivery of the supplies to which such records relate.

4.1.2 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

4.1.3 Certificates of quality. Certificates of quality, supplied by the manufacturer of the corrosion-resistant steel, may be furnished in lieu of actual performance of such testing by the contractor, provided lot identity has been maintained and can be demonstrated to the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the sample size, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in Table I. The unit of product for examination purposes shall be one scissors.

Table I. Sampling Criteria for Examination

Type defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	2.5

4.2.2 For tests. Sampling for tests shall be conducted in accordance with MIL-STD-105, and as indicated in Table II. Where feasible, the same sample unit shall be used for the determination of two or more test characteristics. The unit of product for test purposes shall be one scissors.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:04Z
Check the source to verify that this is the current version before use.

Table II. Sampling Criteria for Tests

Component	Characteristic	Requirement	Test procedure	Inspection level	AQL
Scissors	Hardness test	3.3 & GG-I-526	GG-I-526	S-2	1.5
	Dimensions	3.4		S-2	2.5
	Scissors performance test	3.6	4.4.1	II	1.0
	Copper sulfate test	GG-I-526	GG-I-526	S-2	1.0
	Boil test	GG-I-526	GG-I-526	S-2	1.0

4.2.3 Raw materials. A sufficient quantity of each lot of metal used in the construction of the scissors shall be selected for chemical analysis.

4.3 Examination.

4.3.1 Examination for scissors. The scissors shall be examined to determine compliance with all the requirements contained in this specification. Examination shall be conducted as specified in Tables I and III. Examination, however, shall not be restricted to defects listed in Table III. Any scissors in the sample containing one or more defects shall be rejected and if the number of defective scissors in any sample exceeds the acceptance number for the sample, the lot represented by that sample shall be rejected.

Table III. Classification of Defects

Categories	Defects
Critical	None defined.
Major	
101	Scissors not of the design specified.
102	Points of scissors sharp.
103	Scissors not of finish specified.
104	Scissors not free from cracks, burrs, pits, rough areas, scale and corrosion.
105	Spring handles disengage without slight diagonal twist at proximal end.
Minor	
201	Scissors not marked as specified in 3.7.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:04Z
Check the source to verify that this is the current version before use.

4.3.2 Examination for preparation for delivery. An examination shall be made to determine whether the packaging, packing, and marking comply with the requirements of Section 5. Defects shall be scored as specified in Table IV. Sampling shall be in accordance with MIL-STD-105. The sample unit shall be one container fully prepared for delivery. The lot shall be the number of containers offered for inspection at one time. The inspection level shall be S-2 and the acceptable quality level shall be 4.0 defects per hundred units.

Table IV. Examination for Preparation for Delivery

Examination	Defect
Containers	Not as specified.
Quantity	Quantity in interior packages and shipping containers not as specified.
Materials	Any component missing or damaged.
Workmanship	Inadequate application of components, such as incomplete closure of container flaps, tape improperly applied, or containers distorted.
Markings	Omitted, incorrect, illegible, improper size, location, sequence, or method of application.

4.4 Tests. Tests shall be conducted to determine compliance with specification requirements.

4.4.1 Scissors performance test. The test material shall be rubber dam meeting the requirements specified for National Stock No. 6520-00-754-2769, RUBBER DAM, Medium, 6 inches square. Three separate, consecutive tests shall be performed for each scissors as described and specified in GG-I-526.

5. PREPARATION FOR DELIVERY

5.1 Preservation and Packaging. Preservation and packaging shall be level A or C as specified (see 6.2).

5.1.1 Level A.

Source: https://assist.dla.mil -- Downloaded: 202640-21T10:04Z
Check the source to verify that this is the current version before use.

5.1.1.1 Cleaning and drying. Each pair of scissors shall be thoroughly cleaned and dried in accordance with the applicable method as specified in MIL-P-116.

5.1.1.2 Preservative. A preservative shall not be applied to the scissors.

5.1.1.3 Unit package. Each pair of scissors shall be wrapped in neutral tissue or other suitable anticorrosive barrier material and packaged in accordance with MIL-P-116, method IC-2.

5.1.1.4 Intermediate package. Six unit packages shall be packaged in snug fitting box constructed in accordance with PPP-B-566, PPP-B-636, type CF, class domestic or PPP-B-676. Closure of the box shall be adequate to prevent accidental opening.

5.1.2 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

5.2 Packing. Packing shall be level A, B or C as specified (see 6.2).

5.2.1 Level A. Forty eight intermediate packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.1.1 Case liner. Each Level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes. Each fiberboard box shall be waterproofed as specified in the appendix of PPP-B-636.

5.2.2 Level B. Forty eight intermediate packages shall be packed in an exterior container designed for a type 2 load and constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification. Closure of fiberboard boxes shall conform to method II as specified in PPP-B-636.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

Source: https://assist.dla.mil -- Downloaded: 202610-21T10:04Z
Check the source to verify that this is the current version before use.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Number, title and date of this specification.
(b) Applicable levels of packing and packaging.
(c) National stock number.

6.2 This specification covers National Stock Number 6515-00-619-8306 SCISSORS, TENOTOMY, Curved, Westcott, 4-1/2 inch, appearing in the Federal Supply Catalog.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Project No. 6515-1912

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:04Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

OMB Approval
No. 22 R255

INSTRUCTIONS: The purpose of this form is to solicit beneficial comments which will help achieve procurement of suitable products at reasonable cost and minimum delay, or will otherwise enhance use of the document. DoD contractors, government activities, or manufacturers/ vendors who are prospective suppliers of the product are invited to submit comments to the government. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements. Attach any pertinent data which may be of use in improving this document. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity.

DOCUMENT IDENTIFIER AND TITLE

MIL-S-37151

NAME OF ORGANIZATION AND ADDRESS

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE DOCUMENT CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY DOCUMENT REQUIREMENT CONSIDERED TOO RIGID

3. IS THE DOCUMENT RESTRICTIVE?

☐ YES ☐ NO *(If "Yes", in what way?)*

4. REMARKS

SUBMITTED BY *(Printed or typed name and address - Optional)*

TELEPHONE NO.

DATE

DD FORM 1 JAN 72 1426 REPLACES EDITION OF 1 JAN 66 WHICH MAY BE USED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:04Z
Check the source to verify that this is the current version before use.

FOLD

DEFENSE PERSONNEL SUPPORT CENTER
2800 South 20th Street
Philadelphia, Pa. 19101

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY
DoD - 304

U.S. MAIL

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

FOLD

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T10:04Z
Check the source to verify that this is the current version before use.