A-A-53396A
3 May 1989
SUPERSEDING
A-A-0053396(DM)
19 February 1988

COMMERCIAL ITEM DESCRIPTION

RASP, ANTRUM (Wiener, Trocar Tip)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a trocar tip, Wiener antrum rasp suitable for use in nasal surgical procedures.

Salient characteristics:

Material. The rasp blade and shank shall be fabricated of Class 4 martensitic corrosion-resistant steel in accordance with ASTM Designation F899. The rasp handle shall be fabricated of a suitable corrosion-resistant steel.

Style, design and dimensions. The style, design and dimensions of the rasp shall be in accordance with Figure 1. The blade shall have 13 to 14 serrations per inch and have an outside diameter of 5/32 ± 1/64 inch. The rasp shall have a trocar point. The handle may be hollow.

Hardness. The rasp blade and shank shall have a Rockwell Hardness C scale (HRC) of 50 to 60. The rasp handle shall have a Rockwell Hardness C scale (HRC) of 20, minimum when tested in accordance with ASTM Designations E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM Designation E140.

Finish. The finish of the rasp shall be mirror, satin or matte.

Resistance to corrosion. The rasp shall show no evidence of corrosion when tested in accordance with ASTM Designation F1089.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:19Z
Check the source to verify that this is the current version before use.

Identification marking and labeling. The rasp shall bear the contractor's name or registered trademark and the word "stainless". Rasp of foreign manufactures shall bear the name of the country of manufacture.

Workmanship. The rasp shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One rasp, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 as specified herein. The acceptable Quality level (AQL) shall be 0 for an inspection level of S-2. The unit of product for tests purposes shall be one rasp.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:19Z
Check the source to verify that this is the current version before use.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended, and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:19Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-113-2622	RASP, ANTRUM, WIENER, TROCAR TIP, LARGE

Ordering data (Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD - MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 47182

Project No. 6515-4569

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:19Z
Check the source to verify that this is the current version before use.

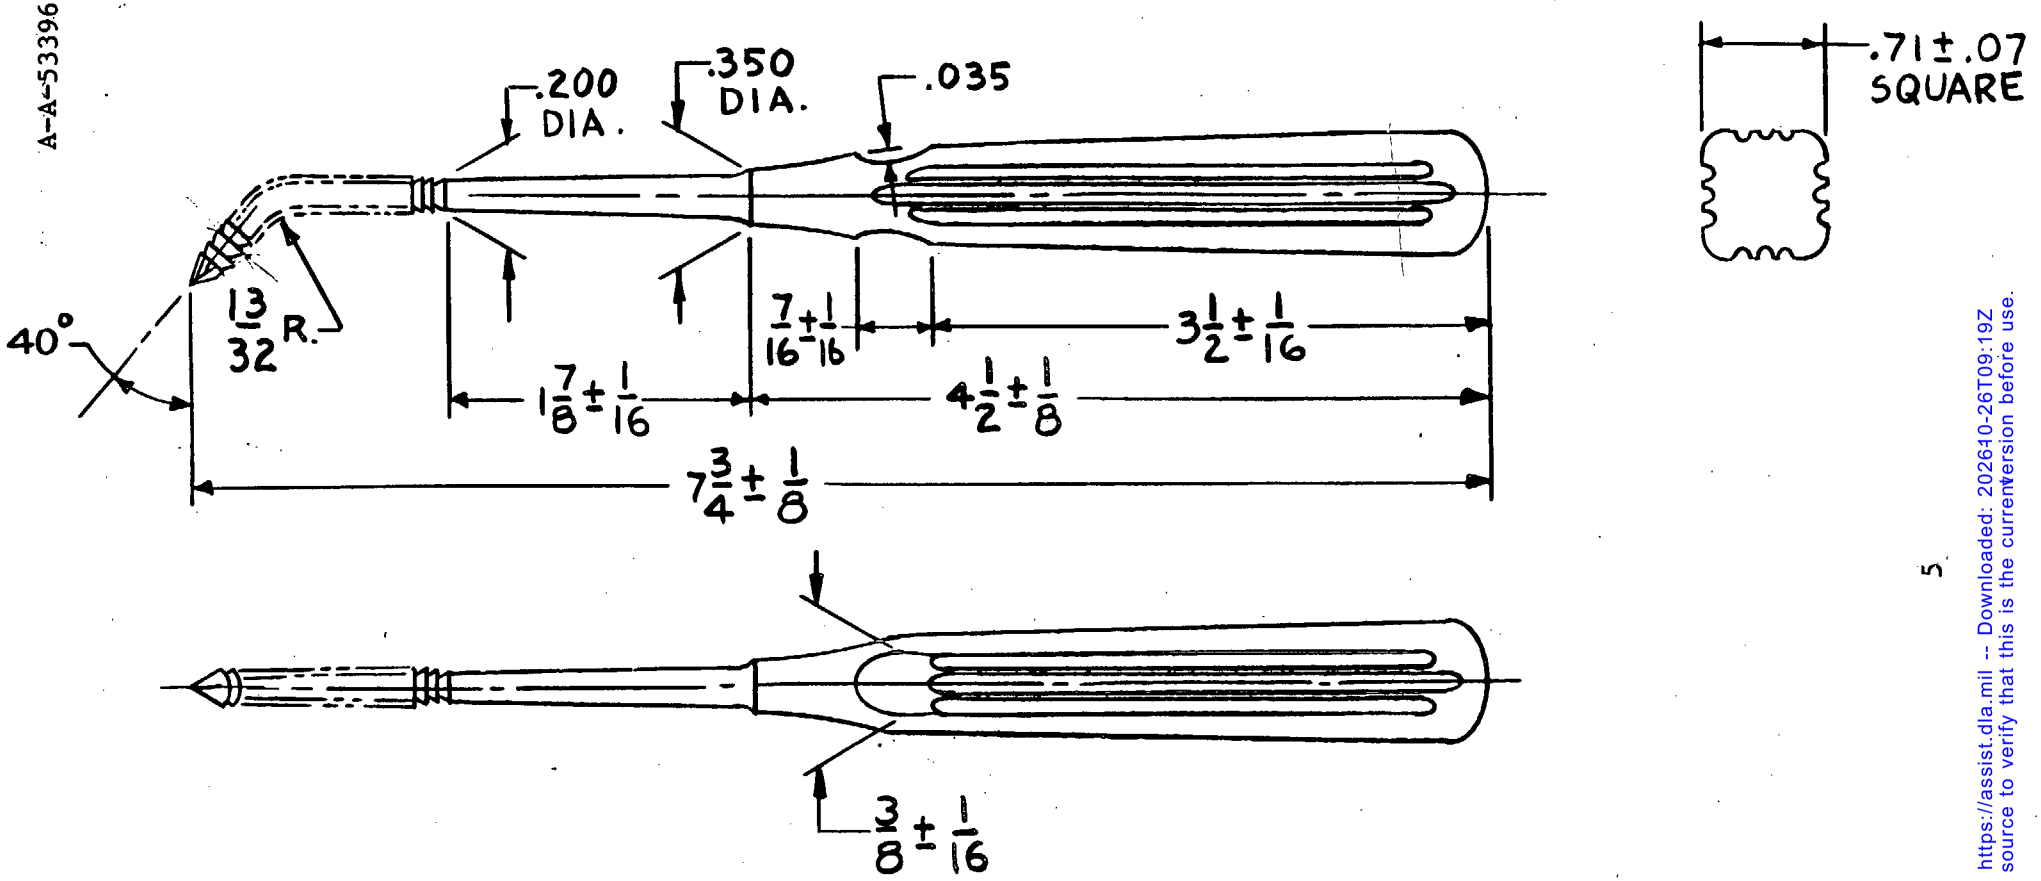

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1/64	± .005	± 1°

FIGURE 1 RASP, ANTRUM, WIENER

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:19Z
Check the source to verify that this is the current version before use.