

FED. SUP CLASS
6640

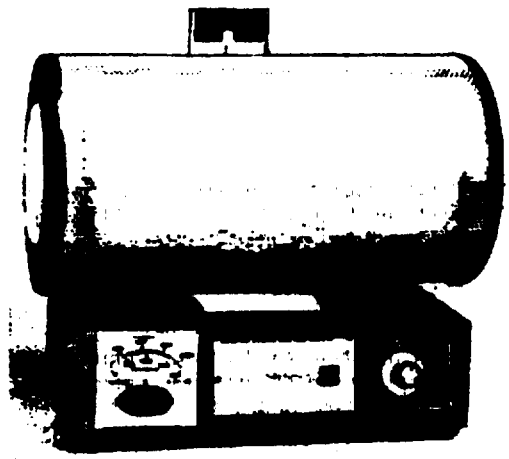

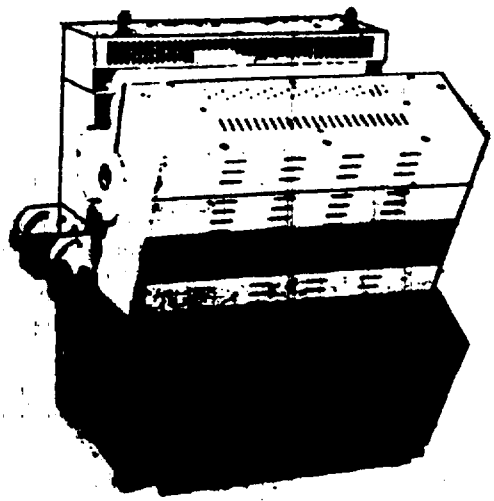

DIMENSIONS (cm)

POWER REQUIREMENTS

PART NUMBER	L						VOLTS AC*	Hz	W
MS3[illegible]							115	60	550
MS36[illegible]							120	50/60	1300
MS3611[illegible]							20 AC/DC	---	1000
MS36158							115	60	800
MS36158-5				8000	8	61	240	50/60	3800
MS36158-6			56	11000	15	91	240	50/60	11000
MS36158-7	23	50	29	960	2.5	30	115/230	50/60	960
MS36158-8	50	23	37	1400	5	30	115/230	50/60	1400
MS36158-9	80	30	37	3400	6.4	61	115/230	50/60	3400

*Unless otherwise specified.

MATERIAL: Furnaces shall be made of steel, ceramic insulation and chromel A or nickel-chromium resistance wire.

DESIGN: MS36158-1 and -2 furnaces shall be cylindrical shape mounted on an iron or steel frame. The chromel A heating wire shall be wound on a grooved refractory through which the combustion tube, or chamber, is inserted and held in position by grooves of the refractory. The heat insulating chamber is enclosed in a metal jacket. To regulate temperature below maximum voltage, an autotransformer or another type of control device must be used.

(A) CANCELLATION

CANCELLED
CANCELLED AFTER 23 OCT 1991
NO SUPERSEDING STANDARD

APPROVED 22 JUN 1961 REVISED (A) 23 OCT 1991

P.A. EA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust MS 99		FURNACE COMBUSTION TUBE, LABORATORY	MS36158
Procurement Specifications NONE	SUPERSEDES		SHEET 1 OF 2

DD FORM 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE CANCELLATION

Project Number 6640-1736-08

USER ACTIVITIES: ARMY - MD, CR
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
NAVY - OS
AIR FORCE - 82

MISC H/A
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:35Z
Check the source to verify that this is the current version before use.

FED. SUP CLASS
6640

MS36158-3 furnace shall be the same construction as -1 and -2, except it shall be powered by a 115 volt, 60 Hz transformer with a 20 volt output.

MS36158-4 shall be a hinged tube furnace with a built-in input adjuster to provide manual control of temperatures from 185° to 1000°C. Heating elements shall be nickel-chromium wire, helically wound and mounted on high temperature ceramic supports. The case shall be finished with heat resistant enamel and equipped with a heavy top supporting hinge, handle and snap catch.

MS36158-5 and -6 furnaces shall have the heating chamber divided into three zones for providing temperature control by use of three thermocouples. Each furnace shall have a controller unit, which will serve as the mounting base.

MS36158-7, -8, and -9 furnaces shall be single ... , but with a split cylindrical chamber that is heated by two semi-cylindri... g units, providing radial heat uniformity. The split-hinge design ... placement of the process tube and easy operation. The h... ally-coiled high temperature resistance wire. Each ... unit, which will serve as the mounting base.

CANCELLED
CANCELLED AFTER 23 OCT 1991
NO SUPERSEDING STANDARD

NOTE: Underwriters Laboratories, ... in design or dimensions ... variations do not affec... ments specified herei...

USER ACTIVITIES: ARMY - MD, SM
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
NAVY - OS
AIR FORCE - 82

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Suggestions for improvements and design applications and the activities are shall be made from this document.

APPROVED 9 OCT 1991 (A) REVISED

P.A. EA	INTERNATIONAL INTEREST	TITLE FURNACE COMBUSTION TUBE, LABORATORY	MILITARY STANDARD MS36158
Other Cust MS 99			
Procurement Specifications NONE	SUPERSEDES		SHEET 2 OF

DD FORM 1 MAY 73 872 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE Project Number 6840-1736-(

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:35Z
Check the source to verify that this is the current version before use.