A-A-50908
June 14, 1985

COMMERCIAL ITEM DESCRIPTION

BOWL, PLASTIR OF PARIS MIXING

The General Services Administration has authorized the use of this commercial item description in preference to Federal Specification ZZ-P-616D.

This commercial item description covers dental mixing bowls.

Salient characteristics:

The mixing bowls shall be of the following sizes as specified:

Extra large
Large
Medium
Small

The mixing bowls shall be suitable for mixing dental gypsum products and alginate hydrocolloids.

The bowls shall be molded from flexible, vinyl elastomeric material, except as an alternate, the extra large bowl may be molded of a rubber compound. Bowls shall be of such design, strength, and flexibility as to provide a sturdy container for vigorous spatulations of alginates and dental gypsum materials without deteriorating. The bowls shall have surface release characteristics which would prevent dental materials, such as dental plaster, stone, and alginates, when mixed in the bowl, from adhering to its surface when the materials have hardened and set. Upon flexing the bowl, it shall form a pouring lip to expel the fluid material, such as gypsum products. The finish of the vinyl bowls shall be smooth and glossy, both inside and outside, except, the extra large bowl may only have a smooth finish. The color of the bowls shall be at the option of the contractor, provided each bowl is one uniform, solid color. Bowls shall be permanently and legibly molded on the outside of base with the name or trademark and size designation of the manufacturer or contractor.

When filled to 1/4 inch from the top, the bowls shall hold the following minimum milliliters of water:

Extra large	1550
Large	525
Medium	250
Small	100

Bowls shall conform to the shape shown in figure I and the dimensions listed in table I for the applicable size specified.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

BOWL, PLASTER OF PARIS MIXING

FIGURE 1

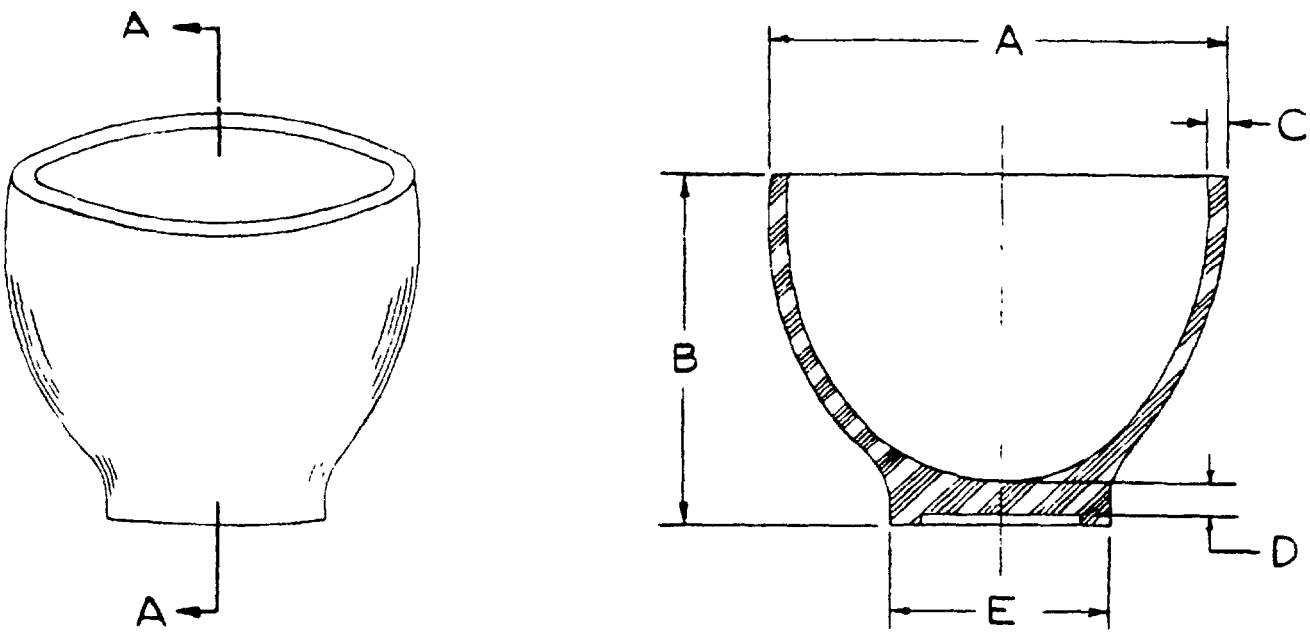


Table I. Dimensions (inches).

SPECIFICATION DESIGNATION SIZE	OUTSIDE DIA AT TOP A	OVERALL HEIGHT B	MIN THK OF SIDE C	MIN THK OF BASE D	OUTSIDE DIA OF BASE E
Extra Large	6-1/4 ± 1/4	6-1/8 ± 1/4	1/8	1/8	2-1/2 ± 1/8
Large	4-3/4 ± 1/4	3-3/4 ± 1/4	1/8	7/64	2-1/4+1/8,-1/4
Medium	4+3/8,-1/4	2-7/8 ± 1/4	3/32	1/8	2+9/64,-1/8
Small	3-1/4 ± 1/4	2-1/8 ± 1/4	3/32	1/8	1-3/4 ± 1/8

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

The specific gravity of the elastomeric material shall be 1.21 to 1.29 when tested in accordance with ASTM Test Method D-792-66R75. The density of the rubber material shall be 1.21 to 1.29 when tested in accordance with ASTM Test Method D-297-81.

The hardness (Durometer Shore A) of the elastomeric material or rubber material shall be 54 to 78 when tested in accordance with ASTM Test Method D-2240-81.

Workmanship. Bowls shall be free from blisters, cracks, voids, embedded foreign matter, or other defects which may impair their function.

Unit. Each (EA). Each bowl, of one size, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specifications where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Sampling for inspection. Sampling for inspection shall be conducted in accordance with MIL-STD-105. Where feasible, the same sample shall be used for the determination of two or more inspection characterisitics. The unit of product for inspection purposes shall be one bowl of each size. Unless otherwise specified, sampling for examination shall be conducted at inspection level II, AQL 2,5, and sampling for tests (when applicable) shall be conducted at inspection level S-1, AQL 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities, labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

6520-00-502-4750	Bowl, Plaster of Paris Mixing, Large
6520-00-502-5050	Bowl, Plaster of Paris Mixing, Medium
6520-00-502-5060	Bowl, Plaster of Paris Mixing, Small
6520-00-526-1602	Bowl, Plaster of Paris Mixing, Extra Large

Ordering Data Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

CIVIL AGENCY COORDINATING ACTIVITY
VA-OSS

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DOD-MB

AGENT:
DLA-DM

Project No. 6520-1734

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:48Z
Check the source to verify that this is the current version before use.