G-M-656a
AUGUST 12, 1958
SUPERSEDING
Fed. Spec. G-M-656
October 5, 1948

FEDERAL SPECIFICATION

MOUNTS, RADIOGRAPHIC FILM, DENTAL

This specification was approved by the Commissioner, Federal Supply Service, General Services Administration, for the use of all Federal agencies.

1. SCOPE AND CLASSIFICATION

1.1 Scope.—This specification covers open window, cardboard mounts, suitable for use in filing dental X-ray films.

1.2 Classification.

1.2.1 *Types.*—Film mounts shall be of the following types, as specified (see 6.1):

Type I.—14 window unit.

Type II.—18 window unit.

2. APPLICABLE SPECIFICATIONS AND STANDARDS

2.1 The following specifications and standards, of the issues in effect on date of invitation for bids, form a part of this specification:

Federal Specifications:

UU-P-31—Paper; General Specifications and Methods of Testing.

PPP-B-566 — Boxes, Folding, Paperboard.

PPP-B-585—Boxes, Wood, Wirebound.

PPP-B-601—Boxes, Wood, Cleated-Plywood.

PPP-B-621—Boxes, Wood, Nailed and Lock-Corner.

PPP-B-636—Boxes, Fiber.

PPP-B-676 — Boxes, Set-Up, Paperboard.

Federal Standards:

Fed. Std. No. 102—Preservation, Packaging, and Packing Levels.

(Activities outside the Federal Government may obtain copies of Federal Specifications, Standards, and Handbooks as outlined under General Information in the Index of Federal Specifications, Standards, and Handbooks and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U. S. Government Printing Office, Washington 25, D. C.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D. C.

(Federal Government activities may obtain copies of Federal Specifications, Standards, and Handbooks and the Index of Federal Specifications, Standards, and Handbooks from established distribution points in their agencies.)

Military Specifications:

MIL-B-10377—Box, Wood, Cleated, Veneer, Paper Overlaid.

MIL-L-10547 — Liners, Case, Waterproof.

Military Standards:

MIL-STD-105 — Sampling Procedures and Tables for Inspection by Attributes.

MIL-STD-129—Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:05Z
Check the source to verify that this is the current version before use.

(Copies of Military Specifications and Standards required by contractors in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

Veterans Administration Specification:

VA Gen. 224—General Specifications for Packings and Markings on Exterior Shipping Containers.

(Copies may be obtained from Veterans Administration, Catalog Division, Washington 25, D. C.)

3. REQUIREMENTS

3.1 Material.

3.1.1 *Paper stock.*—Unless otherwise specified, paper stock used in the fabrication of the dental mounts shall be either granite bristol or white tag. The physical requirements for the paper shall be as specified in table I and shall be capable of meeting the tests specified in 4.3.

3.1.2 *Glue.*—Glue shall be a strong, durable adhesive capable of holding layers of paper stock firmly together.

3.2 Design.

3.2.1 *Type I mount.*—Type I dental film mount shall have fourteen windows designed to hold films 1.25 by 1.625 inch, and shall be as shown in figure 1.

3.2.2 *Type II mount.*—Type II dental film mount shall have eighteen windows designed to hold films 1.25 by 1.625 inch, and shall be as specified in 3.4.

3.3 Construction.—Type I.

3.3.1 *Type I, 14 window unit.*—The construction of the type I dental film mount shall be as shown on figure 1, and as hereinafter specified. The dental film mount shall be constructed of paper stock consisting of either two layers of 0.015 inch each, or three layers of 0.010 inch each, resulting in a total thickness of 0.030 inch, with a tolerance of plus 0.003 minus 0, when glued. The windows shall be rectangular shaped with rounded corners and the marginal separations shall be securely glued together. The placement of the windows shall be as shown in figure 1. The front panel, shall be smooth throughout and all edges of the windows shall be even. In the back panel, both ends of each window shall be cut back, one end to permit easy insertion, and the other end to securely hold and permit full viewing of the film. The longitudinal sides shall be embossed to form a film sliding groove which will securely hold and permit full viewing of the film. The back panel shall be uniformly scored to form three sections when folded along the scored lines. The scoring shall be of such depth as to prevent breaks in the paper stock at the time of creasing.

3.3.2 *Marking.*

3.3.2.1 *Headings.*—Headings for the type I mounts shall be as specified in 3.4.2.1, or as shown in figure 1 (see 6.1).

3.3.2.2 *Windows.*—Imprinted below each window of the type I mount shall be the

TABLE I.—*Physical requirements*

Paper stock	Thickness of each layer	Basis weight pounds per 1000 sheets (sheet size — 22½ in. by 28½ in.)	Minimum bursting strength (pounds per square inch)
	Inches	*Pounds*	P.s.i.
Granite bristol	0.010	175	70
	0.015	250	105
White tag	0.010	186	75
	0.015	296	100

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:05Z
Check the source to verify that this is the currentversion before use.

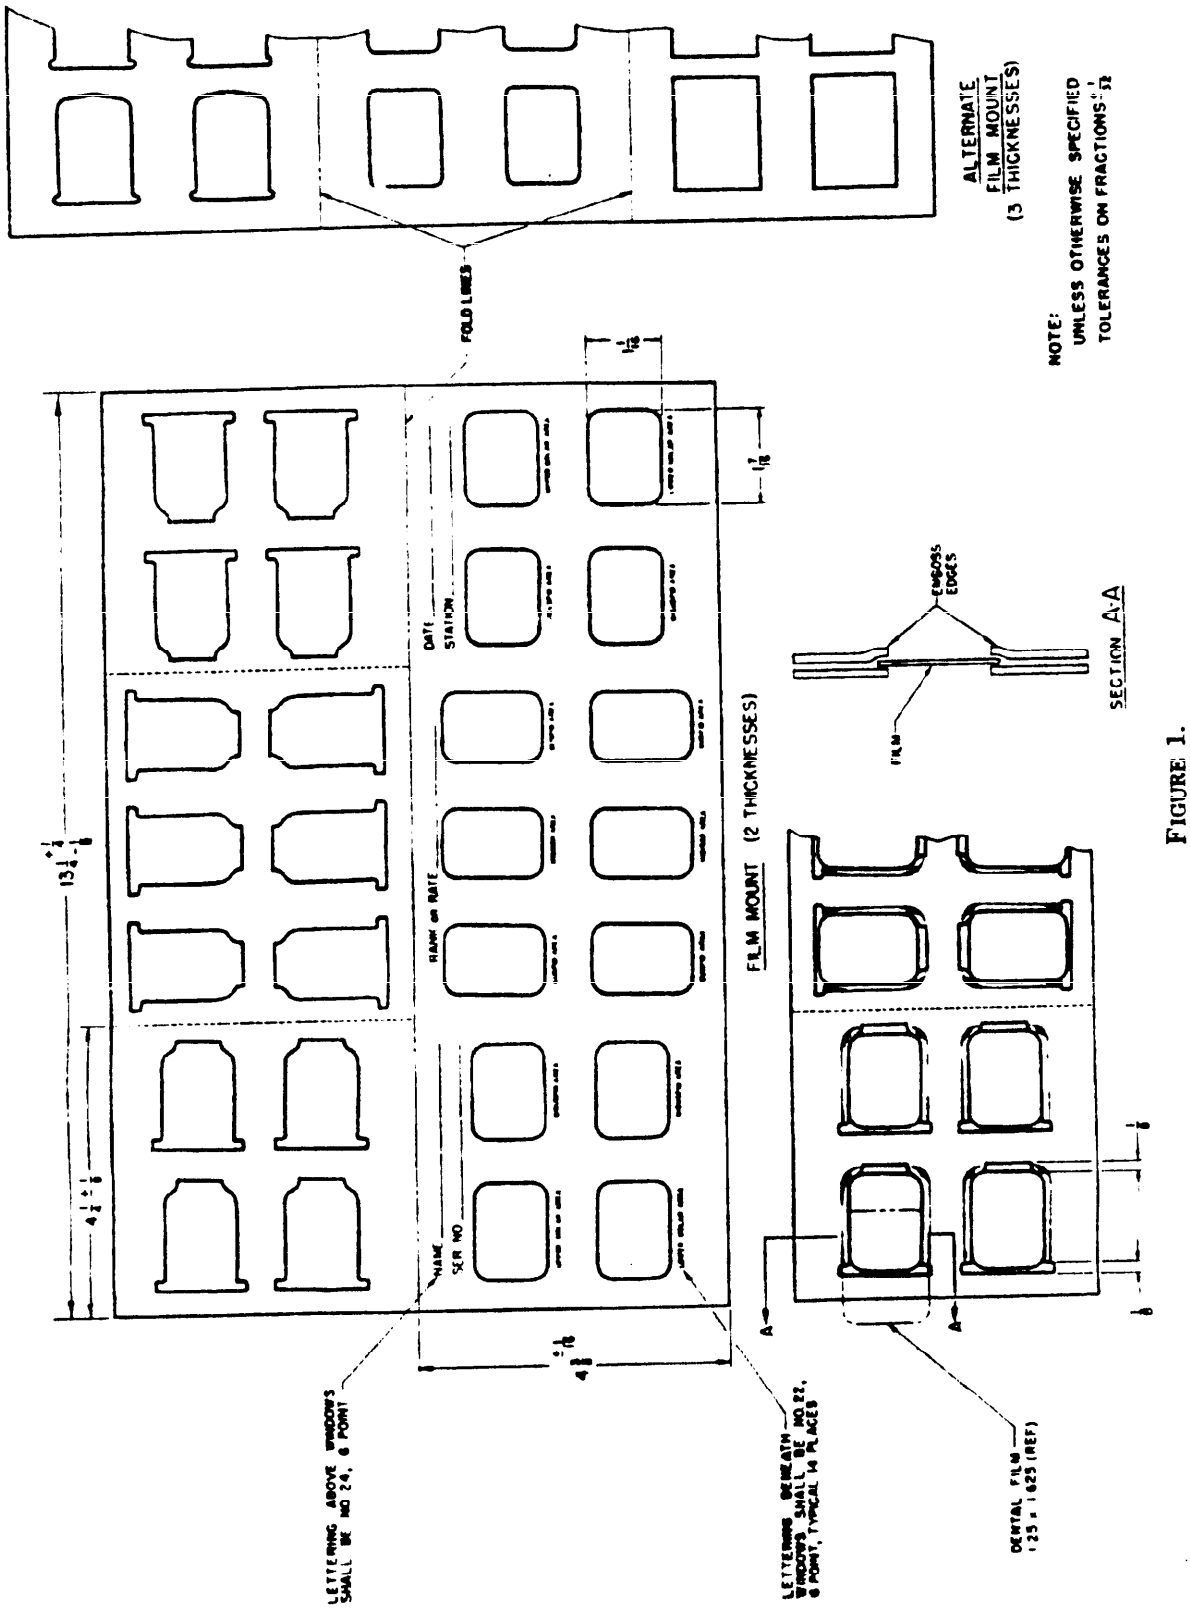


FIGURE 1.

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:05Z
Check the source to verify that this is the current version before use.

identification marking as shown in figure 1, in order that film may be readily identified.

3.4 **Construction.**—Type II.

3.4.1 *Type II, 18 window unit.*—Type II dental film mount shall consist of three thicknesses of paper stock for a total thickness of not less than 0.030 inch. The maximum overall dimensions of the dental mount shall be 13½ inches long by 5¾ inches wide. All windows shall be rectangular with rounded corners. The windows in the mount shall be arranged in three sections; left, middle, and right. The middle section shall have two horizontal rows of three windows each, with the long dimension of the window vertical. The left and right sections shall be provided with two vertical rows of three windows each, with the long dimension of the window horizontal. In the back member, both ends of each opening of the window shall be cut back approximately ⅛ inch; one end shall provide an opening for easy insertion of the film, and the other end shall securely hold the film to permit full viewing of the film. When the films are inserted in place, they shall not come free from the mount, when the mount is struck against a tabletop. The mount shall be scored on the back side in two places, 4¼ inches from each end (right and left), so that it may be folded. The scoring shall be of sufficient depth for easy folding and shall divide the mount into three sections.

3.4.2 *Marking.*—The size of the lettering for the type II mount shall be as indicated in figure 1.

3.4.2.1 *Heading.*—The type II mount shall be imprinted with a heading on each of the three sections (right, middle, and left), as follows:

Name ---------- Date ----------
C. No. ---------- X-ray No.-------
Station No. ----------

3.4.2.2 *Windows.*—Windows of the type II mounts shall be marked immediately below each window in the following manner: The windows of each row of the middle section shall be marked from left to right, as follows: "Cuspid Area", "Incisor Area", and "Cuspid Area". The windows of each row of the left section shall be marked as follows: Top row shall not be marked; middle row from left to right "Upper Molar Area", and "Bicuspid Area"; bottom row from left to right "Lower Molar Area" and "Bicuspid Area". The windows of the right section shall be marked as follows: Top row shall not be marked; middle row from left to right "Bicuspid Area" and "Upper Molar Area"; bottom row from left to right "Bicuspid Area" and "Lower Molar Area".

3.5 **Identification marking.**—Each mount shall be permanently marked with the name or registered trade-mark of the manufacturer.

3.5.1 *Identification marking for Military Medical Supply Agency procurement.* — In addition to the marking required in 3.5, each film mount shall be marked in the lower right-hand corner with a medical services symbol, as shown on figure 2.



FIGURE 2.—Medical services symbol.

3.6 **Workmanship.**—Workmanship shall be first class throughout. The film mounts shall be free from defects which detract from their appearance or may impair their serviceability.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:05Z
Check the source to verify that this is the current version before use.

4. SAMPLING, INSPECTION, AND TEST PROCEDURES

4.1 **Sampling.**—Sampling procedures shall be conducted in accordance with the procedures set forth in Military Standard MIL–STD–105.

4.1.2 *For tests.*

4.1.2.1 *Components.*—For Special Requirement 503 (see 4.2.1), sufficient material shall be extracted at random from each lot of paper stock received, prior to conversion, to prepare the number of specimens for each test as indicated in Federal Specification UU–P–31.

4.1.2.2 *End item.*—Sample size for Special Requirement 504 (see 4.2.1), shall be as indicated for inspection level L–2 in Appendix to Military Standard MIL–STD–105, and a minimum of five individual mounts shall be taken regardless of lot size.

4.2 **Inspection.**—The inspector shall ascertain that the film mounts have been examined and tested in accordance with specification requirements.

4.2.1 *Classification of defects.* — Film mounts shall be inspected in accordance with the following categories and defects. Unit of inspection shall be the individual mount, except where otherwise specified.

Categories and defects

Major *AQL 1.0 percent defective*

101. Mount windows fail to easily accommodate 1.25 by 1.625 dental film.
102. Mount layers not securely and completely glued.
103. Score lines for creasing not present in whole or part.
104. Thickness dimension of finished mount not within tolerance specified.
105. Mount not free of tears, cuts, holes or ruptures.

Minor A *AQL 2.5 percent defective*

201. Dimensions (except finished thickness) not as specified.
202. Mount and/or printing thereon not legible and free of defacing marks, scratches, or peeled areas.
203. Edges not clean cut or neatly and uniformly trimmed.
204. Identification marking, Medical Services Symbol and specified printed data not present in whole or part, or not legible.

Minor B *AQL 2.5 percent defective*

(Unit of Inspection—Package).

251. Labels or printing not free of defacing marks, scratches or tears.

*Special requirements**

501. Style, design, and construction shall be as set forth in figure 2 and specification.
502. Lettering size, printed and identification data on mount shall be as specified.
503. Paper stock shall be either granite bristol or white tag conforming to appropriate physical requirements set forth in table I.
504. When the mount is folded, the three (3) sections shall align squarely; creases at scored lines shall not break and folded ends shall lie flat without bulging when the sections are pressed into contact with each other.
505. Packaging and packing material shall be as specified.
506. Marking material shall be as specified.
507. Marking: Containers shall bear the information as specified.
508. Labeling shall bear the information as specified.

*Noncompliance with any one of the special requirements is cause for rejection.

Note.—Any defect not specifically covered above, but which adversely affects the appearance or serviceability of the amounts, shall be added to the above defects in the proper classification as determined by the inspector.

4.3 **Tests.**—Tests of paper stock shall be conducted in accordance with Federal Specification UU–P–31 for test methods as specified in table II.

TABLE II.—*Test methods*

Tests	Method Number
Basis weight	110
Bursting strength	112
Thickness	173

4.4 **Supplier responsibilities for inspection.**—The supplier shall perform examinations

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:05Z
Check the source to verify that this is the current version before use.

and tests set forth in this specification to substantiate conformance of supplies to specification requirements. The examinations and tests shall be at the expense of the supplier. Suppliers shall have adequate test facilities or shall arrange for test facilities acceptable to the Government to be used for executing specific prescribed tests. Records of examinations and tests performed by the supplier shall be maintained by the supplier and made available to the Government upon the Government's request, at any time, or from time to time for a period of 2 years after the delivery of the supplies to which these records relate. The supplier shall be responsible for compliance with all requirements of this specification, and all other technical requirements of the contract.

5. PREPARATION FOR DELIVERY

The levels of preservation, packaging and packing protection used are defined in Federal Standard No. 102 (for civil agencies only).

5.1 Packaging.

5.1.1 *Unit of issue.*—Twenty-five mounts, as specified, constitute one unit of issue.

5.1.2 *Packaging quantities.*—The number of units of issue indicated in table III shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in procurement document.

5.1.2.1 **Packing variation permitted.** — If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which will insure safe delivery to destination.

5.1.3 *Level A.*

5.1.3.1 *Unit package.*—Each unit shall be adequately protected with cardboard and completely wrapped in kraft paper of not less than 30 pounds basis weight (500 sheets 24 by 36 inches), or equal, and securely taped with kraft gummed paper tape to prevent accidental opening, or each unit shall be packaged in a carton or box of appropriate size conforming to the requirements of Federal Specification PPP–B–566 or PPP–B–676. Carton shall be adequately secured to prevent accidental opening.

5.1.3.2 *Intermediate package.*—Intermediate package shall be a carton of appropriate size constructed in accordance with Federal Specification PPP–B–636 or PPP–B–676. Carton shall be adequately secured to prevent accidental opening.

5.1.4 *Level C.*—One unit (25 mounts) shall be packaged in a set-up paperboard carton of suitable size and design and wrapped in heavy weight kraft paper, ends neatly folded and securely fastened by use of gummed tape.

5.2 Packing.

5.2.1 *Level A.*

5.2.1.1 *Exterior container.*—Exterior container shall be designed for type 2 load and

TABLE III.—*Packaging quantities*

Stock No.	Type	Unit package	Intermediate package	Shipping container
6525–611–0000	I	1 unit	12 units	96 units
6525–611–0025	I	1 unit	not required	40 units
6525–611–0005	II	1 unit	not required	40 units

Source: https://assist.dla.mil -- Downloaded: 202610-26T11:05Z
Check the source to verify that this is the current version before use.

constructed in accordance with Federal Specification PPP–B–585, style 3, for class 3 use; PPP–B–601, table II, using type III, class 1 plywood; PPP–B–621, table III; or Military Specification MIL–B–10377, table II.

5.2.1.2 *Case liner.*—Each level A box shall be lined with a waterproof case liner conforming to Military Specification MIL–L–10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto.

5.2.1.3 *Strapping.* — Strapping, when required, shall be in accordance with applicable box specification.

Note.—Strapping will not be required for shipment forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 *Level B.*

5.2.2.1 *Exterior container.*—Exterior container shall conform to Federal Specification PPP–B–601, table I, using type III, class 1 plywood, or shall be designed for type 2 load and constructed in accordance with Federal Specification PPP–B–585, style 3 for class 2 use; PPP–B–621, table I; or Military Specification MIL–B–10377, table I.

5.2.1.3 *Level C.*

5.2.1.3.1 *Stock No. 6525–611–0000.* — Unless otherwise specified, the subject commodity shall be packed in substantial commercial containers, of the type, size and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.2.1.3.2 *Stock No. 6525–611–0025 or 6525–611–0005.*—Unless otherwise specified, forty unit packages shall be packed in a new shipping container. Shipping containers shall comply with applicable rules in latest issue of Uniform Freight Classification to insure acceptance by common or other carrier for safe transportation at lowest rate to destination.

5.3 **Marking.**

5.3.1 *For military agencies.*

5.3.1.1 *Interior packages.*—Each unit package and each intermediate package shall be marked in accordance with section 5 of Military Standard MIL–STD–129.

5.3.1.2 *Shipping container.*—Shipping container shall be marked in accordance with Military Standard MIL–STD–129. Service color and service symbol markings are required only on direct shipments from the contractor's plant to overseas activities.

5.3.2 *For civil agencies.*

5.3.2.1 *Unit cartons.* — Unless otherwise specified, unit cartons or packages shall be marked with the Veterans Administration stock number, nomenclature, quantity, and name of manufacturer.

5.3.2.2 *Shipping containers.*—Unless otherwise specified, shipping containers shall be marked in accordance with Veterans Administration Specification VA Gen. 224 "General Specifications for Packing and Markings on Exterior Shipping Containers", of the issue in effect on date of invitation for bids.

6. NOTES

6.1 **Ordering data.** — Purchasers should exercise any desired options offered herein, and procurement documents should specify the following:

(*a*) Title, number and date of this specification.
(*b*) Type required (see 1.2.1).
(*c*) Material required, if other than specified (see 3.1.1).
(*d*) Heading required for type I (see 3.3.2.1).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:05Z
Check the source to verify that this is the current version before use.

(*e*) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

(*f*) Marking, if other than specified (see 5.3.2).

6.2 This specification covers the following item appearing in the Armed Services Medical Stock List:

6525–611–0000 MOUNT, RADIOGRAPHIC FILM, DENTAL, 14 Film, 25s.

6.3 This specification does not include all types, classes, grades, sizes, etc., of the commodity indicated by the title of this specification or which are commercially available, but is intended to cover the types, etc., which are normally procured to meet Federal Government requirements.

6.4 **Transportation description.**—Transportation description applicable to this item is:

Photographic Materials, NOIBN

Carload minimum weight 20,000 pounds, subject to Rule 34, Uniform Freight Classification

Motor Volume minimum weight 20,000 pounds.

Notice. — When Government drawings, specification, or other data are used for any purpose other than in connection with a definitely related Government procurement operation, the United States Government thereby incurs no responsibility nor any obligation whatsoever; and the fact that the Government may have formulated, furnished, or in any way supplied the said drawings, specifications, or other data, is not to be regarded by implication or otherwise as in any manner licensing the holder or any other person or corporation, or conveying any rights or permission to manufacture, use, or sell any patented invention that may in any way be related thereto.

MILITARY INTERESTS:

Army—M
Navy—Md
Air Force.

Copies of this specification may be purchased for 5 cents each.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:05Z
Check the source to verify that this is the current version before use.