H-B-00248b(DSA-DM)
10 August 1967
INTERIM REVISION OF
Fed. Spec. H-B-248a
18 December 1958

INTERIM FEDERAL SPECIFICATION

BRUSH, SCRATCH, DENTAL

This interim Federal specification was developed by the Defense Personnel Support Center, 2800 South 20th Street, Philadelphia, Pennsylvania 19101, based upon currently available technical information. It is recommended that Federal agencies use it in procurement and forward recommendations for changes to the preparing activity at the address shown above. The General Services Administration has authorized the use of this interim Federal specification as a valid exception to Federal Specification H-B-248a.

1. SCOPE

1.1 Scope. This specification covers a flexible steel wire scratch brush suitable for dental use.

2. APPLICABLE DOCUMENTS

2.1 The following specifications and standards, of the issue in effect on date of invitation for bids or request for proposal, form a part of this specification to the extent specified herein:

SPECIFICATION

Federal

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Box, Setup.

FSC 6520

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

STANDARDS

Federal

FED-STD-66	Steel: Chemical Composition and Hardenability.
FED-STD-123	Marking for Domestic Shipment (Civilian Agencies).

(Activities outside the Federal Government may obtain copies of Federal Specifications and Standards as outlined under General Information in the Index of Federal Specifications and Standards and at the prices indicated in the Index. The Index, which includes cumulative monthly supplements as issued, is for sale on a subscription basis by the Superintendent of Documents, U.S. Government Printing Office, Washington, D.C. 20402.

(Single copies of this specification and other product specifications required by activities outside the Federal Government for bidding purposes are available without charge at the General Services Administration Regional Offices in Boston, New York, Atlanta, Chicago, Kansas City, Mo., Dallas, Denver, San Francisco, Los Angeles, Seattle, and Washington, D.C.

(Federal Government activities may obtain copies of Federal Specifications and Standards and the Index of Federal Specifications and Standards from established distribution points in their agencies.)

SPECIFICATIONS

Military

MIL-P-116	Preservation, Methods Of.
MIL-L-10547	Liners, Case, and Sheet, Overwrap; Water-Vaporproof, or Waterproof, Flexible.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

(Copies of Military specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. Material shall be as herein specified and suitable for the purpose intended.

3.1.1 Wires. Wires shall be fabricated from drawn, flexible, AISI 1022 carbon steel conforming in chemical composition to the requirements of FED-STD-66. The wires shall be rendered rust-retardant by a suitable galvanized coating.

3.1.2 Tubing. Tubing shall be made of clear cellulose acetate butyrate plastic.

3.2 Style, design, and dimensions. The scratch brush shall be suitable for cleaning dental burs, files, and instruments. The brush shall consist of a bundle of the wires specified in 3.1.1, bent double and fitted securely into the tubing specified in 3.1.2. A sufficient number of the wires shall be included in the bundle, so that the composite diameter of the wires is not less than 1/4 inch when the wires are bent double and squeezed together for insertion into the tubing. The bent end of the wires shall not protrude from the tubing by more than 1/16 inch. The free ends of the wires shall be trimmed uniformly, and there shall be no stray or improperly fitted wires. The edge of the proximal end of the plastic tubing shall be clean-cut, and the distal end shall be free of sharp projections. The tubing shall serve as a suitable hand-grip. Tubing shall be trimmable with a dental laboratory knife, exposing fresh metal surface as the wires wear down. Style, design, and dimensions of the brush shall be in accordance with figure 1.

3.3 Workmanship. Workmanship shall be first class throughout. Scratch brushes shall be free from defects which detract from their appearance or may impair their serviceability. Tubing shall be free from nicks, cuts, and tears.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

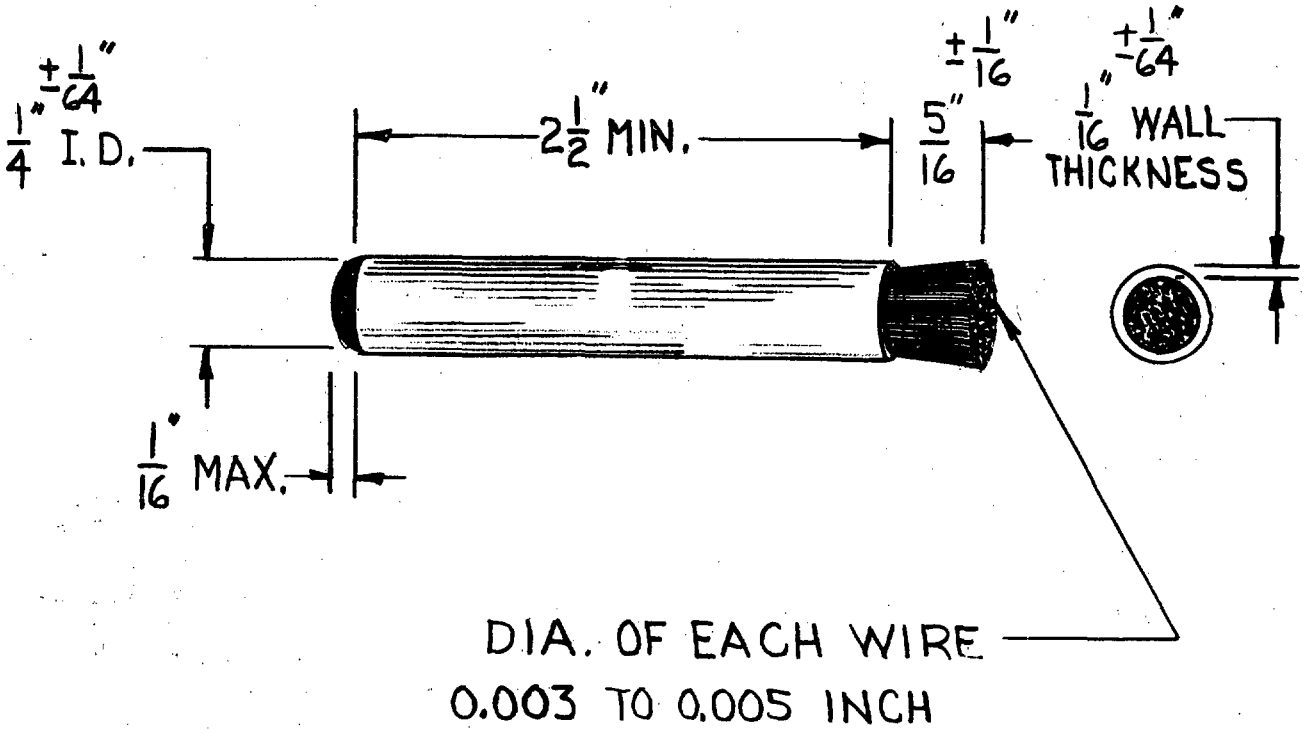


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified, the supplier may utilize his own facilities or any commercial laboratory acceptable to the Government. The Government reserves the right to perform any of the inspections set forth in this specification, where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. When available, certificates of quality, supplied by the manufacturer of the component or material, listing the specified test method and test results obtained, may be furnished in lieu of actual performance of such testing by the contractor.

4.2 Sampling.

4.2.1 For examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in table I.

Table I. Examination Criteria

Type of examination	Inspection level	AQL (percent defective)
Classification of defects:		
Major	II	1.0
Minor	II	4.0
Dimensional examination	S-3	2.5

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

4.2.2 For tests. Sufficient quantity of the raw material from each lot or batch number shall be selected for chemical analysis.

4.3 Examination. The brushes shall be examined to determine compliance with specification requirements.

4.3.1 Classification of defects. Examination shall be conducted in accordance with the classification of defects specified in table II. Examination shall not be restricted to the possible defects listed herein.

Table II. Classification of Defects

Category	Defect
Major:	
101	Wires not securely fitted into tubing.
102	Tubing not free of nicks, cuts, or tears.
103	Edge of proximal end of tubing not clean-cut.
104	Tubing-supported section of brush not rigid.
105	Tubing not trimmable.
106	Wires brittle or not flexible.
107	Wires not coated with rust-retardant material.
108	Style and design not as specified.
Minor:	
201	Free wire ends of brush not trimmed uniformly.
202	Brush not free of stray or improperly fitted wires.
203	Tubing not clear.
204	Edge of distal end of tubing not free of sharp projections.
205	Packing not as specified.
206	Packaging not as specified.
207	Marking not as specified.

4.3.2 Dimensional examination. The brushes shall be examined for dimensional defects. Any dimension not within the tolerances specified in figure 1 shall be classified a dimensional defect.

4.4 Tests. Tests shall be conducted as necessary to determine compliance with the requirements of this specification.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One brush, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table III shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table III. Packaging quantities

Unit package	Intermediate package	Exterior container
Not required	24 units	1152 units

5.1.2.1 Packing variation permitted. If the required number of units to be shipped is less than the number of units specified to be overpacked in an exterior container, such units shall be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Cleaning and drying. Each unit shall be thoroughly cleaned and dried in accordance with the applicable method as outlined in MIL-P-116.

5.1.3.2 Preservative. Not required.

5.1.3.3 Intermediate package. Intermediate package shall be a box of appropriate size constructed in accordance with PPP-B-566 or PPP-B-676, except commercial colors will be acceptable. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 3 use; PPP-B-601, table II, using type I, class 1 plywood; PPP-B-621, table III; or PPP-B-636, type CF, class weather-resistant.

5.2.1.2 Case liner. Each level A wood box shall be lined with a waterproof case liner conforming to MIL-L-10547. Closure and sealing shall conform to applicable paragraphs of appendix thereto. Case liner shall not be required for fiberboard boxes.

5.2.1.3 Closure. Closure of wood boxes shall be in accordance with appendix of applicable box specification. Closure of each fiberboard box shall be as specified in the appendix, and waterproofing shall conform with 30.4 of PPP-B-636.

5.2.1.4 Strapping. Strapping, when required, shall be in accordance with appendix of applicable box specification.

NOTE: Strapping shall not be required for shipments forwarded to a receiving activity within the continental limits of the United States for storage and redistribution.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall conform to PPP-B-601, table I, using type III, class 1 plywood; or shall be designed for type 2 load, and constructed in accordance with PPP-B-585, style 3, for class 2 use; PPP-B-621, table I; or PPP-B-636, type CF, class domestic and method I closure shall be utilized.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Civil agencies. Shipments shall be marked in accordance with FED-STD-123.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

5.3.2 Military agencies.

5.3.2.1 Interior packages. Each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES.

6.1 Ordering data. Procurement documents should specify the following:

(a) Number and date of this specification.

(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

6.2 This specification does not cover all types, classes, grades, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the types which are normally procured to meet Federal Government requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or serve to amend contractual requirements .

SPECIFICATION: H-B-00248b(DSA-DM)

ORGANIZATION

CITY AND STATE

CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

A. GIVE PARAGRAPH NUMBER AND WORDING.

B. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THE SPECIFICATION RESTRICTIVE?

☐ YES ☐ NO *(If "yes", in what way?)*

4. REMARKS *(Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)*

SUBMITTED BY *(Printed or typed name and activity - Optional)*

DATE

DD FORM 1 JAN 66 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T11:06Z
Check the source to verify that this is the current version before use.