A-A-51758
28 November 1986

COMMERCIAL ITEM DESCRIPTION

CANNULA, EAR, (Baron)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers curved Baron ear cannula for use during surgical procedures.

Salient characteristics:

Material. The Baron ear cannula shall be fabricated from class 3 austenitic stainless steel or class 4 martensitic stainless steel in accordance with ASTM F899.

Hardness. Cannula fabricated from austenitic stainless steel shall have a Rockwell hardness of B-75 to B-110. Cannula fabricated from martensitic stainless steel shall have a Rockwell hardness of C-46 to C-53. The cannula shall be tested for hardness in accordance with ASTM E18, or ASTM E92 and E140.

Finish. The finish shall be satin or mirror in accordance with Federal Specification GG-I-526.

Passivation. The cannula shall be properly passivated.

Corrosion-resistance. The cannula shall meet the boil test requirements as specified in GG-I-526. Should the cannula be fabricated from martensitic steel, it shall meet the copper sulfate test requirements of GG-I-526.

Style and design. The cannula shall have a finger tip control on the shaft. At the proximal end, the cannula shall have an enlarged section suitable for connection of tubing. Both the finger device and the tube connector shall be brazed onto the cannula shaft. The bypass hole on the finger device shall have the same cross sectional area as the inside of the cannula shaft. The ear cannula shall meet the dimensional requirements specified in Figure 1.

Marking. Cannula shall bear the name or registered trademark of the manufacturer, the word "stainless" and the french size. Instruments of foreign manufacture shall bear the name of the country of manufacture.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Workmanship. The cannula shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (Ea). One cannula, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for Tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one cannula. AQL shall be 1.0 percent defective. Inspection level shall be S-2.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:00Z
Check the source to verify that this is the currentversion before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-781-5563	CANNULA, EAR, BARON, Curved, 5 Fr
6515-01-113-2650	CANNULA, EAR, BARON, Curved, 7 Fr
6515-01-113-2651	CANNULA, EAR, BARON, Curved, 3 Fr

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:00Z
Check the source to verify that this is the current version before use.

COMMERCIAL ITEM DESCRIPTION A-A-51758

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MDQAS

Project No. 6515-3707

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:00Z
Check the source to verify that this is the current version before use.

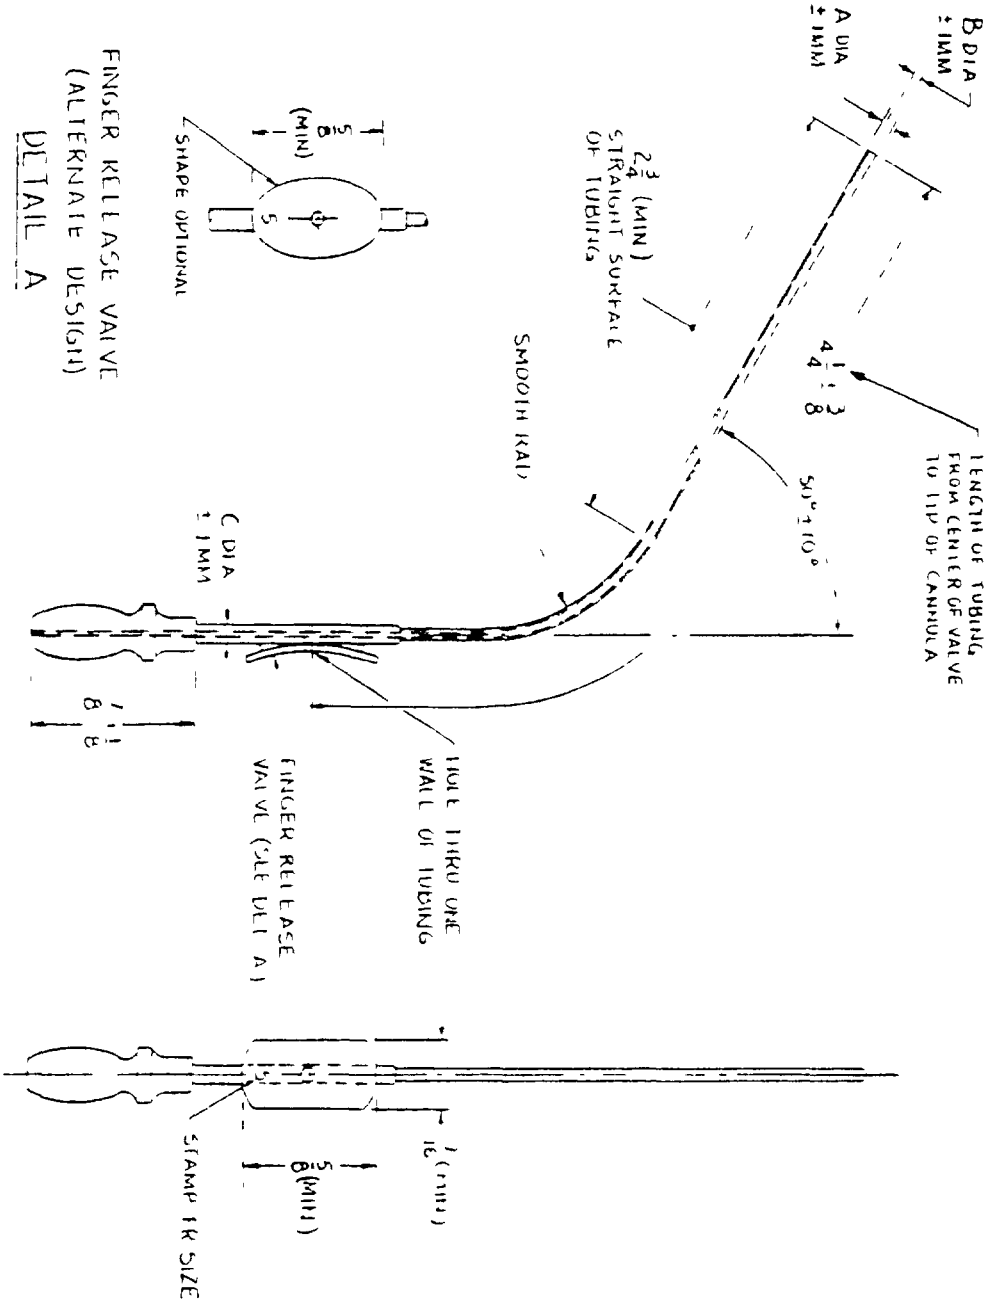

NSN	A (FR)	B MM	C (FR)
6515 00-181-5563	5	.0019	7
6515 01 113 2651	7	.0028	7
6515 01-113-2651	3	.0010	5

NOTE
UNLESS OTHERWISE SPECIFIED ALL DIMENSIONS ARE IN INCHES

FIGURE 1 CANNULA, EAR, BARON, CURVED

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:00Z
Check the source to verify that this is the current version before use.