A-A-51763
2 December 1986

COMMERCIAL ITEM DESCRIPTION

CANNULA, EAR (Rosen)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers various sized Rosen ear cannulae.

Salient characteristics:

The cannula shall be a suction tube, with Luer fitting and obturator, suitable for use in surgical procedures of the middle ear.

Cannula tube. The cannula shall be of the Rosen design consisting of a curved tube permanently attached at the proximal end to a Luer fitting as shown in Figure 1. Overall length of the cannula tube, exclusive of Luer fitting, shall be 3-3/8 ± 1/8 inches.

Luer fitting. The Luer fitting shall be the female lock type specified in ANSI/HIMA MD70.1.

Obturator. The obturator shall have a finger handle and pass completely through the cannula and Luer fitting.

Material. The cannula shall be fabricated of an austenitic corrosion-resistant steel in accordance with ASTM F899. The cannula shall have a hardness of Rockwell B-75 minimum. The hub shall be fabricated of a suitable corrosion-resistant alloy.

Identification markings. The Luer fitting shall bear the manufacturer's name or registered trademark, and the gage of the cannula.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-04-26T09:00Z
Check the source to verify that this is the current version before use.

Sizes. Cannulae shall be of the following sizes, as specified.

Type	Size (gage)
1	14
2	16
3	17
4	20
5	22
6	24

Workmanship. The cannula shall be free from defects which detract from its appearance or impair its serviceability. The surface of the cannula shall be smooth and the lumen void of obstructions.

Unit. Each (EA). One cannula, of the size specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics. The Luer fitting shall be tested for dimensions and performance in accordance with ANSI/HIMA MD70.1. The cannula shall be tested for hardness in accordance with ASTM E18 or ASTM E92 and E140.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one cannula. Inspection level shall be S-1 and acceptance number zero.

Certificates of quality. Certificates of quality, supplied by the manufacturer of the materials, may be furnished in lieu of actual performance of composition testing by the contractor, provided lot identity has been maintained and can be demonstrated by the Government. The certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the NSN, the item identification, the name of the component/material, the lot number, the lot size, the test method, and the test results.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:00Z
Check the source to verify that this is the currentversion before use.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-00-104-8650	CANNULA, EAR, Rosen, 14 Gage, 3-3/8 Inch With Obturator
6515-01-114-1532	CANNULA, EAR, Rosen, 16 Gage, 3-3/8 Inch With Obturator
6515-00-781-5555	CANNULA, EAR, Rosen, 17 Gage, 3-3/8 Inch With Obturator
6515-00-781-5548	CANNULA, EAR, Rosen, 20 Gage, 3-3/8 Inch With Obturator
6515-00-781-5474	CANNULA, EAR, Rosen, 22 Gage, 3-3/8 Inch With Obturator
6515-00-104-8651	CANNULA, EAR, Rosen, 24 Gage, 3-3/8 Inch With Obturator

Ordering data. (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-3773

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:00Z
Check the source to verify that this is the current version before use.

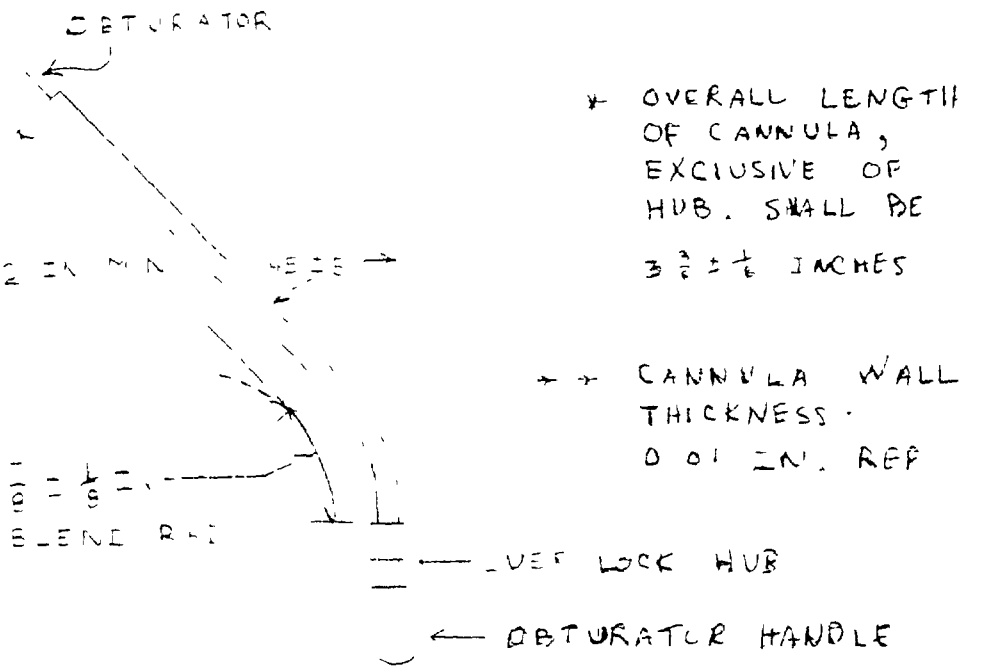


FIGURE 1: CANNULA. EAR, ROSEN,

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.