A-A-51764A
5 May 1988
SUPERSEDING
A-A-0051764(DM)
23 January 1987

COMMERCIAL ITEM DESCRIPTION

FORCEPS, DRESSING (Adson)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers Adson dressing forceps suitable for use in general surgical procedures.

Salient characteristics:

General. The forceps shall be an Adson style dressing forceps having serrated jaws and crosswise grooves or serrations on the handle. The tip shall be aligned to provide a precise meeting of the points.

Material. The dressing forceps shall be manufactured from Class 4 martensitic corrosion-resisting steel as specified in American Society for Testing and Materials (ASTM) Designation F899.

Hardness. The complete instrument shall be properly passivated and shall have a Rockwell Hardness C Scale (HRC) of 40 to 45 at the jaws. The hardness shall be tested in accordance with ASTM Designation E18 or ASTM Designations E92 and E140.

Style, design and dimension. Style, design and dimension of the forceps shall comply with Figure 1.

Finish. The forceps shall have a satin, mirror or matte finish and shall be free from grind or tool marks.

Markings. The forceps shall bear the contractor's name or registered trademark and the word "stainless." Forceps of foreign manufacture shall bear the name of the country of manufacture.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Resistance to corrosion. The forceps shall show no evidence of corrosion as specified in ASTM Designation F1089.

Forceps performance test. The forceps shall have no misalignment of the tips in closing. Upon closing, serrations on the tips which do not interdigitate shall be rejected.

Workmanship. The forceps shall be free from defects which detract from its appearance or impair its serviceability. The forceps shall be without rough edges, burrs, cracks, pits, dents and corrosion.

Unit. Each (EA). One forceps, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Examination. The forceps shall be examined to determine compliance with specification requirements. Sampling shall be in accordance with MIL-STD-105, sampling level II, AQL 2.5.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one forceps. Sampling shall be at an inspection level of S-2 with an AQL of 1.0.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-139-8285	FORCEPS, DRESSING, ADSON, 5 Inch (12 cm) Long

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 59149

Project No. 6515-4275

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.

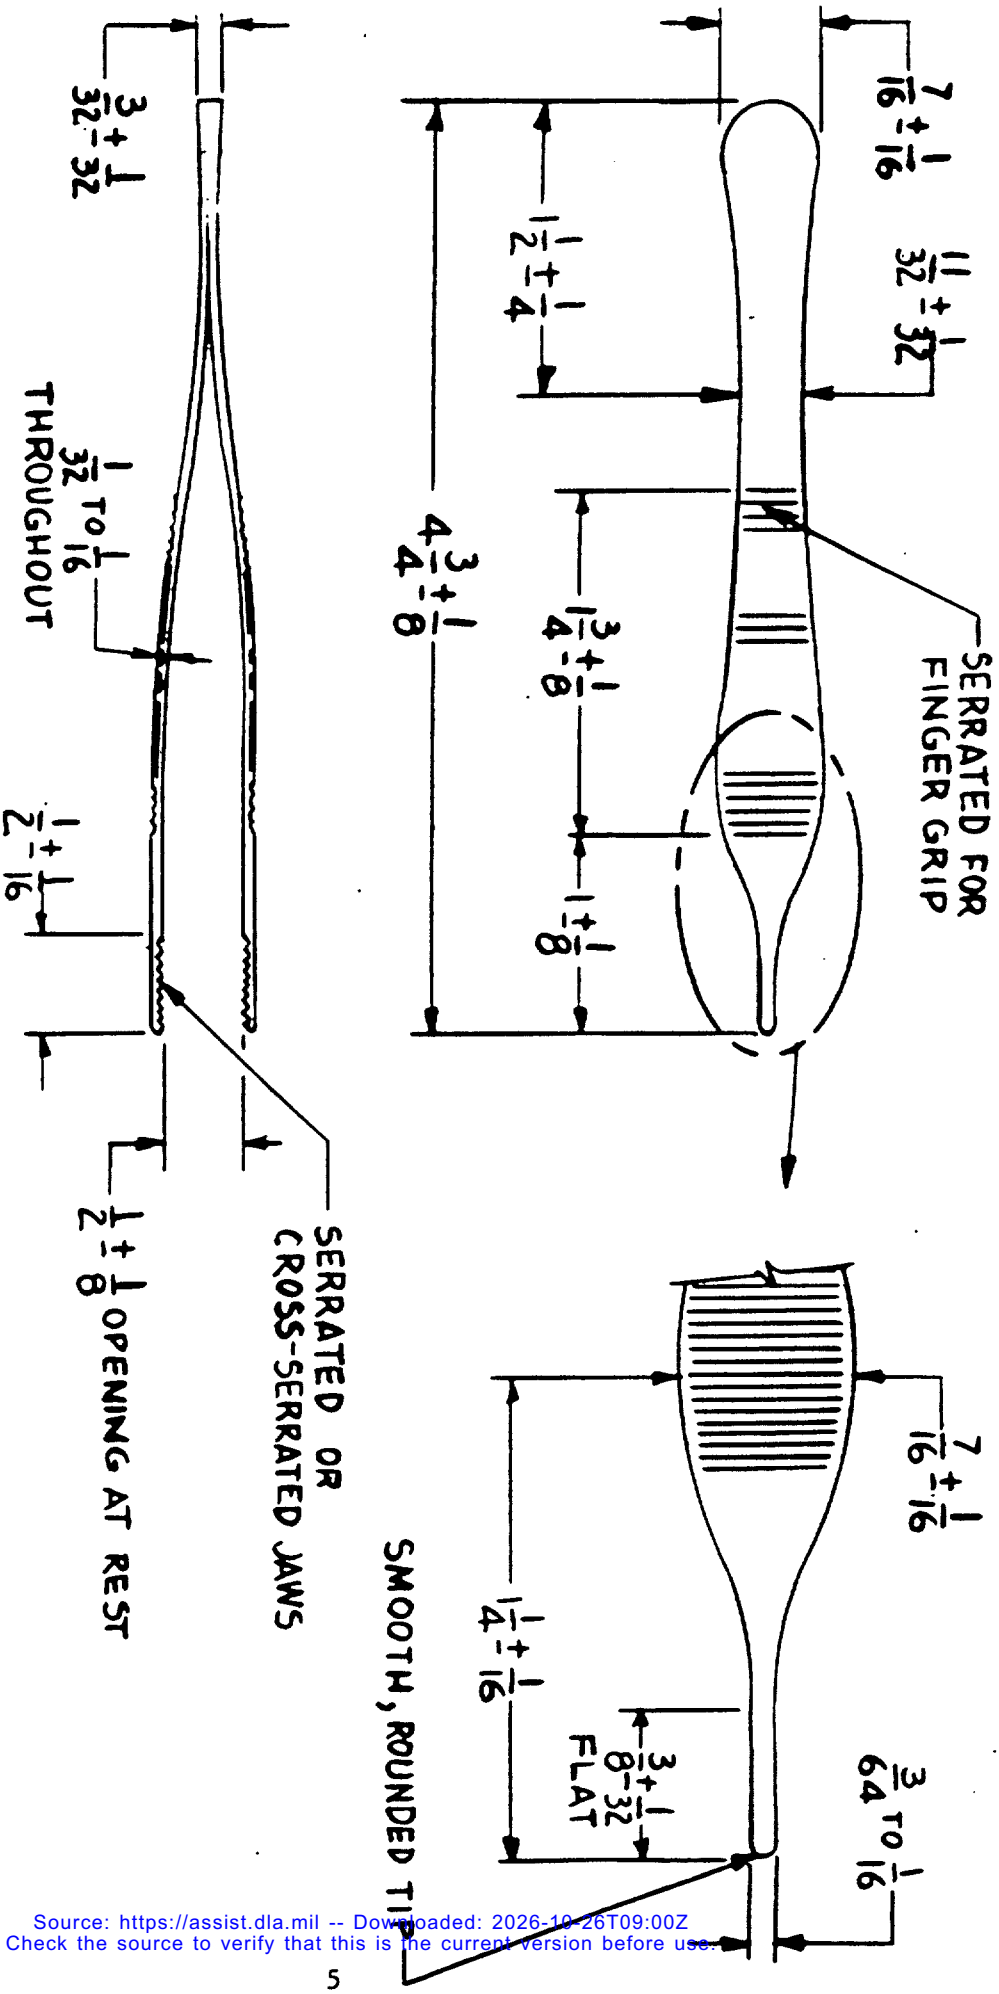


FIGURE 1. FORCEPS, DRESSING, ADSON

NOTE: DIMENSIONS ARE IN INCHES

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:00Z
Check the source to verify that this is the current version before use.