A-A-51781A
6 June 1989
SUPERSEDING
A-A-0051781 (DM)
12 February 1987

COMMERCIAL ITEM DESCRIPTION

HOOK, TISSUE, DOUBLE PRONG (Joseph)

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers four sizes of double-prong Joseph tissue hook for use during surgical procedures.

Salient characteristics:

General. Tissue hooks shall be sharp, of the Joseph design, double-pronged and designed for holding, elevating or exerting traction on a tissue during surgical procedures.

Material. Tissue hooks shall be fabricated from Class 4 martensitic corrosion-resistant steel in accordance with American Society for Testing and Materials (ASTM) Designation F899.

Hardness. Tissue hooks shall have a Rockwell Hardness C Scale (HRC) of 48 to 53 when tested in accordance with ASTM Designation E18 or E92 whichever is applicable. Conversion of hardness values shall be tested in accordance with ASTM Designation E140.

Style and design. Tissue hooks shall be either size 2,5,7,or 10mm and have a sharp double-prong hook with the style and dimensions in accordance with Figure 1. The handle shall be knurled or fluted.

Finish. The finish of the tissue hooks shall be satin or mirror.

Passivation. Tissue hooks shall be properly passivated.

Identification marking and labeling. Tissue hooks shall be marked with the name or registered trademark of the contractor and the work "stainless". If the tissue hooks are of foreign manufacture, the instrument shall bear the name of the country of manufacture.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Corrosion resistance. Tissue hooks shall show no signs of corrosion when tested in accordance with ASTM Designation F1089.

Workmanship. Tissue hooks shall be uniform and free from cracks, pits, burrs, sharp edges, scale rough areas, corrosiuon, grind or tool marks, and dirt or polishing materials.

PRODUCT QUALITY LEVEL

Visual and dimensional examination. Shall be examined to verify that the design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements specified.

Unit. Each (Ea). One hook, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105 and as specified herein. Unit of product for examination purpose shall be one forceps. Sampling shall be inspection level II with an acceptable quality level (AQL) of 1.0.

Examination. Examination shall be conducted to determine compliance with the specification requirements.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one tissue hook. AQL shall be 1.0 percent defective. Inspection level shall be S-2.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580, as amended and as implemented by Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-110-1373	Hook, Tissue, Double-Prong, Joseph, 5 mm
6515-01-110-1378	Hook, Tissue, Double-Prong, Joseph, 10 mm
6515-01-110-1379	Hook, Tissue, Double-Prong, Joseph, 7 mm
6515-01-110-1380	Hook, Tissue, Double-Prong, Joseph, 2 mm

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4582

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.

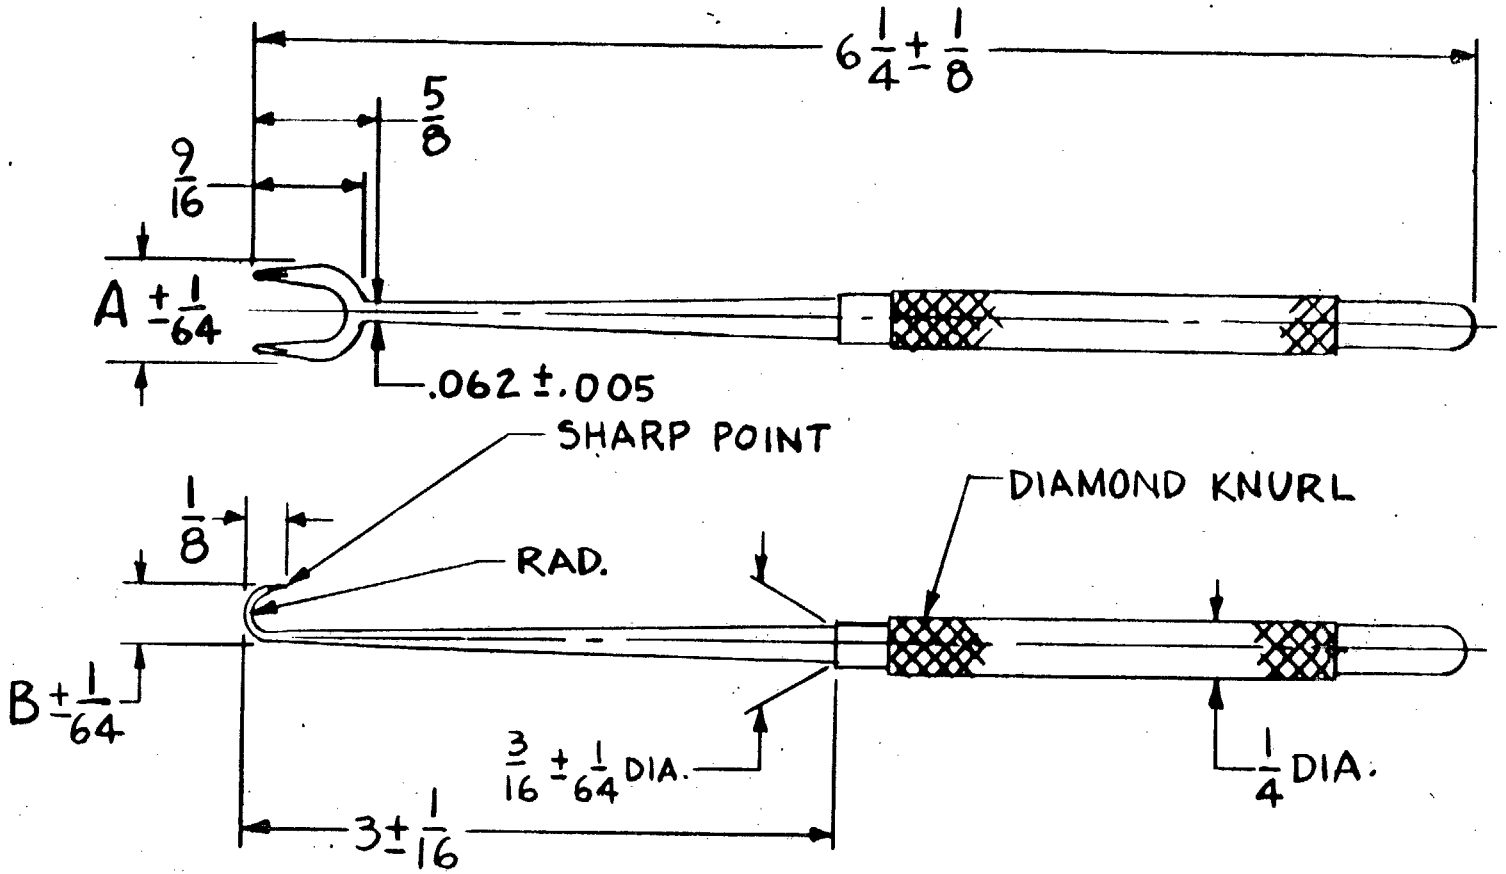

SIZE	NSN	A	B
5 MM	6515-01-110-1373	1/4	3/16
10MM	6515-01-110-1378	7/16	1/4
7 MM	6515-01-110-1379	11/32	7/32
2 MM	6515-01-110-1380	11/64	3/16

NOTE:

FRACTIONAL TOLERANCES ± 1/32 UNLESS OTHERWISE SPECIFIED.

ALL DIMENTIONS ARE IN INCHES UNLESS OTHERWISE SPECIFIED.

FIGURE 1 HOOK, TISSUE, DOUBLE PRONG, JOSEPH

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:01Z
Check the source to verify that this is the current version before use.