A-A-0053014(DM)
8 September 1987

INTERIM COMMERCIAL ITEM DESCRIPTION

SPREADER, BONE, PEDIATRIC (Baby Inge)

The General Services Administration has authorized the use of this interim commercial item description which was developed by the Defense Personnel Support Center, Directorate of Medical Materiel, DPSC-RST, 2800 South 20th Street, Philadelphia, PA, 19101, based upon currently available technical information.

This interim commercial item description covers a pediatric bone spreader of the Baby Inge style, used for pediatric thoracolumbar spinal, hand, knee, or ankle procedures.

Salient characteristics.

General. The definitions of the terms and components used in this specification are in accordance with ASTM F921.

Material. The material of the bone spreader shall be Class 4 martensitic corrosion-resistant steel in accordance with ASTM F899.

Hardness. The Rockwell hardness of the bone spreader shall be C48 to C53.

Style, design and dimensions. The bone spreader shall have an overall length of 6-1/8 inches with a maximum jaw opening of 1-1/4 inches. The jaw teeth shall be non-cutting. The ratchet-style handle shall be self-retaining. The bone spreader shall be in accordance with Figure 1.

Finish. The finish of the bone spreader shall be mirror, satin, or matte. The matte finish shall exhibit a uniform, non-directional surface texture equivalent to that produced by lightly blasting the prepared surface with fine abrasives under pressure.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:14Z
Check the source to verify that this is the current version before use.

Corrosion-resistance. The bone spreader shall show no signs of corrosion or plating of copper when tested for corrosion resistance as specified in Federal Specification GG-I-526.

Performance. The spreader shall function smoothly, without drag or binding. Under no circumstances should looseness or free play interfere with the proper function of this instrument when opening or closing.

Identification marking. In addition to the requirements specified in Federal Specification GG-I-526, the bone spreader shall also be marked "stainless".

Tests. Corrosion resistance, hardness, and performance shall be tested as specified under Quality Assurance Provisions.

Workmanship. The bone spreaders defects which detract from its appearance or impair their serviceability.

Product Quality Level

Visual and dimensional examination. Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for assuring the materials are in accordance with requirements specified.

Unit. Each (EA). One bone spreader, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:14Z
Check the source to verify that this is the currentversion before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, and as indicated in table I. Unit of product for examination purpose shall be one bone spreader.

TABLE I. Sampling for Inspection.

Type of defect	Inspection level	AQL (percent defective)
Major	II	1.0
Minor	II	4.0

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:14Z
Check the source to verify that this is the current version before use.

TABLE II. Classification of Defects.

Categories	Defects
Critical	None defined.
Major	
101	Bone spreader not free from cracks, pits, burs, sharp edges, scale, rough areas or corrosion.
102	Finish of the bone spreader not as specified.
103	Style and design not as specified.
Minor	
201	Identification markings not present, not complete, not correct, or not legible.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified below. The unit of product for test purpose shall be one bone spreader.

TABLE III. Sampling for tests.

Characteristic	Requirement	Test procedures	Inspt. level	AQL
Composition Analysis	ASTM F899		*	0.0
Hardness test	ASTM E18 E92 E140	ASTM E18 E92 E140	S-2	1.0
Dimensions	Rqrmt's		S-1	2.5
Copper Sulfate test	GG-I-526	GG-I-526	S-2	1.0
Boil test	GG-I-526	GG-I-526	S-2	1.0
Performance	Rqrmt's		S-2	1.0

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:14Z
Check the source to verify that this is the current version before use.

Tests.

Corrosion resistance. The bone spreader shall be tested as specified in Federal Specification GG-I-526.

Hardness. Hardness shall be tested in accordance with ASTM E18 or E92 whichever is applicable. Conversion of hardness values shall be in accordance with ASTM E140.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:14Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number (s) are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-125-3228	SPREADER, BONE, PEDIATRIC, Baby Inge, 6-1/8 inches (15 cm) long

Ordering Data: (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and /or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4134

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:14Z
Check the source to verify that this is the currentversion before use.

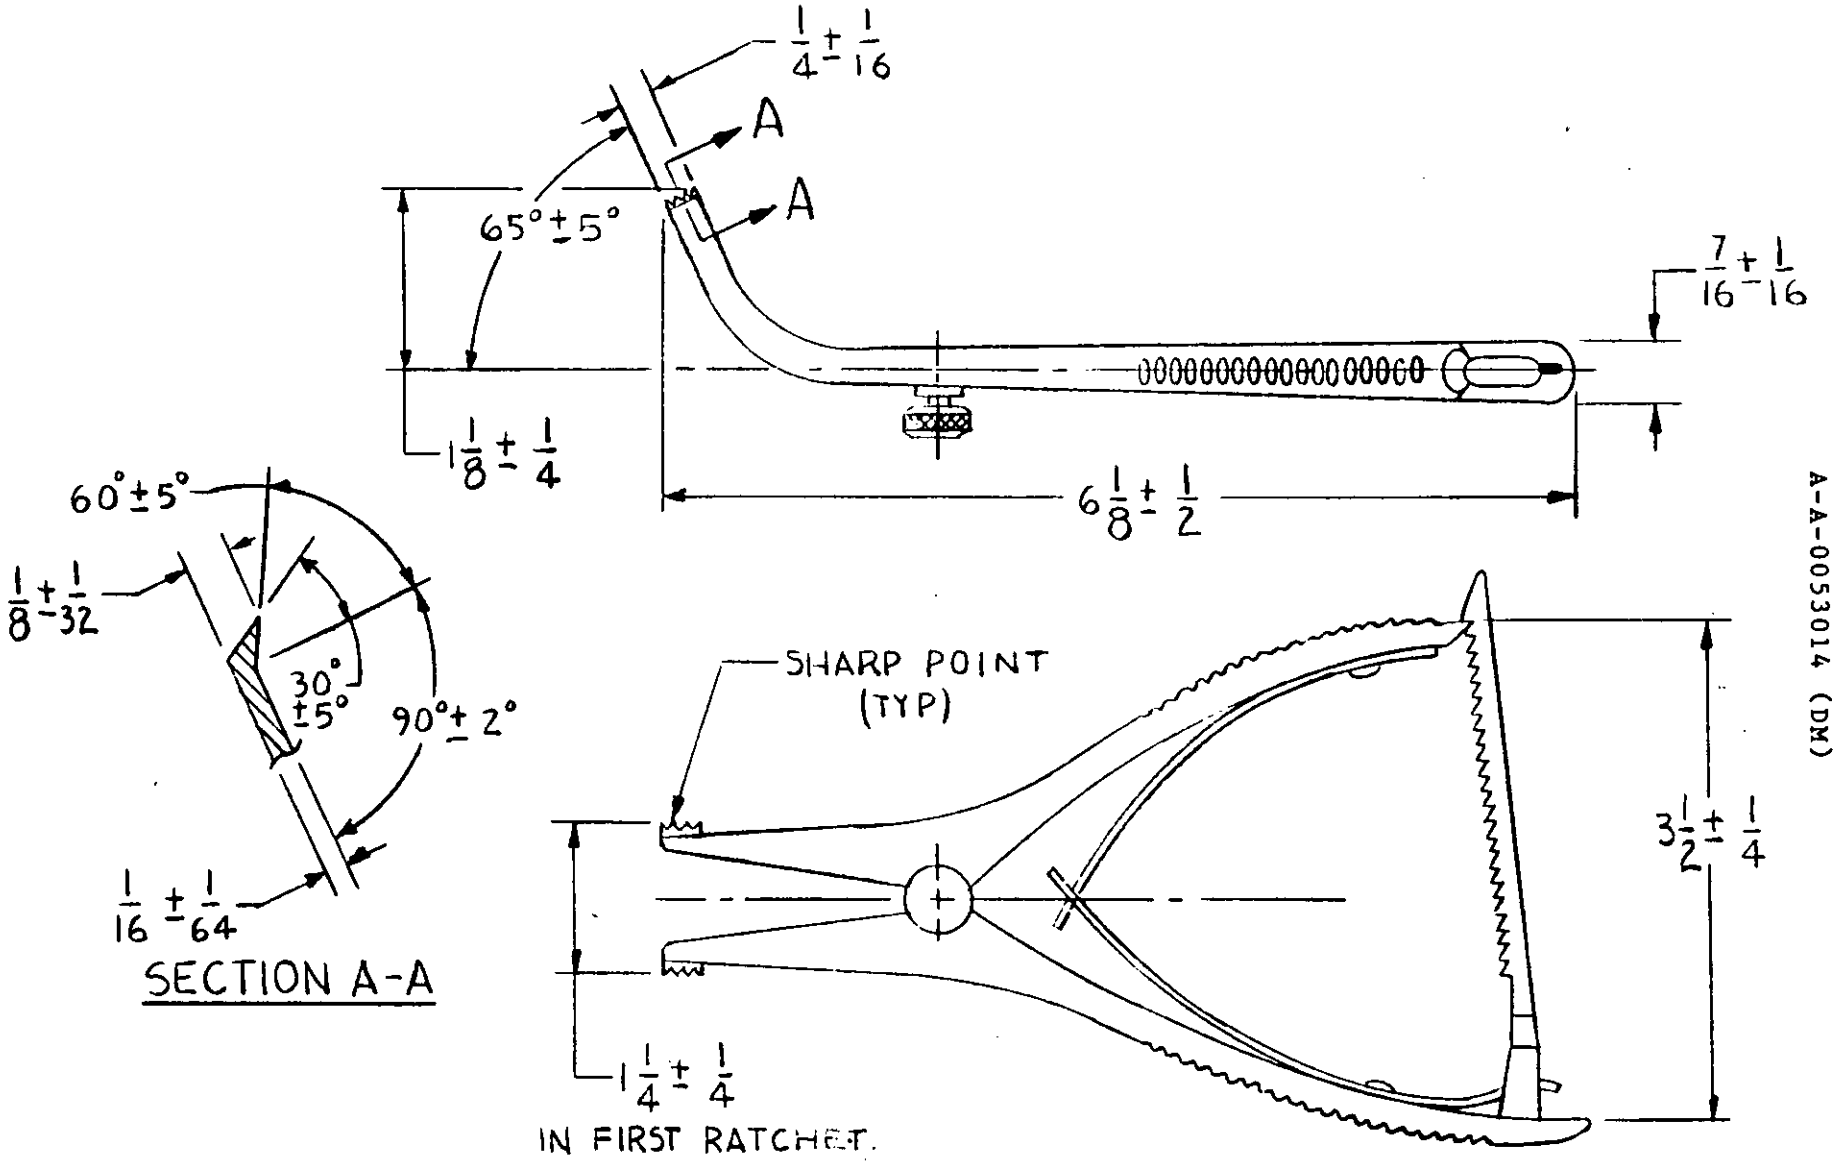

A-A-0053014 (DM)

FIGURE 1 SPREADER, BONE, BABY INGE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:14Z
Check the source to verify that this is the current version before use.