A-A-53022A
7 January 1991
SUPERSEDING
A-A-0053022(DM)
25 June 1987

COMMERCIAL ITEM DESCRIPTION

STAPLES, BONE FIXATION

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers serrated bone fixation staples, with spikes, suitable for use in orthopedic surgery.

Salient characteristics:

Style and design. Staples shall be in accordance with Figure 1.

The staples shall be U-shaped bone fixation staples used in orthopedic surgery. The staples shall have two legs, parallel to within ± 0.01 inch, each one inch in length. Legs shall have rectangular cross sections and shall have a minimum of five serrations on the outerside of the legs to prevent the staples from backing out of the bone.

Staples shall have spikes on the underside of the bridge between the legs.

Staples shall be compatible with driver-extractor (See Note 2).

Material. Staples shall be fabricated from cobalt-chromium-molybdenum alloy in accordance with ASTM Designation F75.

Marking and surface preparation. Manufacturers name (or trademark), manufacturers catalog number, and size denominations shall be clearly marked on the topside of the staple bridge. Surface preparation and marking shall be in accordance with ASTM Designation F86.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:14Z
Check the source to verify that this is the current version before use.

Corrosion properties. The staples shall show no evidence of corrosion when subjected to the following test:

Boil. Staple shall be scrubbed with alkaline cleaner corresponding to part II of ASTM Designation B322, rinsed thoroughly in distilled water, and dried. After cleaning, the staple shall be boiled in distilled water in a glass beaker for 30 minutes, and allowed to remain submerged for an additional 24 hours.

Workmanship. The staples shall be free from defects which detract from their appearance or impair their serviceability.

Unit. Each (EA). One staple, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:14Z
Check the source to verify that this is the current version before use.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. The acceptable quality level (AQL) shall be 1.0 for an inspection level of S-2. The unit of product for test purposes shall be one staple.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch/pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufacturedto metric dimensions and those dimensions exceed the tolerance specified in the inch/pound units, a request should be made to the contracting officer to determine of the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:14Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE 1: The following National Stock Numbers are covered by this document:

NSN	ITEM IDENTIFICATION
6515-01-176-0690	STAPLE, BONE FIXATION Cobalt-Chromium, Extra Small
6515-01-175-2316	STAPLE, BONE FIXATION Cobalt-Chromium, Small
6515-01-175-2317	STAPLE, BONE FIXATION Cobalt-Chromium, Medium
6515-01-175-2318	STAPLE, BONE FIXATION Cobalt-Chromium, Large

NOTE 2: The bone fixation staples shall be compatible with a driver-extractor, fixation staple (NSN 6515-01-164-3146).

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:

DLA-DM


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 06708

Project No. 6515-4570

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:14Z
Check the source to verify that this is the current version before use.

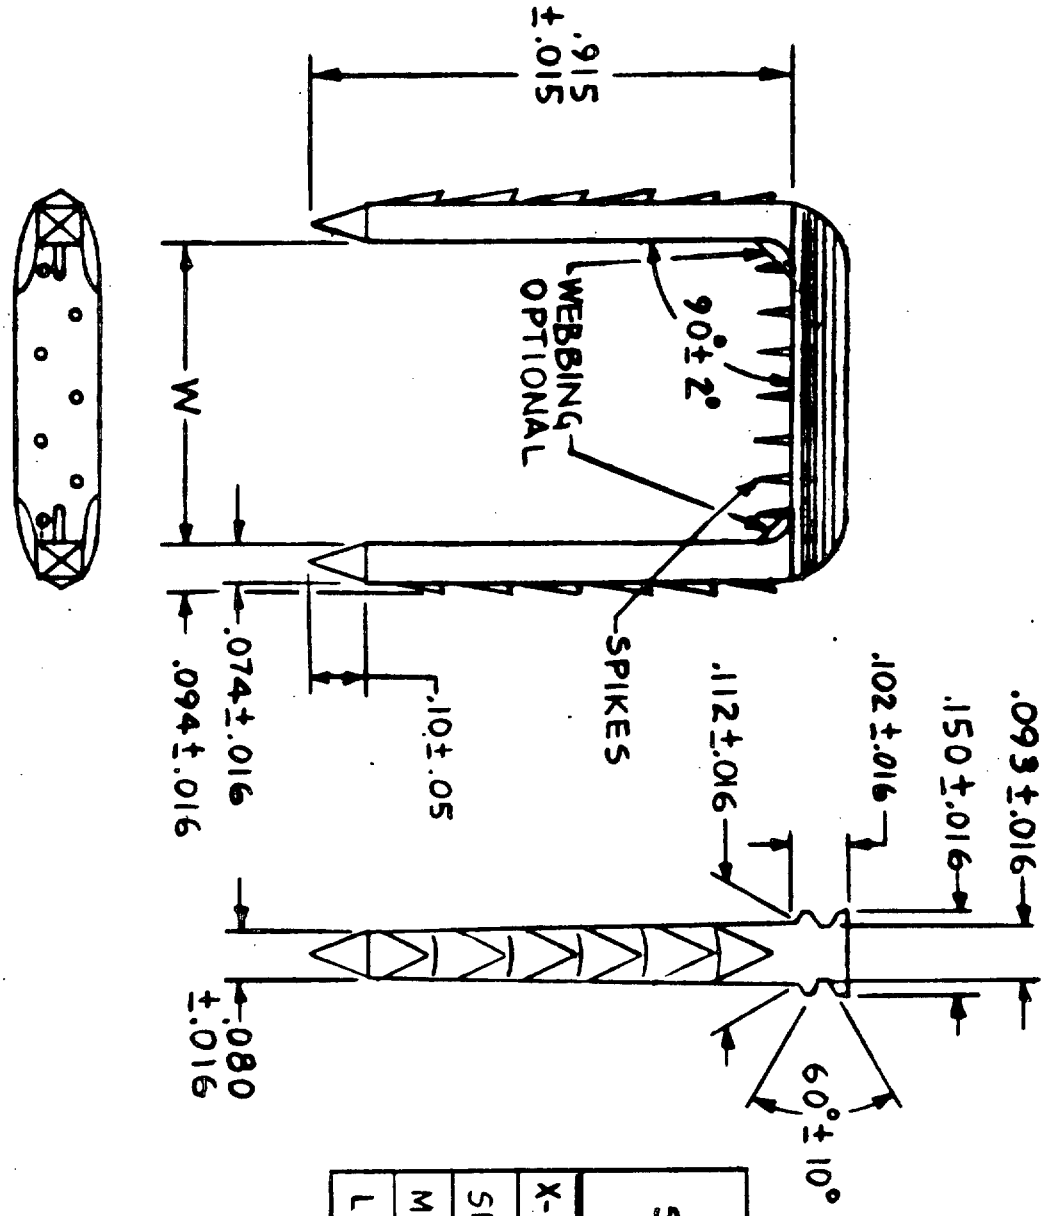

SIZE	WIDTH BETWEEN LEGS ± 1/64 INCHES W	NUMBER OF SPIKES ± 1
X-SMALL	1/4	3
SMALL	5/16	5
MEDIUM	7/16	7
LARGE	9/16	7

FIGURE 1 STAPLE, BONE FIXATION

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:14Z
Check the source to verify that this is the current version before use.