A-A-53328
18 December 1987

COMMERCIAL ITEM DESCRIPTION

DILATOR SET, UTERINE, HANK

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-D-36798(1), dated 11 May 1972, which is cancelled.

This commercial item description covers a set of Hank-design, double-ended uterine dilators in a carrying case.

Salient characteristics:

General. Shall be a set of double-ended, Hank-design, uterine dilators enclosed in a roll-up type, cloth case. The set shall contain six (6) dilators, 2 sizes per dilator, American sizes 9 to 20 inclusive.

Dilators.

Material. The dilators shall be fabricated from Class 3, austenitic steel conforming to ASTM (American Society for Testing and Materials) F899.

Style and design. The dilators shall be Hank-design dilators conforming to Figure 1. The dilators shall have suitable dulled or rounded tips at each end. The dilators shall have stops at the base of its curved tips.

Hardness. When tested as specified in Federal Specification GG-I-526, the dilators shall have a Rockwell Hardness of B75, minimum.

Boil test. The dilators shall pass the Boil test requirements specified in GG-I-526.

Marking requirements. Dilators shall be marked as directed in Figure 1. Dilators of foreign manufacture shall be marked with the legend "stainless."

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:18Z
Check the source to verify that this is the current version before use.

Finish. Dilators shall have a bright, smooth overall finish. Dilators shall be properly passivated.

Case.

Material. The case shall be fabricated from 9.85 oz. Army duck cloth.

Style and design. The case shall be a "roll-up" design case. The case shall contain 6 retaining loops (one per dilator), two inside flaps, and two tie tapes. Case edges shall be tape bound and vinyl coated. As an alternate, the case edges may be tape bound, turned under, and sewn.

Physical properties. The physical properties of the case shall conform to Table 1 when subjected to the indicated tests. All testing shall conform to FED-STD-191.

TABLE 1

Property	Numeric Value	Test Method FED-STD-191
Weight per sq. yd., minimum	9.85 oz.	5041
Yarn ply, minimum, warp	2	Visual examination
Yarn ply, minimum, filling	2	Visual examination
Texture, yarns per inch, minimum, warp	52	5050
Texture, yarns per inch, minimum, filling	40	5050
Breaking strength, minimum, warp	160 lbs.	5100
Breaking strength, minimum, filling	110 lbs.	5100

Color. The case shall be vat dyed olive drab No. 7.

Workmanship. All components (dilators and cases) shall be free from any defects which detract from their appearance or impair their serviceability.

Unit. Set (SE). One dilator set, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:18Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Inspection shall be conducted at level II, AQL (Acceptable Quality Level) 1.5 percent. The unit of product for test purposes shall be one set.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:18Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Public Law 94-580 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

NOTE: This document covers the following National Stock Number (NSN):

NSN	ITEM IDENTIFICATION
6515-00-325-5500	DILATOR SET, UTERINE, Hank, Set of 6

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:.

DoD-MB

Agent:

DLA-DM

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:18Z
Check the source to verify that this is the currentversion before use.


CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

PGC 45421

Project No. 6515-3572

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:18Z
Check the source to verify that this is the current version before use.

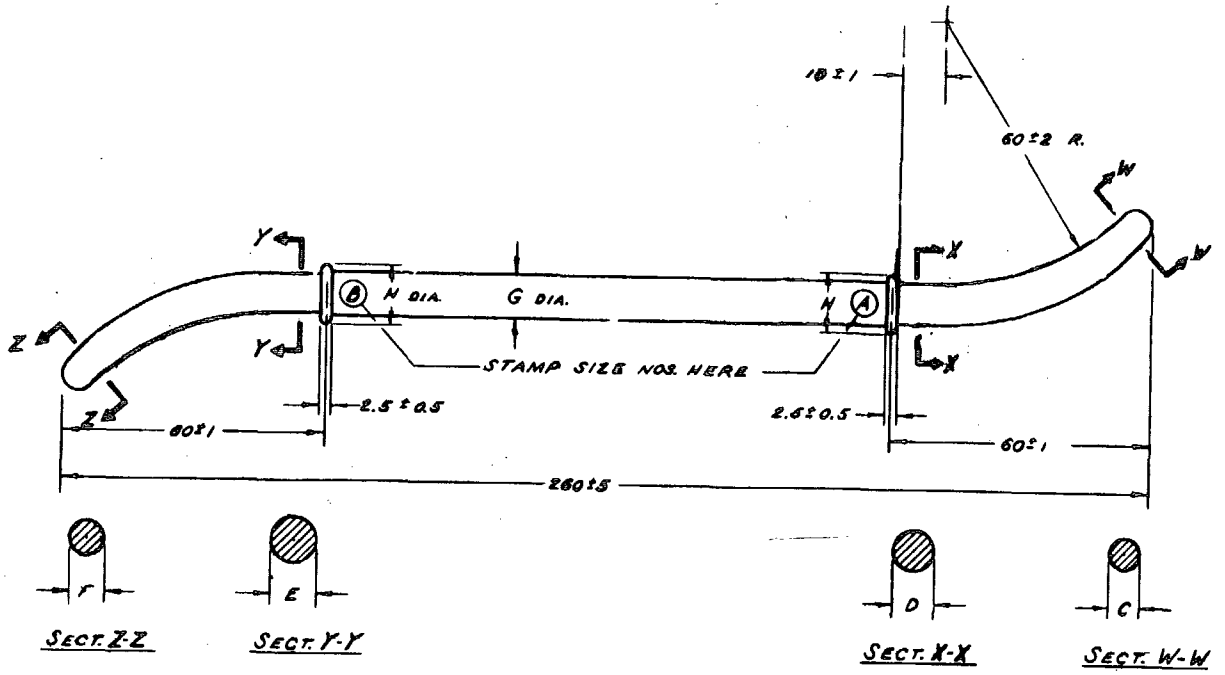

SIZE		SIZE No.	C	D	E	F	G	H
9 & 10	A	9	3.4 ± 0.1	4.5 ± 0.1			5.0 ± 0.1	8.5 ± 0.5
	B	10			5.0 ± 0.1	3.8 ± 0.1		
11 & 12	A	11	4.2 ± 0.1	5.5 ± 0.1			6.0 ± 0.1	9.5 ± 0.5
	B	12			6.0 ± 0.1	4.6 ± 0.1		
13 & 14	A	13	5.0 ± 0.1	6.8 ± 0.1			7.0 ± 0.1	10.5 ± 0.5
	B	14			7.0 ± 0.1	5.4 ± 0.1		
15 & 16	A	15	5.8 ± 0.1	7.5 ± 0.1			8.0 ± 0.1	11.5 ± 0.5
	B	16			8.0 ± 0.1	6.2 ± 0.1		
17 & 18	A	17	6.6 ± 0.1	8.5 ± 0.1			9.0 ± 0.1	12.5 ± 0.5
	B	18			9.0 ± 0.1	7.0 ± 0.1		
19 & 20	A	19	7.4 ± 0.1	9.5 ± 0.1			10.0 ± 0.1	13.5 ± 0.5
	B	20			10.0 ± 0.1	7.8 ± 0.1		

NOTE:
ALL JOINTS TO BE SILVER SOLDERED
ALL DIMENSIONS IN MILLIMETERS

FIGURE 1
DILATOR SET, UTERINE, HANK

Source: https://assist.dla.mil -- Downloaded: 202640-26T09:18Z
Check the source to verify that this is the current version before use.