METRIC

A-A-51363A
15 June 1992
SUPERSEDING
A-A-51363
21 March 1986

COMMERCIAL ITEM DESCRIPTION

DRAIN, SURGICAL, Rubber, T-type, Sterile

The General Services Administration has authorized the use of this commercial item description as a replacement for Military Specification MIL-D-36140A which is cancelled.

This commercial item description covers sterile gravity drains for fluid drain of the ureter or gall bladder in general surgical and treatment procedures.

Salient Characteristics:

General. This specification covers surgical drains of the following sizes:

Size 14 French
Size 16 French
Size 22 French

The specific drain size to be provided for each stock number is indicated under notes.

The drain shall be fabricated in the form of a letter "T" the juncture of which shall be smooth without seams or groove marks.

Material. The drains shall be of natural latex rubber, non-pyrogenic, nontoxic and meet the requirements of the United States Pharmacopiea (USP) for Class IV Plastics.

Style, design and dimensions. The drain shall be in accordance with Figure 1.

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Physical properties. The drain shall show no visible evidence of deterioration (surface brittleness and tackiness) and shall not show a decrease of greater than 25 percent in ultimate elongation and breaking strength when subjected to the Standard Test Method for Rubber - Deterioration in an Air Oven, ASTM Designation D573.

Sterility. The surgical drain shall be sterile when tested in accordance with the USP or AAMI guidelines. Sterility Assurance Level shall be 0.000001.

Identification marking and labeling. Each drain shall be legibly and permanently marked with name of manufacturer or registered trademark, French size, and date of manufacture (year, month).

Labeling. Labeling shall conform with the requirements of the Federal Food, Drug and Cosmetic Act, and in addition the label of the immediate container shall identify the T-tube cross bar length, French size, contractor's name or trademark and the legend "sterile".

Workmanship. The drain shall be processed in such a manner as to be uniform in quality and free from defects that will affect life, serviceability, or appearance. Surfaces and ends of the drain shall be smoothly finished to prevent irritation in patient.

Unit. Package (PG). One package containing 10 individually packaged drains of one size only, as specified, constitutes one unit. Each drain shall be individually packaged sterile in a sealed peel-open container capable of maintaining sterility of contents unless package is damaged or opened. The sealed container shall be designed to permit ready dispensing of the T-tube drain by sterile techniques.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract of purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. The unit of product for test purposes shall be one drain.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producer's own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order.

NOTE: The following National Stock Numbers and their Item Identifications are covered by this document:

NATIONAL STOCK NUMBER	ITEM IDENTIFICATION
6515-01-262-4500	DRAIN, SURGICAL, Rubber, T-type, 14 Fr, 10s
6515-01-262-8705	DRAIN, SURGICAL, Rubber, T-type, 16 Fr, 10s
6515-01-125-6591	DRAIN, SURGICAL, Rubber, T-type, 22 Fr, 10s

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

Preparing Activity:

DoD-MB

Agent:


DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6515-5291
Location: \word\nish\draincid

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T08:54Z
Check the source to verify that this is the current version before use.

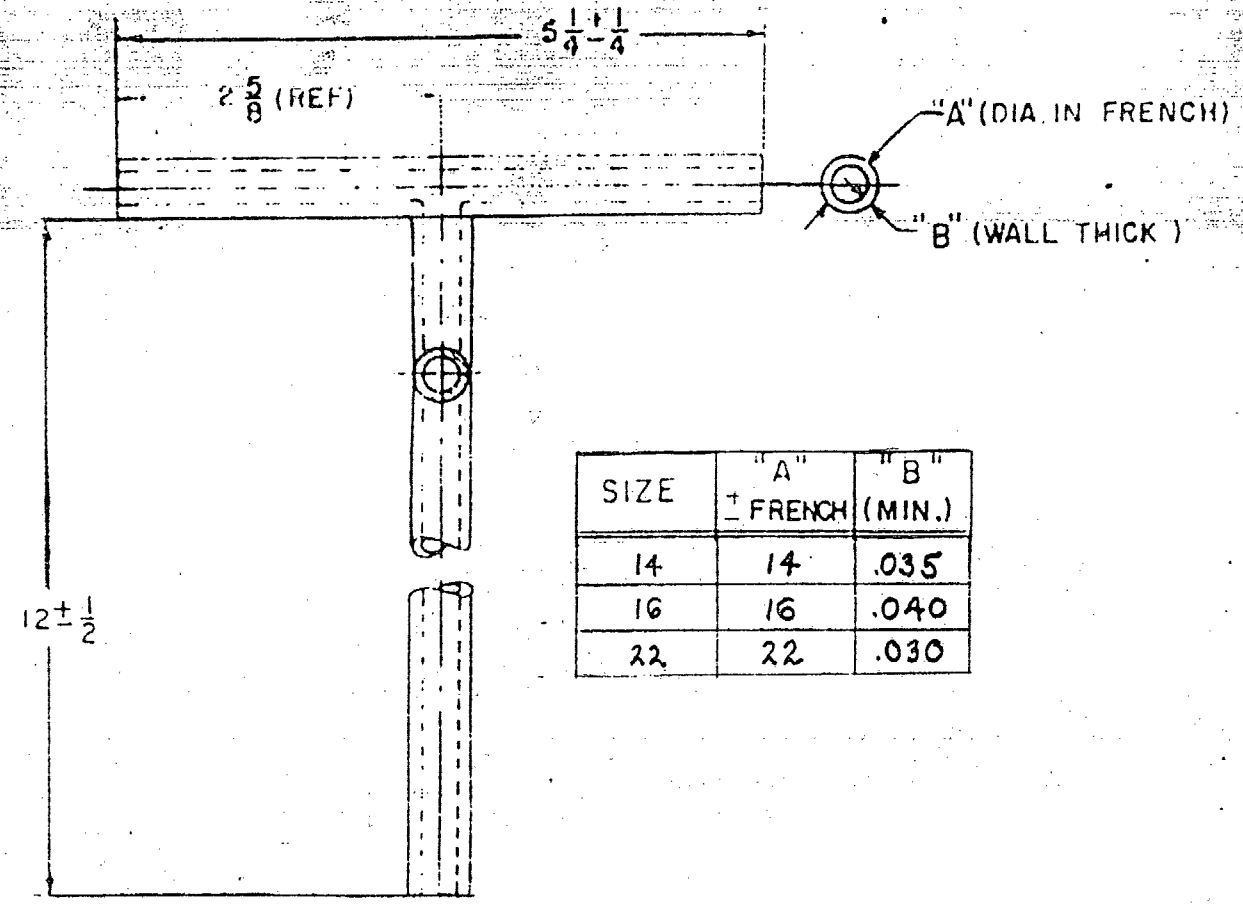

SIZE	"A" ± FRENCH	"B" (MIN.)
14	14	.035
16	16	.040
22	22	.030

A-A-51363A

FIGURE 1. SURGICAL RUBBER DRAINS, T-TYPE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26 10:26:51
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8 In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-51363A	15 June 1992

3. DOCUMENT TITLE
DRAIN, SURGICAL, Rubber, T-type, Sterile

4. NATURE OF CHANGE *(Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)*

5. REASON FOR RECOMMENDATION

6. SUBMITTER

a. NAME (Last, First, Middle Initial)	b. ORGANIZATION	
c. ADDRESS (Include Zip Code)	d. TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	7. DATE SUBMITTED (YYMMDD)

8. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial 215-737-2870	(2) AUTOVON 444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT: Defense Quality and Standardization Office 5203 Leesburg Pike, Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

Source: https://assist.dla.mil -- Downloaded: 2026-10-26 08:54Z
Check the source to verify that this is the current version before use.