COMMERCIAL ITEM DESCRIPTION

TABLE, ANESTHETIST'S

The General Services Administration has authorized the use of this Commercial Item Description as a replacement for Federal Specifications AA-T-0041E and AA-T-41C.

This Commercial Item Description covers one type of corrosion-resisting steel anethetist's table with two removable trays and one drawer under the lower tray.

Salient characteristics:

The anesthetist's table shall consist of a frame mounted on casters, two removable trays, two tray supports, and a drawer under the lower tray. Figure 1 shows a typical configuration and dimensions for the table.

The table frame shall primarily consist of four uprights formed of two inverted "U's" of one inch outside diameter, No. 16 gage. There shall be a 3/8 inch diameter rod welded to the two back uprights approximately 3-1/4 inches above the top tray. The frame shall be mounted on four 2-inch diameter conductive swivel casters with ball bearings.


The trays shall have minimum dimensions of 12-3/4 inches wide by 18-3/4 inches long by 5/8 inch deep. The two tray supports shall be 1 inch by 3/16 inch bars welded at approximately 29 inches and 15 inches above the floor. Two 6-inch long hooks for masks shall be welded to the upper rear cross bar of the support.

The table shall be constructed of 300 series stainless steel throughout and polished to a No. 4 finish, or brighter, on all exposed surfaces.

The drawer shall be 20 gage or heavier with minimum inside dimensions of 12 by 12 by 4 inches and mounted directly below the bottom tray. The drawer front shall be 16 gage, minimum, with a chrome plated pull. The drawer shall operate on slides welded to the lower tray support and shall be removable for cleaning. A positive stop to prevent inadvertent removal and

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

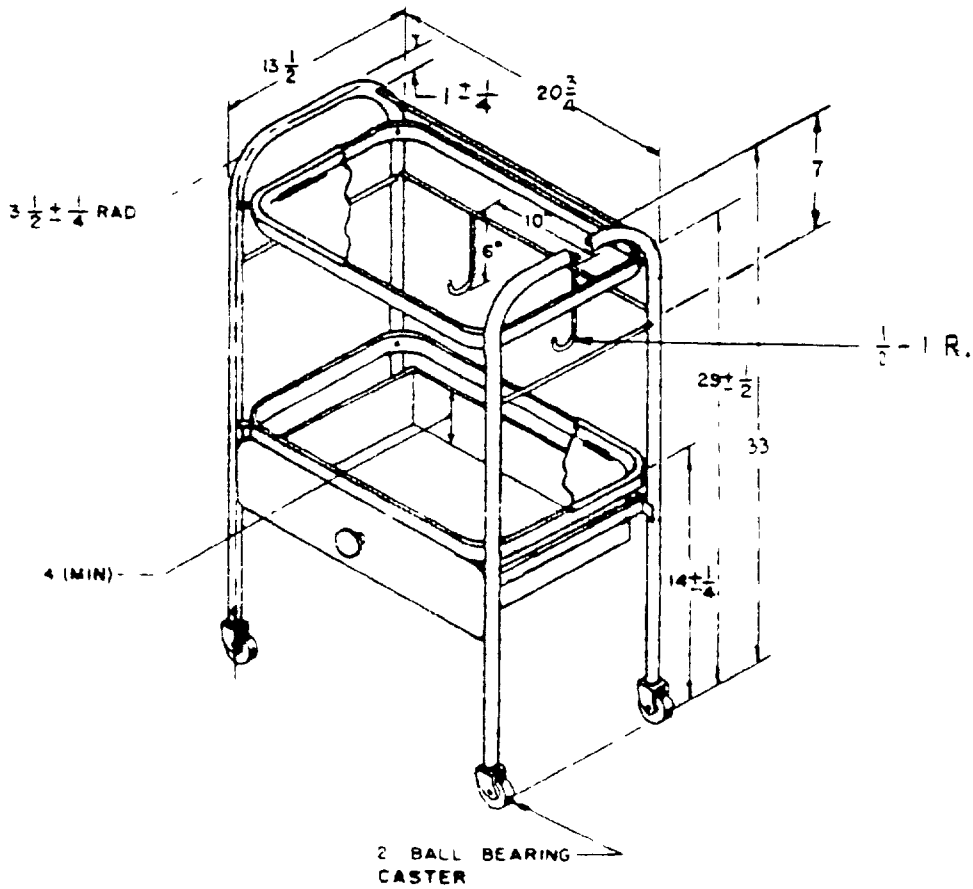

UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES		
TOLERANCES ON		
FRACTIONS	DECIMALS	ANGLES
± 1	±	±

FIGURE 1 ANESTHETIST'S TABLE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

a means to keep the door closed when the table is moved shall be provided.

All exposed table surfaces shall be free from pit marks, weld seams, and scale. All exposed corners on the anesthetist's table shall be broken, rounded, or otherwise treated to eliminate sharp edges. The manufacturer's name or registered trademark shall be permanently and legibly marked on each table. Each tray shall be similarly marked by impressing the underside without penetration of the inside surface of the tray.

Workmanship. The anesthetist's table shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One table, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one anesthetist's table as specified in this description.

Sampling for tests. Sample sizes for tests shall be as indicated for inspection level S-2 in MIL-STD-105, except that the acceptance number shall be zero for all sample sizes, and a minimum of three (3) sample tables shall be taken.

Tests. Tests shall be conducted, as necessary, to determine compliance with specification requirements.

Conductivity test. Tests for electrical conductivity shall be conducted on the table as described in section 469 of National Fire Protection Association, NFPA No. 56A.

Chemical Analysis test. Tests for chemical analysis shall be conducted in accordance with method 111.2 or 112.2 of [illegible]. In lieu of the above, a certificate of quality, may be furnished, showing results of tests performed to indicate that material is as specified in 3.1.

Stability test.

1. Uprights. The table shall be placed on a level surface and examined for rocking conditions in both lateral directions. The distance between the bottom of the caster wheels and the floor surface shall be recorded for any caster wheel not resting on the floor surface.

2. Trays. Each tray shall be placed in a tray frame and examined for improper fit or wobbling. Trays which will not seat flush in the frame or wobble more than 1/8 inch in either lateral axis when placed on the tray frame are classified as defects.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document:

6530-00-708-8425

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03
VA-OSS
USPHS
FDA-MPQAS

PREPARING ACTIVITY.

DoD - MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

Project No. 6530-2138

Location:
CID/TABLE/ANESTHETIST/H11-37

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-54214	TABLE, ANESTHETIST'S

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last, First, MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

(Fold along this line)

DEFENSE LOGISTICS AGENCY

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4956 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge (*DO NOT STAPLE*) and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE. This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.