A-A-54216
31 July 1990

COMMERCIAL ITEM DESCRIPTION

STAND, BASIN

(Corrosion-Resisting Steel)

The General Services Administration has authorized the use of this commercial item description as a replacement for Federal Specification RR-S-705 which is cancelled

This Commercial Item Description covers a corrosion-resisting steel basin stand

Salient Characteristics

The basin stand shall be either of the following two types

Type 1 - Stand, Basin, Single, Corrosion-Resisting Steel, for 9 quart basins

Type 2 - Stand, Basin, Double, Corrosion-Resisting Steel, for 7 quart basins

The material for the stands and basins shall be corrosion-resisting steel conforming to American Iron and Steel Institute (AISI) type 302 or type 304. The stands shall sit level on the floor and be free from wobble.

The design and construction of the basin stand shall be as shown for the applicable type in figures 1, 2, 3, and 4 and as specified herein.

Type 1 stand


The type 1 stand shall have one basin ring which shall accommodate one 9 quart basin. One basin shall be furnished with each stand.

AMSC N/A FSC 6530


DISTRIBUTION STATEMENT A Approved for public release, distribution is unlimited

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

COMPONENT	TYPE I DIMENSIONS		TYPE II DIMENSION	
LEG	A	33 ± 1	A	33 ± 1
TRANSVERSE BRACE	B	13 13/32 ± 1/8	B	12 1/4 ± 1/32
	C	8 1/4 ± 1/4	C	8 1/4 ± 1/4
LENGTHWISE BRACE	D	13 1/4 ± 1/8	D	30 ± 1/4
BASIN RING	E	I D OR DISTANCE BETWEEN, RODS [illegible]	E	I D 11 15/16 ± 1/16

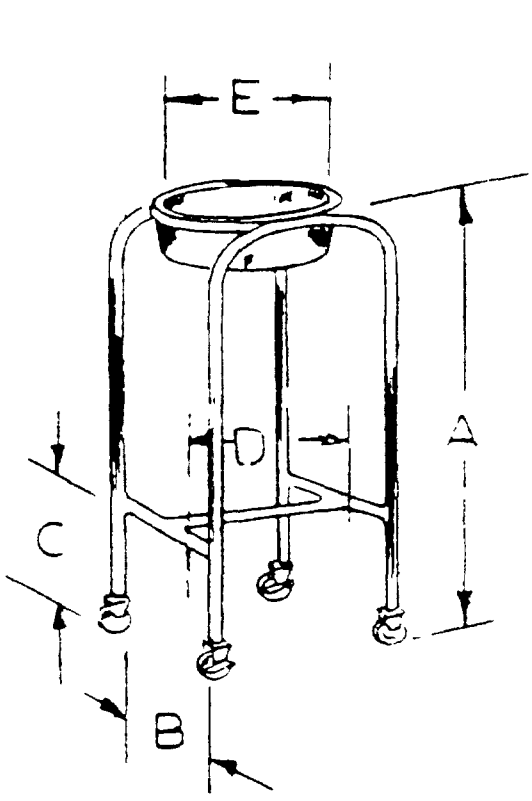

TYPE I ONE BASIN STAND

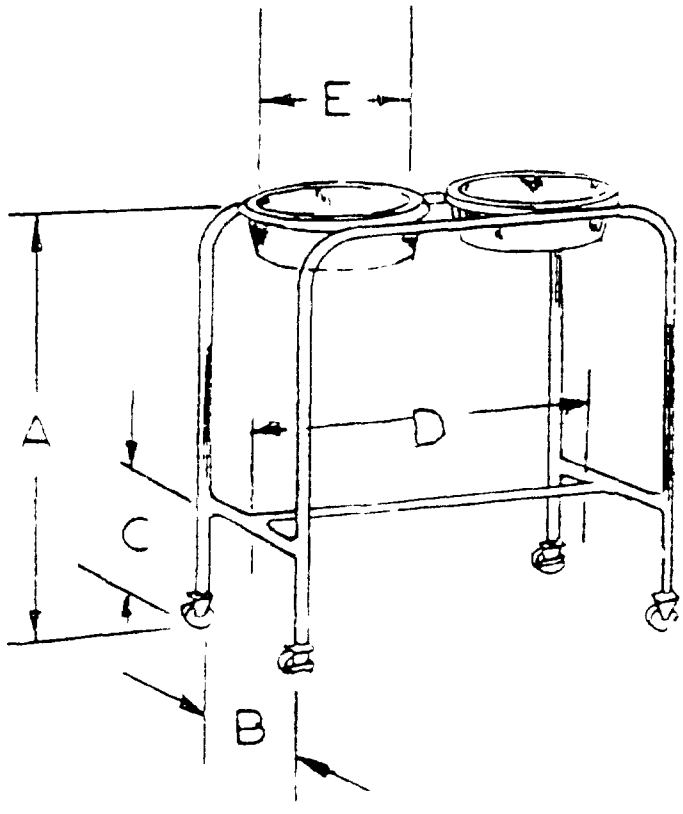

TYPE II TWO BASIN STAND

FIGURE 1. Stand, basin

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

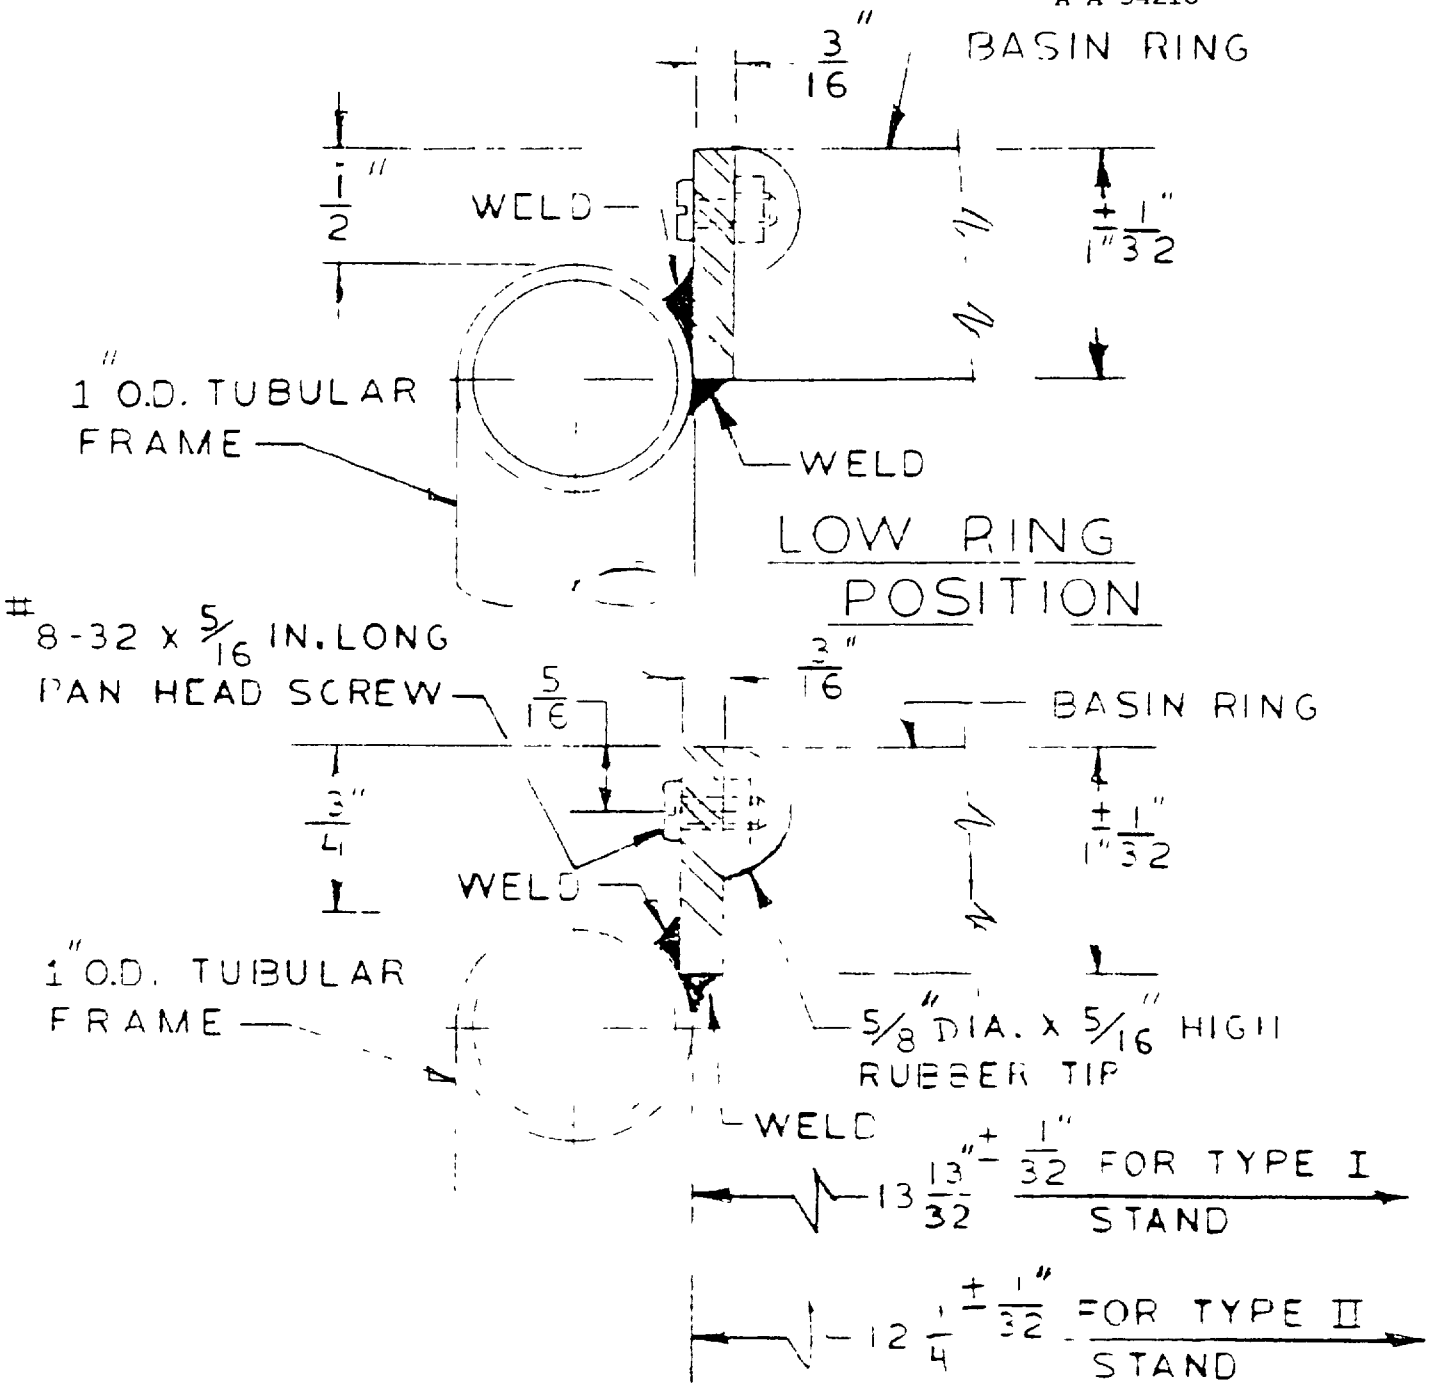


FIGURE 2. High ring position

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.


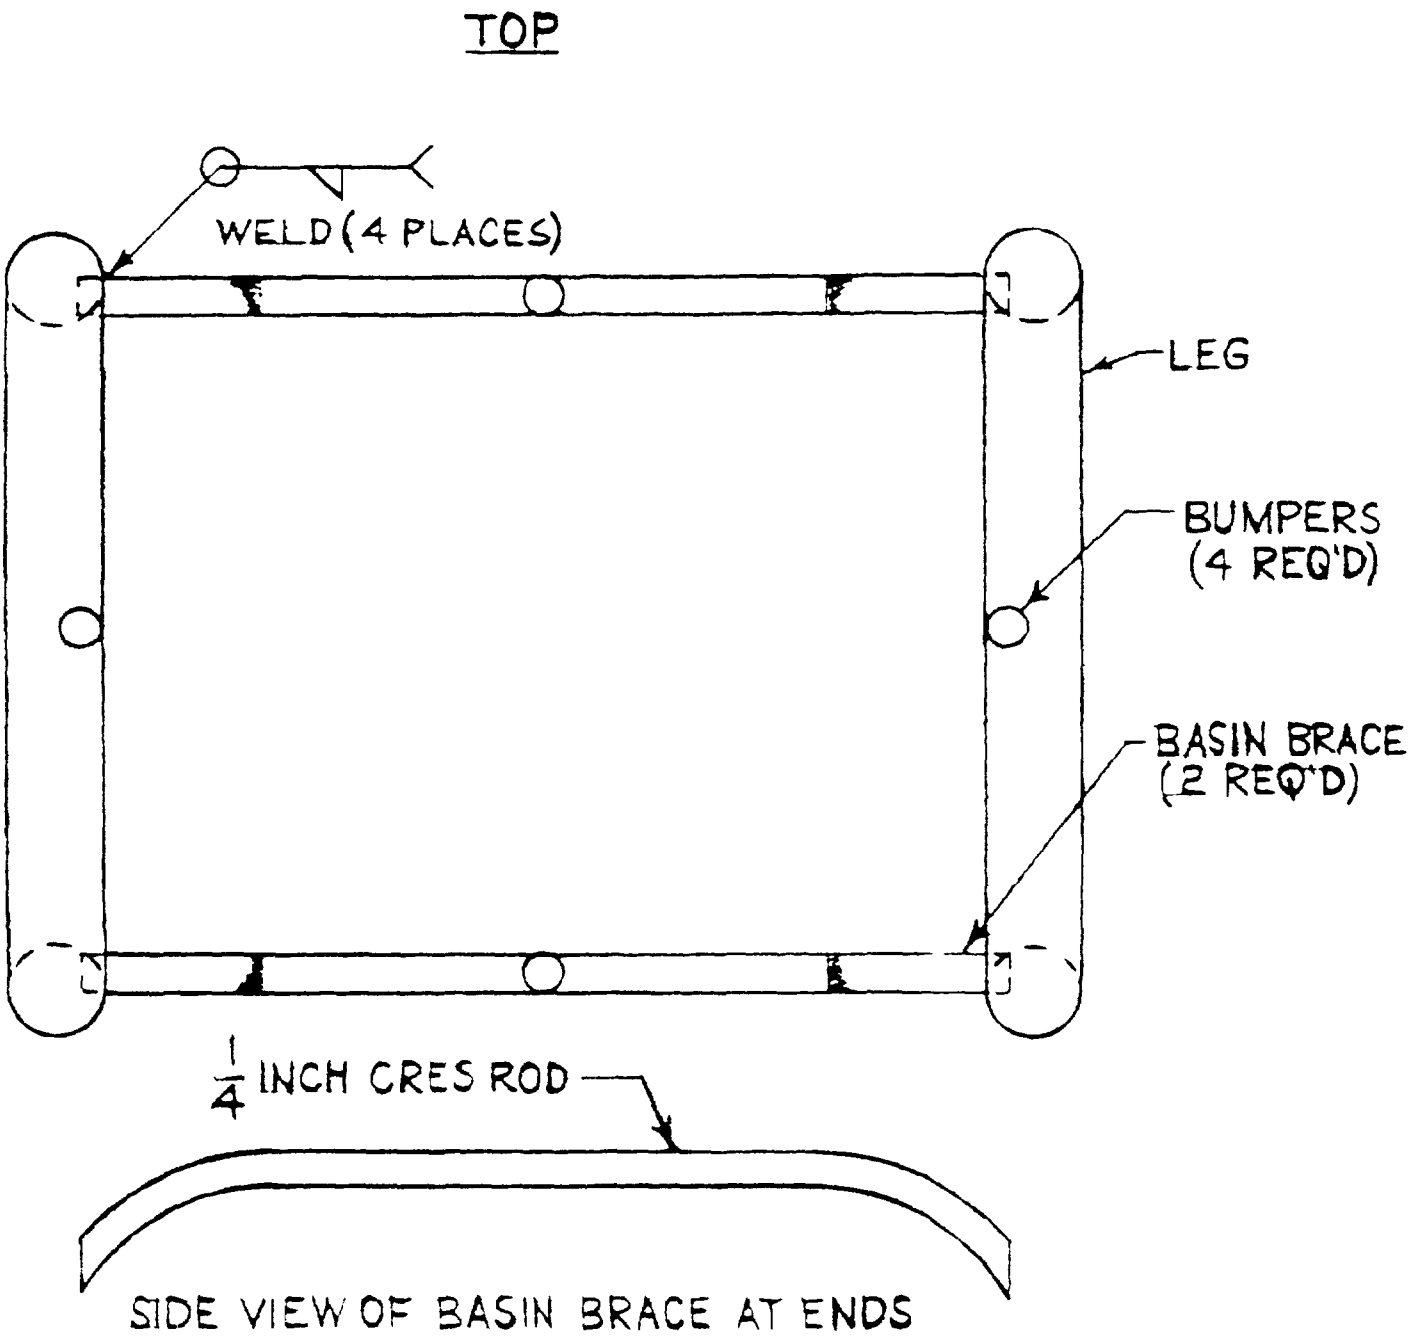


FIGURE 3. Alternate basin brace construction for one basin stand.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

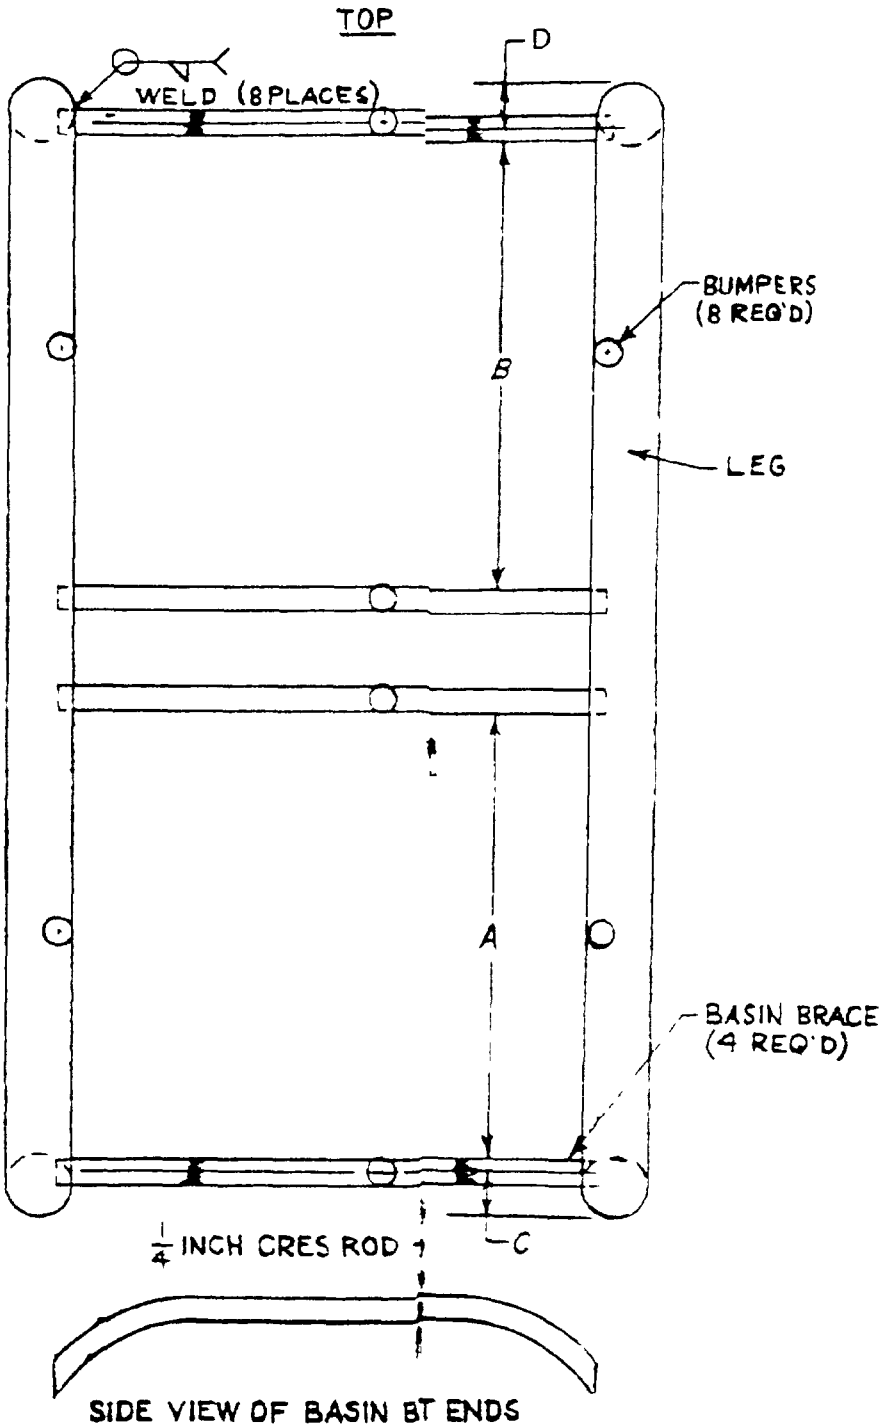

NOTE: BASIN BRACES SHALL BE I SUCH THAT BASINS WHEN SEATED ON THE RUBBER CONDUCTIVE REMAIN IN A POSITION NORMAL TO THE UPRIGHTS. FURTHER, SIN BRACES SHALL BE LOCATED SUCH THAT DIMENSIONS "B" ARE EQUAL AND "C" AND "D" ARE EQUAL.

FIGURE 4. Alternate basin brace ction for two basin stands.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

The stand frame shall be made from seamless or welded tubing with a wall thickness not less than 0 049 inch nor greater than 0 065 inch Round tubing shall be 7/8 inch plus 1/8 inch, minus 1/64 inch in diameter Square tubing shall be 7/8 inch plus or minus 1/64 inch wide Two lengths of tubing shall be bent and shaped on 3 inch radii to form two well-rounded inverted 'U's Each 'U' tubing shall form one longitudinal side of the top and two legs The dimensions shall be as shown in figure 1 The legs of the frame shall be equipped with casters

The transverse braces shall be made from seamless or welded tubing with a wall thickness not less than 0 049 inch nor greater than 0 065 inch Round tubing shall be either 3/4 inch plus or minus 1/64 inch or 7/8 inch plus 1/8 inch minus 1/64 inch in diameter Square tubing shall be 7/8 inch plus or minus 1/64 inch wide As an alternate to round or square tubing for the transverse braces, 3/8 inch diameter corrosion-resisting steel rod shall be allowed The tubing or rod shall be welded to each end of the frame and shall protrude at least 1/4 inch within the wall of the frame Dimensions shall be as shown in figure 1

The longitudinal brace shall be made from seamless or welded tubing with a wall thickness not less than 0 049 inch nor greater than 0 065 inch Round tubing shall be either 1/2 inch plus or minus 1/64 inch or 7/8 inch plus 1/8 inch minus 1/64 inch in diameter Square tubing shall be 7/8 inch plus or minus 1/64 inch wide As an alternate to round or square tubing for the longitudinal brace, 3/8 inch diameter corrosion-resisting steel rod shall be allowed The tubing or rod shall be welded to the middle point of the two transverse braces, forming a double 'T' brace as shown in figure 1 Dimensions shall be as shown in figure 1

The basin ring shall be fabricated from corrosion-resisting steel strip 1/8 inch to 3/16 inch thick and 31/32 inch to 1-1/4 inch wide The steel strip shall be shaped into a ring and shall be attached to the top of the frame and shall extend 1/2 inch to 3/4 inch above the top of the frame as shown in figure 2 The ring shall be welded into a single seamless piece before being welded to the frame The steel strip basin ring shall be continuously welded to the frame midpoint from the ends by welds not less than 1-1/4 inches in length

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

As an alternate, the basin support shall consist of 1/4 inch corrosion-resisting steel rod welded to the legs as shown in figure 3 The steel rod basin braces shall be level with the top of the frame

There shall be four well-rounded, electrically conductive, rubber bumper tips, attached to the inner surface of the basin ring by a screw which passes through the ring and into the back of the rubber for basin rings constructed of steel strip Basin supports fabricated from corrosion-resisting steel rod shall have the rubber tips fastened to the frame and brace rods in the same manner as described above and in figure 3 As an alternative, three electrically conductive bumper tips may be fastened to the basin rings as described above, however, the bumper tips shall be located 120 degrees apart from each other The basin shall rest on top of the basin ring and shall be prevented from rattling by the rubber tips

Type 2 stand

The type 2 stand shall have two basin rings and shall accommodate two 7 quart basins Two basins shall be furnished with each stand

The frame, longitudinal brace, and transverse braces shall be made of the same material and construction as specified for type 1 stands except as indicated in figure 1

The basin rings shall be made of the same material and construction as specified for type 1 except the ring shall be welded into a single seamless piece as indicated in figure 1 The steel strip basin rings shall be continuously welded to the frame from the ends, by welds not less than 1-1/4 inches in length

As an alternate, the basin support shall consist of 1/4 inch diameter corrosion-resisting steel rod welded to the legs as shown in figure 4 The steel rod basin braces shall be level with the top of the frame The rubber bumper tips shall be the same material and design as specified for the type 1 stand except as indicated in figure 4 As an alternate, three electrically conductive bumpers may be

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

fastened to the basin rings as described above However, the bumpers shall be located 120 degrees apart from each other The basin shall rest on top of the basin ring or support and shall be prevented from rattling by the rubber tips

General

Each basin stand shall be equipped with 3 inch diameter electrically conductive casters The casters shall be light duty, stem-mounted with nonadjustable socket adapter, swivel-type, with natural rubber, synthetic rubber, or polyurethane composition rubber wheels with resilient tread Two casters shall have side brakes If utilized, rubber adapters in rubber expanding stems shall be of electrically conductive rubber or have metal clips designed so that positive metal to metal contact is made as the adapter is expanded The stand, with the casters in place shall be electrically conductive when tested according to NFPA Standard 99, Health Care Facilities

All surfaces to be welded shall be free from grease, oil, oxides, or any other foreign matter Any cleaning method which will remove these substances and leave the surface clean is satisfactory All weld joints shall blend into the adjacent metal in gradual, smooth curves Beads shall be smooth and free of slag, excessive undercut or excessive spatter Sufficient metal shall be added to provide a suitable fillet or reinforcement All welds shall be continuous with no visible voids pinholes, or cracks

Exposed or accessible edges corners, and surfaces of the stand shall be free of burrs, sharpness and sharp projections The stand finish shall be free of coarse grind marks dents cracks or crimps All exposed metal surfaces shall be polished to a smooth No 4 commercial finish or better The finished stand shall be free from oil, grease and dirt

Workmanship The basin stand shall be free from defects which detract from its appearance or impair its serviceability

Unit Each [illegible] of the type specified constitutes one unit

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions

Responsibility for inspection Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements

Records Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate

Inspection Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item

Sampling for examination Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4 0 (percent defective) and an inspection level of II The unit of product for examination purposes shall be one basin stand

Sampling for tests Sampling for the electrical conductivity test shall be conducted in accordance with MIL-STD-105, with an AQL of 0 (percent defective) and an inspection level of S-4 Sampling for dimensional examination shall be conducted in accordance with MIL-STD-105 with an AQL of 2 5 (percent defective) and an inspection level of S-1 The unit of product for test purposes shall be one basin stand

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Tests Tests shall be conducted to determine compliance with specification requirements Where feasible, the same sample shall be used for the determination of two or more test characteristics

Metric products Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units a request should be made to the contracting officer to determine if the product is acceptable

The contracting officer has the option of accepting or rejecting the product

Contractor certification The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings specifications standards and quality assurance practices The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract

Regulatory requirements

Federal Food Drug and Cosmetic Act If the product covered by this document has been determined by the U S Food and Drug Administration to be under its jurisdiction, the offeror contractor shall comply and be responsible for compliance by its subcontractors/suppliers with the requirements of the Federal Food, Drug and Cosmetic Act as amended and regulations promulgated thereunder In addition the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes ordinances and regulations

Recovered materials The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23 4 to the maximum extent practical

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions handling, etc involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order

Ordering data Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order

NOTES 1 The following National Stock Numbers are covered by this document

6530-00-708-1025 (Type 1)
6530-00-708-1000 (Type 2)

2 The type 1 stand shall be suitable for use with NSN 6530-00-771-0225, Basin, Wash The basin furnished with the type 1 stand shall be in accordance with size II of Commercial Item Description A-A-50814

3 The type 2 stand shall be suitable for use with NSN 6530-00-771-0105, Basin, Wash The two basins furnished with the type 2 stand shall be in accordance with size I of Commercial Item Description A-A-50814

MILITARY INTERESTS

Custodians

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY

DoD-ME

Agent

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES

VA-OSS
USPHS
FDA-MPQAS

Project Number 6530-2145

Location: STANDCID 13A

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1. DOCUMENT NUMBER	2. DOCUMENT TITLE
A-A-54216	STAND, BASIN, (Corrosion-Resisting-Steel)

3a. NAME OF SUBMITTING ORGANIZATION	4. TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
	☐ USER
b. ADDRESS *(Street, City, State, ZIP Code)*	☐ MANUFACTURER
	☐ OTHER *(Specify)*

5. PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6. REMARKS

7a. NAME OF SUBMITTER *(Last, First, MI)* – Optional	b. WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c. MAILING ADDRESS *(Street, City, State, ZIP Code)* – Optional	8. DATE OF SUBMISSION *(YYMMDD)*

DD FORM 82 MAR 1426 PREVIOUS EDITION IS OBSOLETE.

Source: https://assist.dla.mil - Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

DEFENSE LOGISTICS AGENCY

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4956 WASHINGTON D C

POSTAGE WILL BE PAID BY THE DEFENSE LOGISTICS AGENCY

Commander
Defense Personnel Support Center
ATTN DPSC-RSTE
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.