A-A-54219
31 July 1990

COMMERCIAL ITEM DESCRIPTION

CART, SURGICAL DRESSING

(Corrosion-Resisting Steel)

The General Services Administration has authorized the use of this commercial item description as a replacement for Federal Specification AA-C-112D which is cancelled.

This Commercial Item Description covers a corrosion-resisting steel surgical dressing cart.

Salient Characteristics:

The surgical dressing cart shall be fabricated from American Iron and Steel Institute (AISI) Type 302 or Type 304 corrosion-resisting steel. The general design of the cart shall be as shown in figure 1 and as specified herein. Each cart shall consist of four uprights, a top, a shelf, a top guard rail, an adhesive tape bar and cutter, basin and pail supports, a basin, a pail, and two each of swivel and rigid casters. The cart shall rest evenly, without rocking on level surface.

The basin and pail supports shall be located in a fixed position at the end of the cart directly below the top of the cart and directly above the shelf, respectively, or they may be constructed so that the basin swings out from under the top of the cart and the pail slides out from under the shelf. The cart shall be of welded construction throughout.

The four uprights shall be of equal length, made of tubing having a wall thickness of 0.065 inch and an outside diameter of one inch. The top ends shall be closed with

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:31Z
Check the source to verify that this is the current version before use.

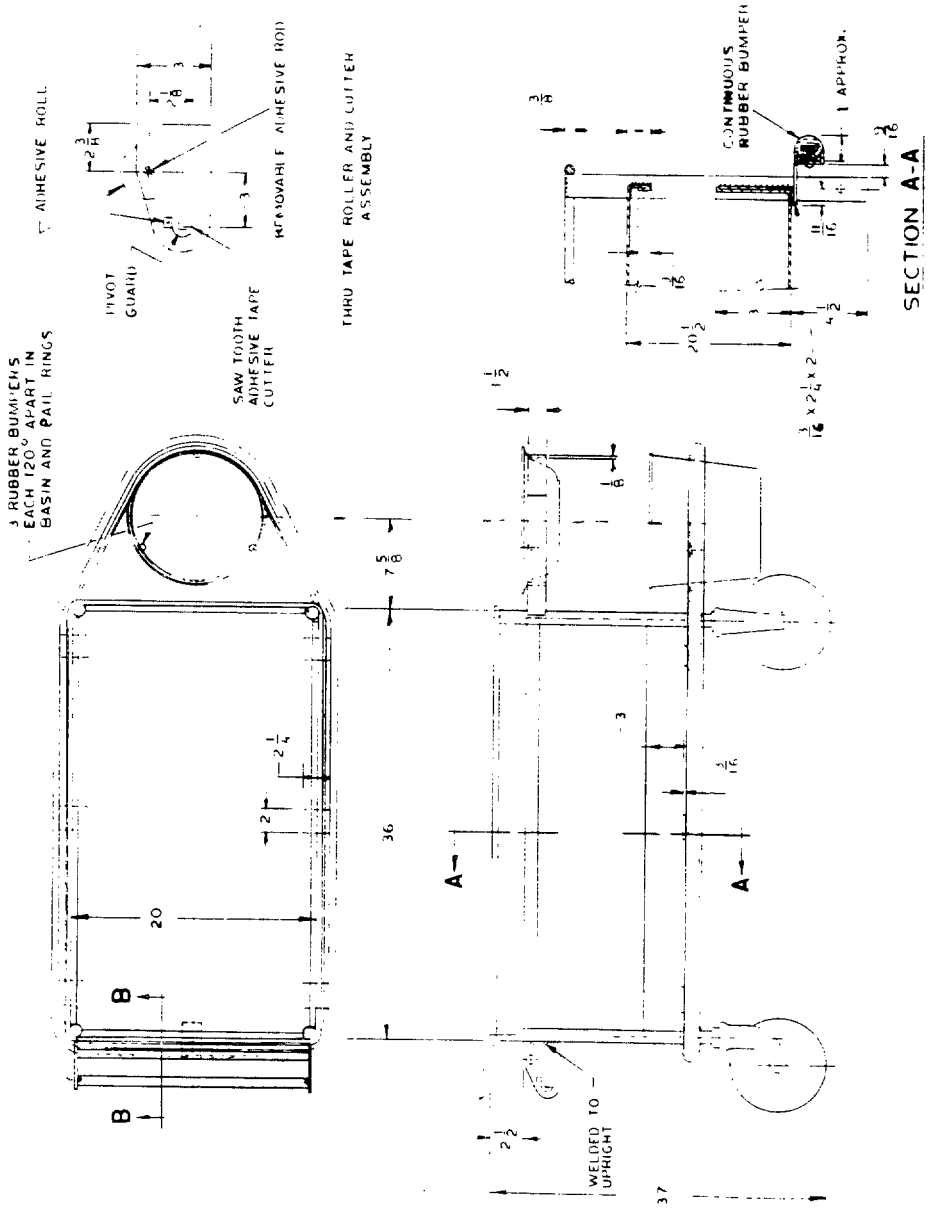


FIGURE 1. Cart, dressing, surgical, corrosion-resisting steel.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

corrosion-resisting steel caps welded smoothly and continuously. The bottom ends shall be fitted with caster mountings to permit replacement of casters.

The dressing cart shall have a top and a pan-type medial shelf each made of corrosion-resisting steel 0.062 inch thick. The corners of the top and shelf shall be notched on 2-1/2 inch radius. The welding shall be continuous on the insides along the intersections of the flanges and uprights. As an alternate to the continuous welding of the insides along the intersections of the flanges and uprights of the medial shelf, the top and outside edges of the intersections of the flanges and uprights shall be continuously welded and the outside facing surfaces of the hemmed shelf edge shall be flared out, welded and polished.

The guardrail shall be made of corrosion-resisting steel rod not less than 3/8 inch in diameter, shall encircle the uprights, flush with the tops of the uprights (see figure 1), and shall be continuously welded (top, bottom, and sides) to each. The welds shall be ground and polished to form a flat surface, flush with the tops of the uprights.

The end of the cart having swivel casters shall be fitted with 1/8 inch thick brackets as indicated in figure 1. The brackets shall incorporate a removable adhesive tape bar, and a tape cutter. The tape bar shall be retained securely in place, but shall be removed easily to install rolls of tape. The brackets shall be butted against and welded to the center of the uprights. Welding to the upright shall be continuous on all contact surfaces. A 3/4 inch by 1/2 inch wide angle, 0.062 inch thick, shall span the brackets and shall be continuously welded to the brackets. A steel saw-toothed adhesive tape cutter suitably plated to resist rust and corrosion shall be secured to the vertical leg of the angle with bolts and acorn nuts. The cutting blade shall be carbon steel having hardened teeth of appropriate number and design to enable it to readily cut adhesive tape brought over its edge with an upward rolling motion in either direction. A hacksaw blade of the correct size shall be an acceptable alternate. A guard 0.062 inch thick shall be loosely pivoted to the brackets, so that in its normal pendant position, it will cover the cutting edge and minimize the danger of injury to personnel using the cart.

Source: https://assist.dla.mil -- Downloaded: 202610-26T09:31Z
Check the source to verify that this is the current version before use.

The pivots shall consist of corrosion-resisting steel rivets suitably spaced with corrosion-resisting steel washers to form smooth and easily working joints. The tape bar shall be corrosion-resisting steel having a diameter of 1/2 inch. The end of the cart having fixed casters shall be fitted with two mounting rings, each formed from a single piece of corrosion-resisting steel. Each mounting ring shall be fitted with three conductive rubber bumpers, equidistantly spaced, securely fastened, but capable of being replaced. The bumpers shall support the utensils and shall prevent rattling while the cart is in motion. The bracket for holding each mounting ring shall be welded flush with the outside surface of the uprights. The weld shall be continuous and shall extend on all contact surfaces of the bracket and uprights. This shall include fillet welds at the ends. Each mounting ring shall be continuously welded at all contact surfaces of the bracket. The upper mounting ring shall be of sufficient diameter to accept the wash basin so that the side of the basin rests against the rubber bumpers. The point of contact between the rubber bumpers and the basin shall be just below the beaded edge and not more than one inch down from the top of the basin. The lower mounting ring shall be of sufficient diameter to accept the pail so that the side of the pail rests against the rubber bumpers. The point of contact between the pail and the bumpers shall be between 2-1/4 inches and 3-1/2 inches of the rim of the pail.

The cart shall be mounted on four ball-bearing casters, two rigid-type casters on one end and two swivel-type on the opposite end. The casters shall conform to class C, 8 inch wheel diameter, style b, mounting as specified in FF-C-77. Caster forks and wheel discs shall be cold rolled steel, chromium, zinc, or cadmium plated. The casters shall be fitted with conductive-rubber tires. The cart shall roll and turn easily on casters.

A basin and a pail, each formed of seamless corrosion-resisting steel, shall be furnished with each cart. The basin shall have a wall thickness of 0.027 inches minimum and a capacity of at least 3-7/8 quarts. The depth of the basin shall not exceed 4-3/4 inches and the diameter shall be such as to provide a stable and secure fit in the upper mounting ring. The pail shall have a wall thickness of 0.015 inch minimum and a capacity of at least twelve quarts.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

The depth of the pail shall be not greater than 10-1/2 inches, and the diameter shall be such as to rest firmly in the lower mounting ring.

All welding shall be done with welding rods of corrosion-resisting steel, similar in composition to the welded members. All visibly exposed welds shall be ground smooth, to eliminate traces of pit marks and seams, and polished to blend with adjacent surfaces.

All exposed corrosion-resisting steel surfaces shall be cleaned and shall be given a No. 4 standard finish (ground and polished). Unexposed welds and surfaces shall be finished in accordance with the best commercial practice. The cart finish shall be free of chipped areas, cracks, scratches, roughness, or tool marks.

The cart, with the casters in place, shall be electrically conductive when tested in accordance with NFPA Standard 99, Health Care Facilities.

Workmanship. The surgical dressing cart shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One cart, as specified, constitutes one unit.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one surgical dressing cart.

Sampling for tests. Sampling for electrical conductivity test shall be conducted in accordance with MIL-STD-105, with an AQL of 0 (percent defective) and an inspection level of S-2. The unit of product for test purposes shall be one surgical dressing cart.

Sampling for tests. Sampling for other tests, including dimensional tests, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 percent defective) and an inspection level of S-2. The unit of product for test purposes shall be one surgical dressing cart.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

NOTE: The following National Stock Number is covered by this document.

6530-00-774-1025

MILITARY INTERESTS:

Custodians:

Army - MD
Navy - MS
Air Force - 03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
USPHS
FDA-MPQAS

Project Number: 6530-2151

Location: CARTCID.13A

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.