A-A-54242
13 September 1990

COMMERCIAL ITEM DESCRIPTION

PROBE, CRYOSURGICAL, STRAIGHT, 1 mm Tip

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a straight probe, with thermocouple, suitable for use in removing cataracts especially those which are intumescent and require greater surface contact.

Salient characteristics:

General. The probe shall be suited for low pressure defrost operation and be comparable with a cryosurgical system specifically designed to operate in such a fashion (See Note 2). The probe is attached tea probe handle in the distal end of the probe delivery line system. This should be attached to the control console using nitrous oxide gas to provide controlled freezing temperatures to -89°C at an operating pressure range of 425 to 625 psi, as regulated by the control console.

Characteristics. The probe shaft shall be 1.8 mm outside diameter. Shaft length shall be 27 mm. The probe shall have 1 mm hemispherical freeze tp protruding beyond the end of the insulating sleeve covering the shaft. The probe and sleeve shall be capable of being flush autoclaved or gas sterilized. The probe shall be protected by a removable probe sheath. The probe delivery line system shall consist of high pressure probe delivery line and a coaxial exhaust line which is flexible. The probe, including the handle, delivery line system, and line exhaust plug, shall be in accordance with Figure 1.

Material. The probe shaft, probe sheath, freeze tip, and handle shall be fabricated from Class 3 austenitic stainless steel in accordance with ASTM Designation F899. The probe sleeve and probe delivery line shall be fabricated of teflon plastic capable of maintaining its flexibility and ability to insulate to -89°C. The coaxial exhaust line shall be fabricated from medical grade silicone rubber.

AMSC N/A FSC 6515

DISTRIBUTION STATEMENT A. Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Low temperatures performance. When the cryosurgical system is operated, it shall be tested for temperature reproductivity and tractive force conformance with ASTM Designation F882.

Workmanship. The cyrosurgical system shall be free from defects which detract from its appearance or impair its serviceability.

Visual and dimensional examination. Probes shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials. The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements.

Unit. Each (EA). One cryosurgical microprobe, as specified, constitutes one unit.

QUALITY ASSURANCE PROVISIONS.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means and chemical properties) of the item.

Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Inspection shall be level S-2. Material and compatibility testing shall be 1.5 % AQL. Performance testing shall be at 1.0% AQL. The unit of product for test purposes shall be one cryosurgical microprobe.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Contract certification. The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerance specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the products is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction , the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and /or order.

NOTE 1: The following National Stock Number is covered by this document:

NSN	Item Description
6515-01-165-6720	PROBE, Cryosurgical, Straight, 1 mm Tip

NOTE 2: The cryosurgical system and control console with which the probe is to be compatible is standardized under National Stock Numbers (NSNs) 6515-01-205-2378 and 6515-00-137-6510.

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order).

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No. 6515-4724

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

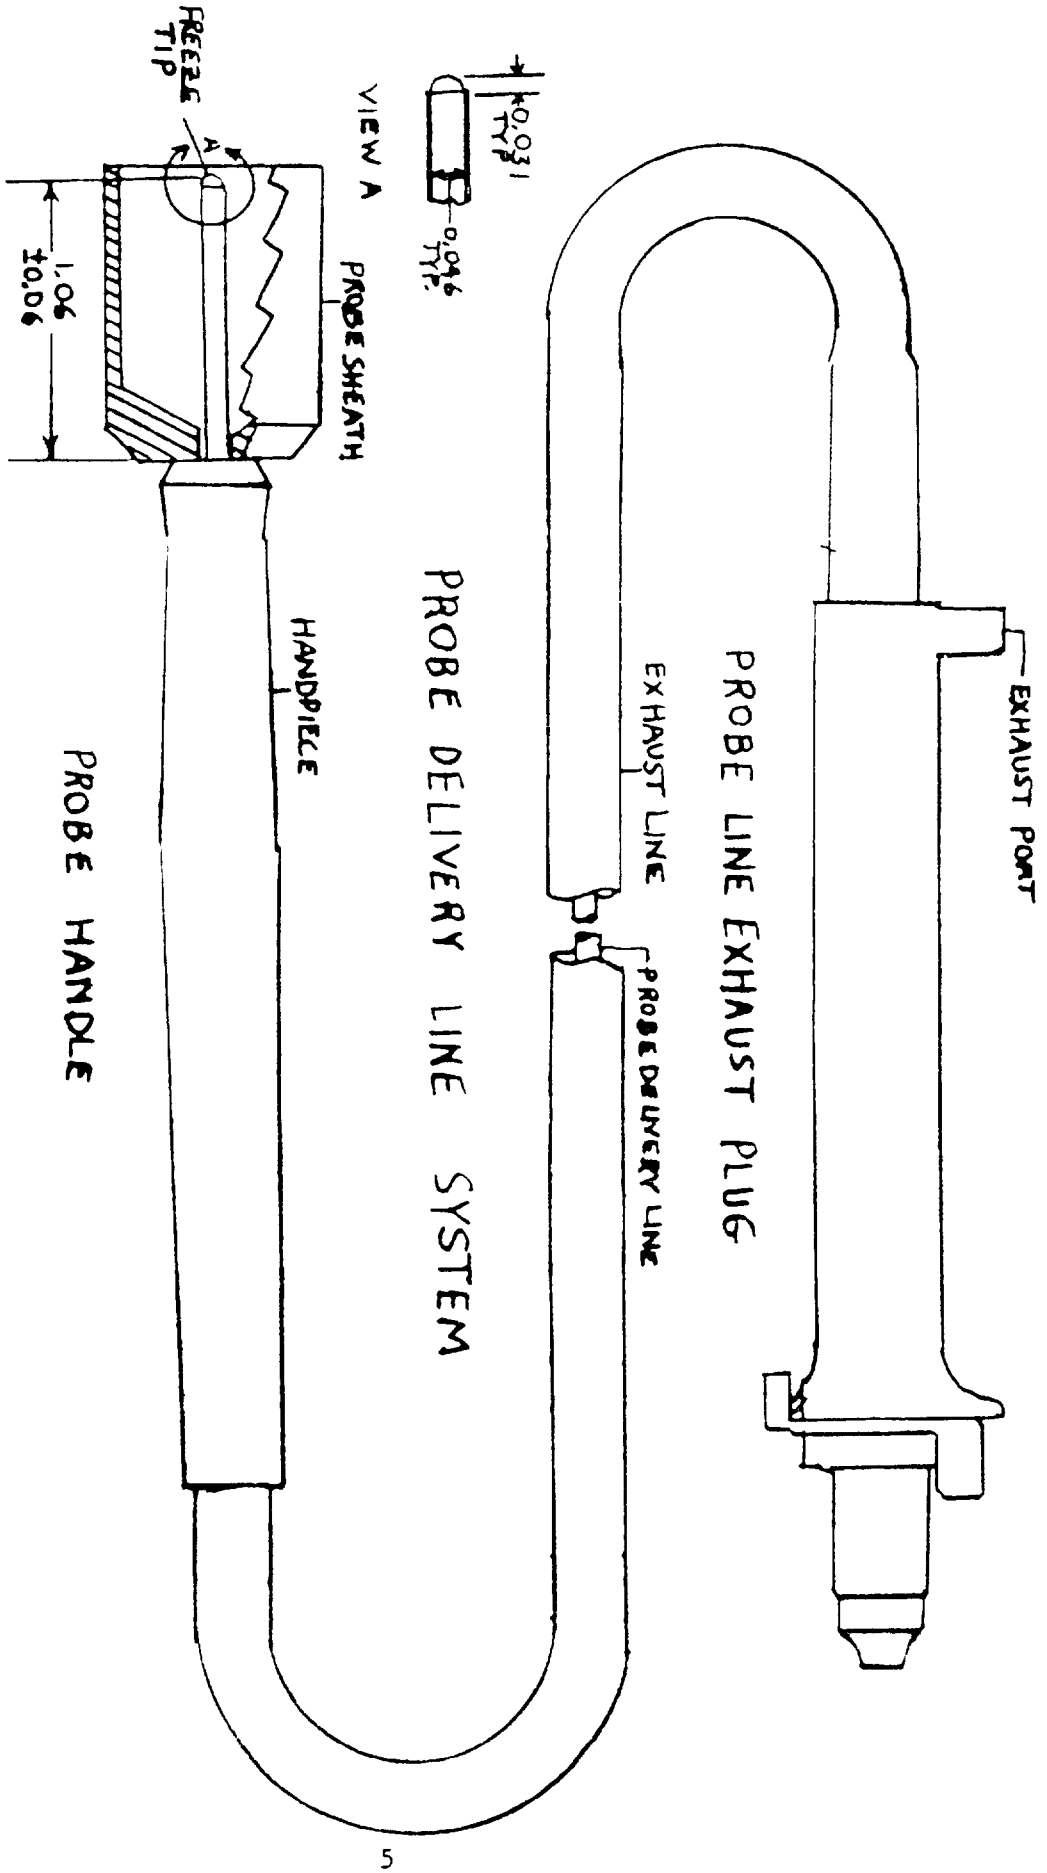


FIGURE 1 PROBE, CRYOSURGICAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems Enter in block 6 any remarks not related to a specific paragraph of the document If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document*(s)* or to amend contractual requirements

(Fold along this line)

(Fold along this line)

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS FORM, CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-54242	PROBE, CRYOSURGICAL, STRAIGHT, 1 mm Tip

3a NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b ADDRESS *(Street City State ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last First MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street City State ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.