A-A-54243
14 September 1990

COMMERCIAL ITEM DESCRIPTION

PROBE, CRYOSURGICAL, MICRO, CURVED, Without Thermocouple, 1 mm Tip

The General Services Administration has authorized the use of this commercial item description.

This commercial item description covers a curved microprobe, without thermocouple suitable for use in the removal of foreign bodies in the vitreous, cataracts, and retrieval of disloaded and sublubricated lenses

Salient characteristics

General The probe shall be suited for low pressure defrost operation and be ccmpatible with a cryosurgical system specifically designed to operate in such a fashion (See Note 2) The probe is attached to a probe handle of the distal end of the probe delivery line system This shall be attached to the with a control console probe line exhaust plug The probe shall be compatible with a cryosurgical system which, as a minimum, consists of a control console using nitrous oxide gas to provide controlled freezing temperatures to -89°C at an operating pressure range of 425 to 625 psi, as regulated by the control console

Characteristics. The probe shaft diameter shall be 1 mm and 1 3 mm outside diameter including the insulating sleeve Shaft length shall be 2.7 mm The probe shall have a 1 mm hemispherical freeze tip protruding beyond the end of the insulating sleeve covering the shaft. The probe and sleeve shall be capable of being flash autoclaved or gas sterilized. The probe shall be protected by a removable probe sheath. The hand piece portion of the probe handle shall be imprinted 'no thermocouple' The probe delivery line system shall consist of a high pressure probe delivery line and a coaxial exhaust line which is flexible. The probe, including the handle, delivery line system, and line exhaust plug, shall be in accordance with Figure 1

AMSC N/A FSC 6515
DISTRIBUTION STATEMENT A Approved for public release; distribution is unlimited

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Material The probe shaft, probe sheath, freeze tip, and handle shall be fabricated from Class 3 austenitic stainless steel in accordance with ASTM Designation F899.

The probe sleeve and probe delivery line shall be fabricated of teflon plastic capable of maintaining its flexibility and ability to insulate to -89°C. The coaxial exhaust line shall be fabricated from medical grade silicone rubber

Low temperatures performance. When the cryosurgical system is operated, it shall be tested for temperature reproductivity and tractive force conformance with ASTM Designation F882

PRODUCT QUALITY LEVEL

Visual and dimensional examination Shall be examined to verify that design, construction and workmanship are in accordance with applicable requirements.

Materials The supplier shall be responsible for performing tests to assure that materials are in accordance with requirements

Unit Each (EA) One cryosurgical microprobe, as specified, constitutes one unit

QUALITY ASSURANCE PROVISIONS

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Inspection Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means and chemical properties) of the item

Tests Tests shall be conducted to determine compliance with specification requirements Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Sampling for tests Sampling for tests shall be conducted in accordance with MIL-STD-105 and as specified herein. Inspection shall be level S-2 Material and compatibility testing shall be 1 5 % AQL Performance testing shall be at 1 0% AQL The unit of product for test purposes shall be one cryosurgical microprobe

Contract certification The contractor shall certify that the product offered meets the salient characteristics of this description and conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The Government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract

Metric products Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard No. 376, and all other requirements of this document are met

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch/pound units, a request should be made to the contracting officer to determine if the product is acceptable

The contracting officer has the option of accepting or rejecting the product

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Regulatory requirements.

Federal Food, Drug, and Cosmetic Act. If the product covered by this document has been determined by the U S Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal State, and local statutes, ordinances, and regulations

Recovered materials The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23 4 to the maximum extent practical

Preservation, packaging, packing, labeling, and marking Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and /or order

NOTE 1· The following National Stock Number is covered by this document·

NSN	Item Description
6515-01-139-7674	PROBE, Cryosurgical, Micro, Curved, Without Thermocouple, 1mm Tip

NOTE 2: The cryosurgical system and control console with which the probe is to be compatible is standardized under National Stock Numbers (NSNs) 6515-01-205-2378 and 6515-00-137-6510

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Ordering data (Intermediate/exterior package quantities and labeling and marking must be specified in the contract and/or order)

MILITARY INTERESTS:

Custodians:

Army-MD
Navy-MS
Air Force-03

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

VA-OSS
PHS
FDA-MPQAS

Project No 6515-4724

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

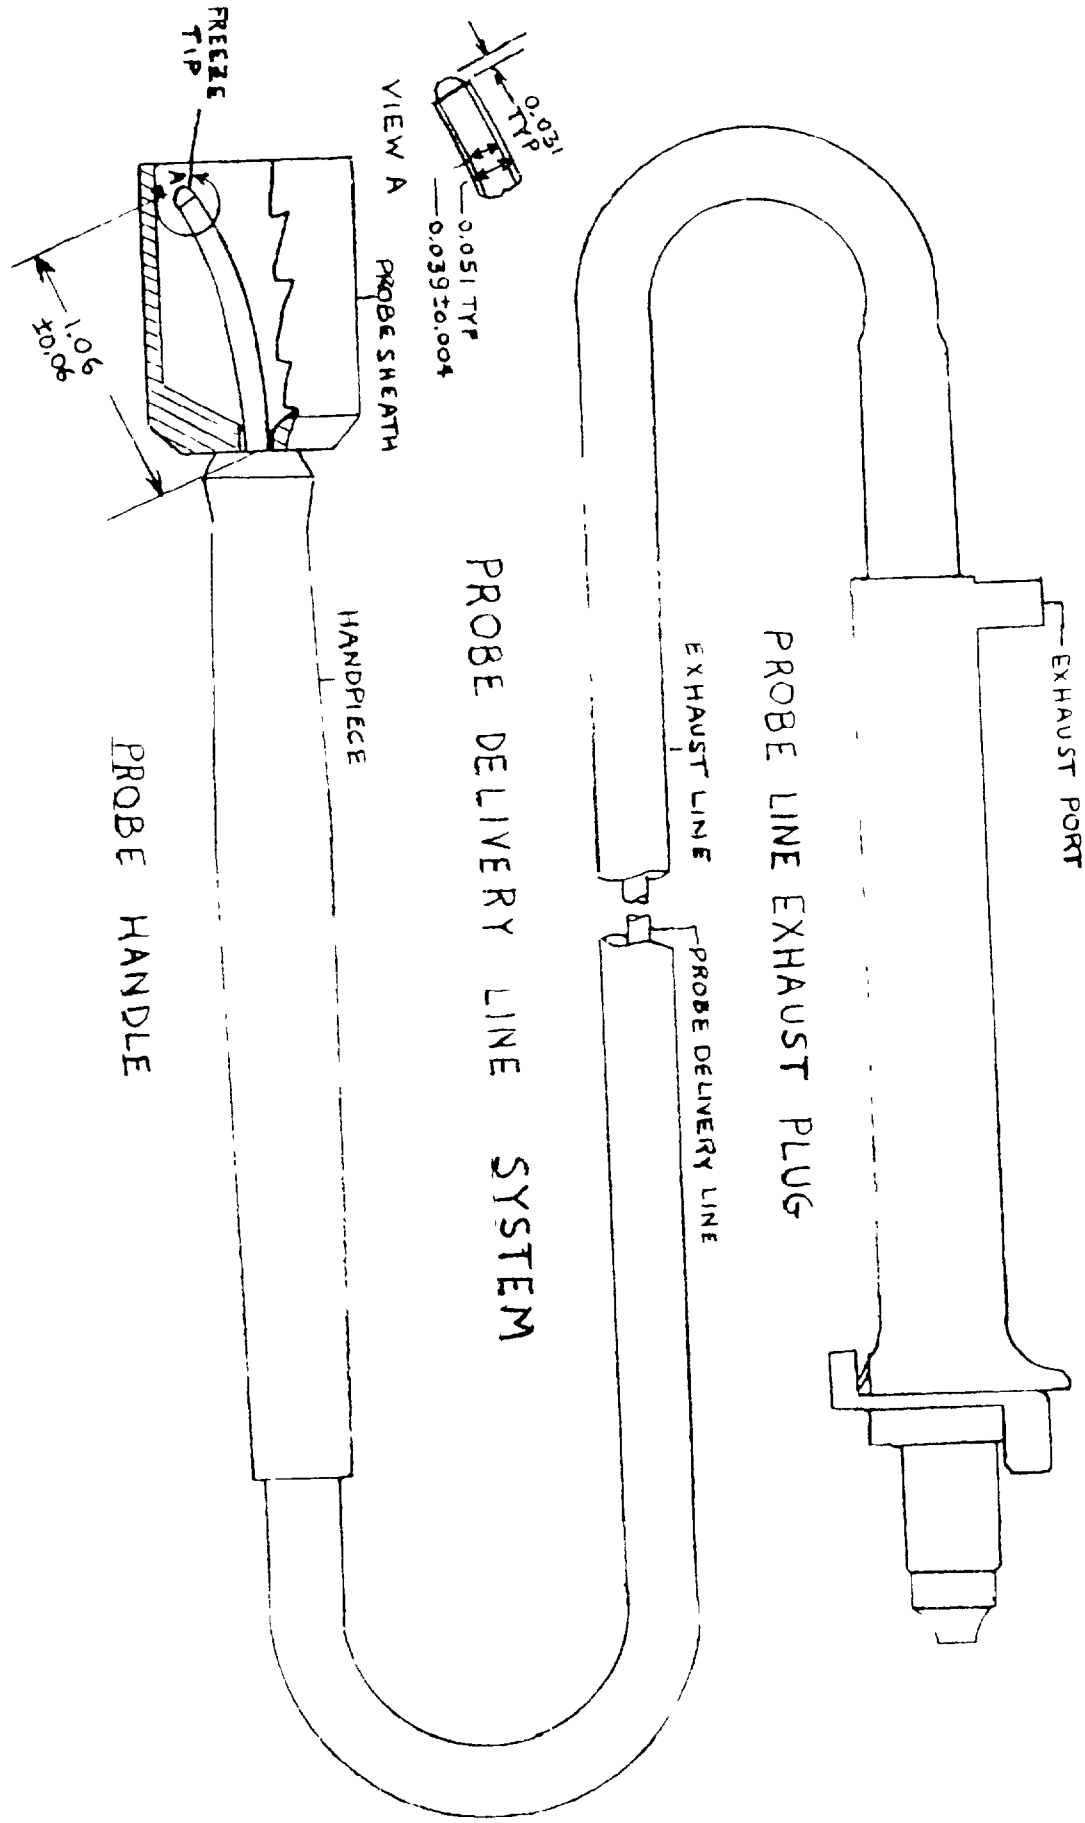


FIGURE 1 PROBE, CRYOSURGICAL

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

(TO DETACH THIS F ', CUT ALONG THIS LINE.)

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

(See Instructions – Reverse Side)

1 DOCUMENT NUMBER	2 DOCUMENT TITLE
A-A-54243	PROBE, CRYOSURGICAL, MICRO, CURVED, Without Thermocouple, 1 mm Tip

3a. NAME OF SUBMITTING ORGANIZATION	4 TYPE OF ORGANIZATION *(Mark one)*
	☐ VENDOR
b ADDRESS *(Street City State ZIP Code)*	☐ USER
	☐ MANUFACTURER
	☐ OTHER *(Specify)* _____

5 PROBLEM AREAS

a. Paragraph Number and Wording

b. Recommended Wording

c. Reason/Rationale for Recommendation

6 REMARKS

7a NAME OF SUBMITTER *(Last First MI)* – Optional	b WORK TELEPHONE NUMBER *(Include Area Code)* – Optional
c MAILING ADDRESS *(Street City State ZIP Code)* – Optional	8 DATE OF SUBMISSION *(YYMMDD)*

DD FORM 1426 PREVIOUS EDITION IS OBSOLETE

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

INSTRUCTIONS In a continuing effort to make our standardization documents better, the DoD provides this form for use in submitting comments and suggestions for improvements. All users of military standardization documents are invited to provide suggestions. This form may be detached, folded along the lines indicated, taped along the loose edge *(DO NOT STAPLE)*, and mailed. In block 5, be as specific as possible about particular problem areas such as wording which required interpretation, was too rigid, restrictive, loose, ambiguous, or was incompatible, and give proposed wording changes which would alleviate the problems. Enter in block 6 any remarks not related to a specific paragraph of the document. If block 7 is filled out, an acknowledgement will be mailed to you within 30 days to let you know that your comments were received and are being considered.

NOTE This form may not be used to request copies of documents, nor to request waivers, deviations, or clarification of specification requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

(Fold along this line)

(Fold along this line)

OFFICIAL BUSINESS
PENALTY FOR PRIVATE USE $300

NO POSTAGE NECESSARY IF MAILED IN THE UNITED STATES

BUSINESS REPLY MAIL
FIRST CLASS PERMIT NO 4966 Alexandria, VA

POSTAGE WILL BE PAID BY

Commander
Defense Personnel Support Center
ATTN: DPSC-RSTS
2800 South 20th Street
Philadelphia, Pennsylvania 19101-8419

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.