INCH-POUND

A-A-54255A
31 May 1994
SUPERSEDING
A-A-54255
17 September 1990

COMMERCIAL ITEM DESCRIPTION

TABLE, EXAMINING AND TREATMENT

(Steel, Cabinet Type)

The General Services Administration has authorized the use of this Commercial Item Description.

This Commercial Item Description covers a steel, cabinet type, examining and treatment table with upholstered top.

Salient characteristics:


Style and design. The examining and treatment table shall be a cabinet type with an adjustable two-section upholstered top suitable for use in medical treatment facilities.


The table shall be generally designed as shown in figure 1. The upholstered top shall consist of a head section and a seat section. A one piece top consisting of head and foot section shall be acceptable. The seat section shall have a suitable perineal cutout. The seat section shall be capable of being raised, or shall have tapered extra padding for patient comfort in the chair position. The head section shall have a raised portion that serves as a pillow. The head section shall contain a concealed paper roll attachment to accommodate a paper roll 3-1/2 inches in diameter by 18 inches wide. A combination restraining strap and paper cutter shall be provided on the top of the table. This may be in the form of an extruded vinyl strip and may be located anywhere on the table's upper surface.

AMSC N/A FSC 6530

DISTRIBUTION STATEMENT A: Approved for public release; distribution is unlimited.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

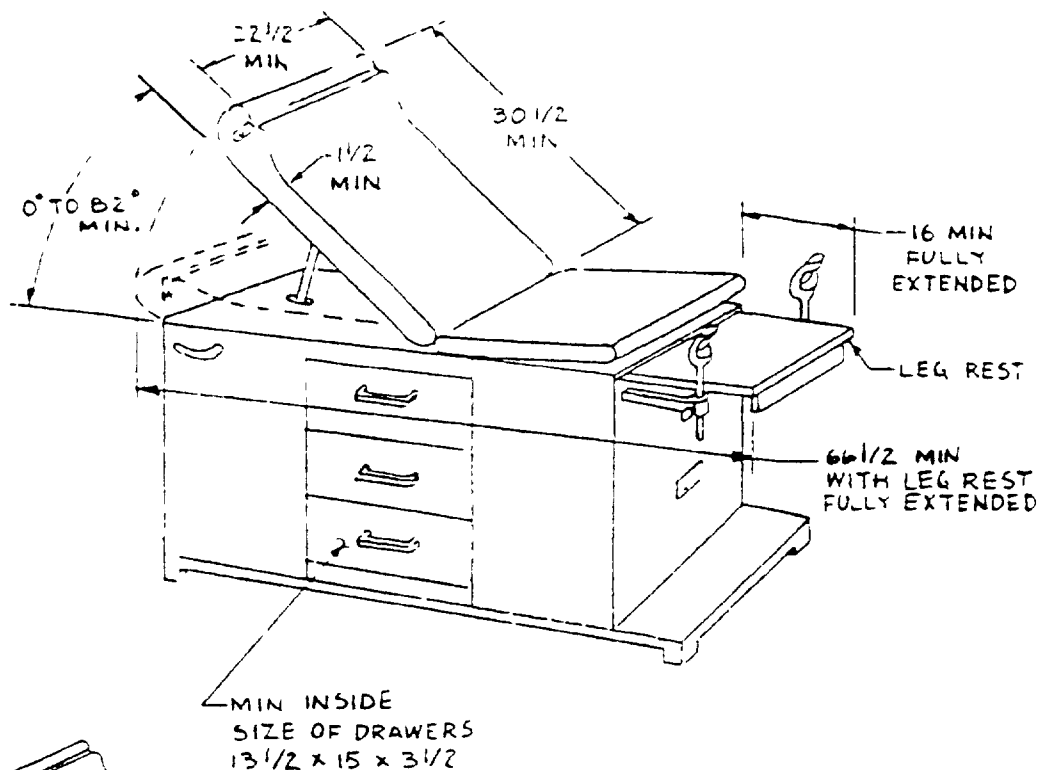

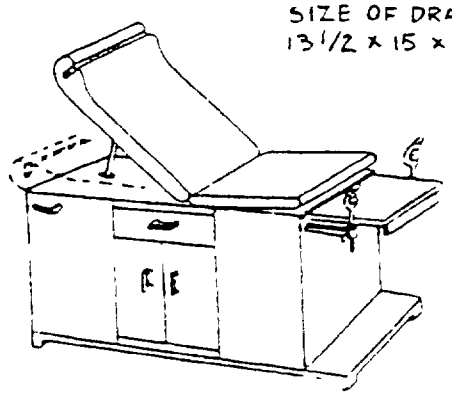

ALTERNATE STORAGE CONFIGURATION

NOTES:
1. DRAWING FOR GENERAL STYLE AND DESIGN. LOCATION OF COMPONENTS IS FOR GUIDANCE ONLY.
2. ALL DIMENSIONS IN INCHES UNLESS OTHERWISE SPECIFIED

FIGURE 1 Table. (Typical configuration)

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

The cabinet shall be fabricated of sheet steel and shall be supported by legs or by other means at the four bottom corners. Means of adjusting the supports to accommodate uneven floors shall be provided. As an alternate, the cabinet body shall be secured by bolts or welding to a base supported by adjustable glides.

As a minimum the cabinet shall contain a drawer and a storage compartment or, as an alternate, shall contain three drawers. The storage compartment door(s) shall be of double wall construction. Each door shall have a knob or a handle and a suitable device to hold it closed. The drawers shall be fabricated of metal, high strength plastic, or other suitable materials. Each drawer shall have a suitable pull for opening. Doors and drawer fronts, when metal, shall be filled with sound deadening material. Plastic drawers with particle board fronts, covered on all surfaces with plastic laminate, shall be acceptable.

The seat end of the cabinet body shall contain two stirrups, an upholstered pullout leg rest, and a dual electrical outlet. The electrical outlet may be located on either side of the table. The outlet shall be attached to a 3-conductor power cord a minimum of 10 feet long terminated in a 3-prong male, hospital grade plug. The lower section of the leg rest shall be provided with a treatment basin. The stirrups shall be swivel type, offering a minimum of three lateral and easily locked positions. Stirrups which are both laterally and vertically adjustable shall be an acceptable alternate. A suitable mounting step of the fixed type shall be provided at the seat end of the table. As an alternate, a retractable step shall be provided. The trend area of the step shall be covered with a grained or ribbed rubber, or equal, mat.

The head and seat sections shall be padded with urethane foam and upholstered with vinyl.

Materials. The cabinet body, drawer fronts, and door fronts shall be fabricated from suitable carbon steel sheet having a minimum thickness of 0.0359 inch.

Drawers shall be one piece molded of a high strength plastic Sheet steel constructed drawers shall also be acceptable.

Padding shall be urethane foam with a density of 2.55 to 2.7 pounds per cubic foot. Foam shall meet the flame retardance requirements of California Technical Bulletin 117.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Upholstery shall consist of a base layer of cloth with a vinyl wear layer and a sublayer of expanded vinyl foam. The wear layer shall have a leather grain surface. The colored vinyl shall be given a 4 mil (0.004) clear vinyl overcoat. Minimum weight per square yard shall be 21 ounces. Tensile strength in both the warp and filler direction shall not be less than 67 pounds. As an alternate the top shall be vacuum formed consisting of urethane fire-retardant foam with a density of 1.8 to 5.2 pounds per cubic foot covered with a vinyl skin with an outer wear layer, a middle layer of expanded vinyl and an inner vinyl layer.

The stirrups shall be fabricated of a suitable metallic alloy and finished in a manner that provides a durable professional appearance.

The table top substructure for the head, seat, and leg pullout shall be fabricated form either plywood or particle board not less than 3/4 thick. As an alternate, steel shall be acceptable for the substructure. One half inch particle board shall be acceptable for the leg pullout substructure only.

All hardware and other metal parts shall be fabricated from suitable corrosion-resistant metals.

All parts not specified shall be fabricated of materials generally commercially recognized as suitable for the intended purpose.

Finish. All sheet steel parts and other steel parts except corrosion-resisting steel and plated steel shall be cleaned, primed, and powder coated with an epoxy based paint. The color shall be the manufacturer's standard color and shall produce a pleasing professional appearance in combination with the upholstery color. As an alternate to epoxy powder coat, two coats of baked on alkyd enamel with a final texture finish shall be acceptable. Appropriate cleaning and priming operations shall precede enamel coating.

The stirrups shall be finished by chrome plating or powder coated with an epoxy paint.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Door and handles, knobs, and like hardware shall be plated or otherwise finished to provide corrosion resistance, durability, and a pleasing appearance. All other hardware shall be plated to provide corrosion-resistance.

Performance. The table shall support a load of 350 pounds with no apparent or permanent deflection. The head section in all raised positions shall not collapse or move when a load of 125 pounds is applied perpendicular to the plane of the section and 12 inches from the head end. The seat section shall support a load of 250 pounds in all raised positions.

The head section shall be fully adjustable through 82 degrees from the horizontal position. The head section shall lock securely at any point.

The stirrups shall adjust through a range of up to 18 inches from the seat end of the table. At their maximum horizontal and vertical positions, the stirrups shall be capable of withstanding a 50 pound force applied perpendicular to the heel support section of the stirrup.

The step shall support 250 pounds without any sign of distortion.

The drawers shall open easily and smoothly and shall be restrained from coming all of the way out to prevent accidents.

The power cord shall be capable of withstanding a pull of 35 pounds without pulling out of the strain relief or putting tension on the connections at the outlet.

The table shall show no signs of breakdown when subjected to the dielectric strength test as specified in Underwriters Laboratory Standard UL 544.

Manuals. Each table shall be furnished with two copies of a technical manual that contains complete instructions for installation, operation, maintenance, cleaning, and a list of component parts.

Workmanship. The table shall be free from defects which detract from its appearance or impair its serviceability.

Unit. Each (EA). One table, as specified, constitutes one unit.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Quality Assurance Provisions.

Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the contractor is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or purchase order, the contractor may use his own or any facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government The Government reserves the right to perform any of the inspections set forth in the specification where such inspections are deemed necessary to assure supplies and services conform to prescribed requirements.

Records. Records of examinations and tests performed by or for the contractor shall be maintained by the contractor and made available to the Government upon the Government's request, at any time, or from time to time, during the performance of the contract and for a period of three years after delivery of the supplies to which such records relate.

Inspection. Inspection, as used herein, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties) of the item.

Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105, with an AQL of 4.0 (percent defective) and an inspection level of II. The unit of product for examination purposes shall be one examining and treatment table.

Sampling for tests. Sampling for tests, including dimensional test, shall be conducted in accordance with MIL-STD-105, with an AQL of 2.5 (percent defective) and an inspection level of S-1. The unit of product for test purposes shall be one examining and treatment table.

Tests. Tests shall be conducted to determine compliance with specification requirements. Where feasible, the same sample shall be used for the determination of two or more test characteristics.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Metric products. Products manufactured to metric dimensions will be considered on an equal basis with those manufactured using inch-pound units, providing they fall within the tolerances specified using conversion tables contained in the latest revision of Federal Standard 376, and all other requirements of this document are met.

If a product is manufactured to metric dimensions and those dimensions exceed the tolerances specified in the inch-pound units, a request should be made to the contracting officer to determine if the product is acceptable.

The contracting officer has the option of accepting or rejecting the product.

Contractor certification. The contractor shall certify and maintain substantiating evidence that the product offered meets the salient characteristics of this Commercial Item Description, and that the product conforms to the producers' own drawings, specifications, standards, and quality assurance practices. The government reserves the right to require proof of such conformance prior to first delivery and thereafter as may be otherwise provided for under the provisions of the contract.

Regulatory requirements.

Federal Food, Drug and Cosmetic Act. If the product covered by this document has been determined by the U.S. Food and Drug Administration to be under its jurisdiction, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of the Federal Food, Drug and Cosmetic Act, as amended, and regulations promulgated thereunder. In addition, the offeror/contractor shall comply, and be responsible for compliance by its subcontractors/suppliers, with the requirements of all other applicable Federal, State, and local statutes, ordinances, and regulations.

Recovered materials. The offeror/contractor is encouraged to use recovered material in accordance with Federal Acquisition Regulation Subpart 23.4 to the maximum extent practical.

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

Preservation, packaging, packing, labeling, and marking. Unless otherwise specified, preservation, packaging, and packing shall be to a degree of protection to preclude damage to containers and/or contents thereof under normal shipping conditions, handling, etc., involving shipment from the supply source to the receiving activity, plus reshipment from receiving activity, and shall conform to applicable carrier's rules and regulations. Intermediate and exterior package quantities and labeling and marking shall be as specified in the contract and/or order.

Ordering data. Intermediate/exterior package quantities, labeling, and marking must be specified in the contract and/or order.

NOTE: The following National Stock Number is covered by this document.

6530-01-351-9319

MILITARY INTERESTS:

Custodians:

Air Force - 03
Army - MD
Navy - MS

PREPARING ACTIVITY:

DoD-MB

Agent:

DLA-DM

CIVIL AGENCY COORDINATING ACTIVITIES:

FDA-MPQAS
USPHS
VA-OSS

Project Number: 6530-2415

Location: TABL13C.DOC

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.

STANDARDIZATION DOCUMENT IMPROVEMENT PROPOSAL

INSTRUCTIONS

1. The preparing activity must complete blocks 1, 2, 3, and 8. In block 1, both the document number and revision letter should be given.
2. The submitter of this form must complete blocks 4, 5, 6, and 7.
3. The preparing activity must provide a reply within 30 days from receipt of the form.

NOTE: This form may not be used to request copies of documents, nor to request waivers, or clarification of requirements on current contracts. Comments submitted on this form do not constitute or imply authorization to waive any portion of the referenced document(s) or to amend contractual requirements.

I RECOMMEND A CHANGE:	1. DOCUMENT NUMBER	2. DOCUMENT DATE (YYMMDD)
	A-A-54255A	940531

3. DOCUMENT TITLE
TABLE, EXAMINING AND TREATMENT (Steel, Cabinet Type)

4. NATURE OF CHANGE (Identify paragraph number and include proposed rewrite, if possible. Attach extra sheets as needed.)

5. REASON FOR RECOMMENDATION

6. SUBMITTER

(a) NAME (Last, First, Middle Initial)	(b) ORGANIZATION	
(c) ADDRESS (Include Zip Code)	(d) TELEPHONE (Include Area Code) (1) Commercial (2) AUTOVON (If applicable)	(e) DATE SUBMITTED (YYMMDD)

7. PREPARING ACTIVITY

a. NAME	b. TELEPHONE (Include Area Code)	
Defense Personnel Support Center ATTN: DPSC-MSE	(1) Commercial 215-737-2870	(2) AUTOVON 444-2870
c. ADDRESS (Include Zip Code) 2800 South 20th Street Philadelphia, PA 19145	IF YOU DO NOT RECEIVE A REPLY WITHIN 45 DAYS, CONTACT Defense Quality and Standardization Office 5203 Leesburg Pike Suite 1403, Falls Church, VA 22041-3466 Telephone (703) 756-2340 AUTOVON 289-2340	

DD Form 1426, OCT 89 Previous editions are obsolete. 98

Source: https://assist.dla.mil -- Downloaded: 2026-10-26T09:31Z
Check the source to verify that this is the current version before use.