MILITARY SPECIFICATION

TEMPLATE, DENTAL

This specification is mandatory for use by all Departments and Agencies in the Department of Defense.

1. SCOPE

1.1 Scope. This specification covers a dental template suitable for use in properly positioning 20-degree posterior teeth during prosthetic setup.

2. APPLICABLE DOCUMENTS

2.1 Specifications and standards. The following documents, of the issue in effect on date of invitations for bid or requests for proposal, form a part of this specification to the extent specified herein:

SPECIFICATIONS

Federal

PPP-B-566	Boxes, Folding, Paperboard.
PPP-B-585	Boxes, Wood, Wirebound.
PPP-B-601	Boxes, Wood, Cleated-Plywood.
PPP-B-621	Boxes, Wood, Nailed and Lock-Corner.
PPP-B-636	Box, Fiberboard.
PPP-B-676	Boxes, Setup.

STANDARDS

Military

MIL-STD-105	Sampling Procedures and Tables for Inspection by Attributes.
MIL-STD-129	Marking for Shipment and Storage.

Source: https://assist.dla.mil -- Downloaded: 202610-21T08:56Z
Check the source to verify that this is the current version before use.

(Copies of specifications and standards required by suppliers in connection with specific procurement functions should be obtained from the procuring activity or as directed by the contracting officer.)

3. REQUIREMENTS

3.1 Material. The template shall be fabricated from No. 16 Brown and Sharpe gage (0.0508 inch) brass sheet.

3.2 Style, design, and dimensions. The dental template shall be suitable for use as a setup guide in positioning upper, 20-degree posterior teeth, so that the axis and cusps of the teeth are in proper relationship to the occlusal plane. The template shall conform to Figure 1 for style, design, and dimensions. When initially formed, the curvature of the entire template shall be that of a segment of a 12 ± 1 inch sphere. The anterior region shall be further contoured and stamped with the instructions for use specified in 3.5.

3.3 Plating. The template shall be either chrome-over-nickel or nickel plated. The plating shall be firmly attached to the brass.

3.4 Finish. The template shall have a smooth satin or bright finish.

3.5 Instructions for use. The directions for use shall be die-stamped on the anterior portion of the template, and shall read: "For 20° posteriors. Raise lingual cusps of 1st and 2nd upper bicuspids 1 mm. All other cusps touch".

3.6 Workmanship. Workmanship shall be first class throughout. The template shall be free from defects which detract from its appearance or may impair its serviceability.

4. QUALITY ASSURANCE PROVISIONS

4.1 Responsibility for inspection. Unless otherwise specified in the contract or purchase order, the supplier is responsible for the performance of all inspection requirements as specified herein. Except as otherwise specified in the contract or order, the supplier may use his own or any other facilities suitable for the performance of the inspection requirements specified herein, unless disapproved by the Government. The Government reserves the right to perform any of the inspections set forth in this specification where such inspections are deemed necessary to assure that supplies and services conform to prescribed requirements.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.

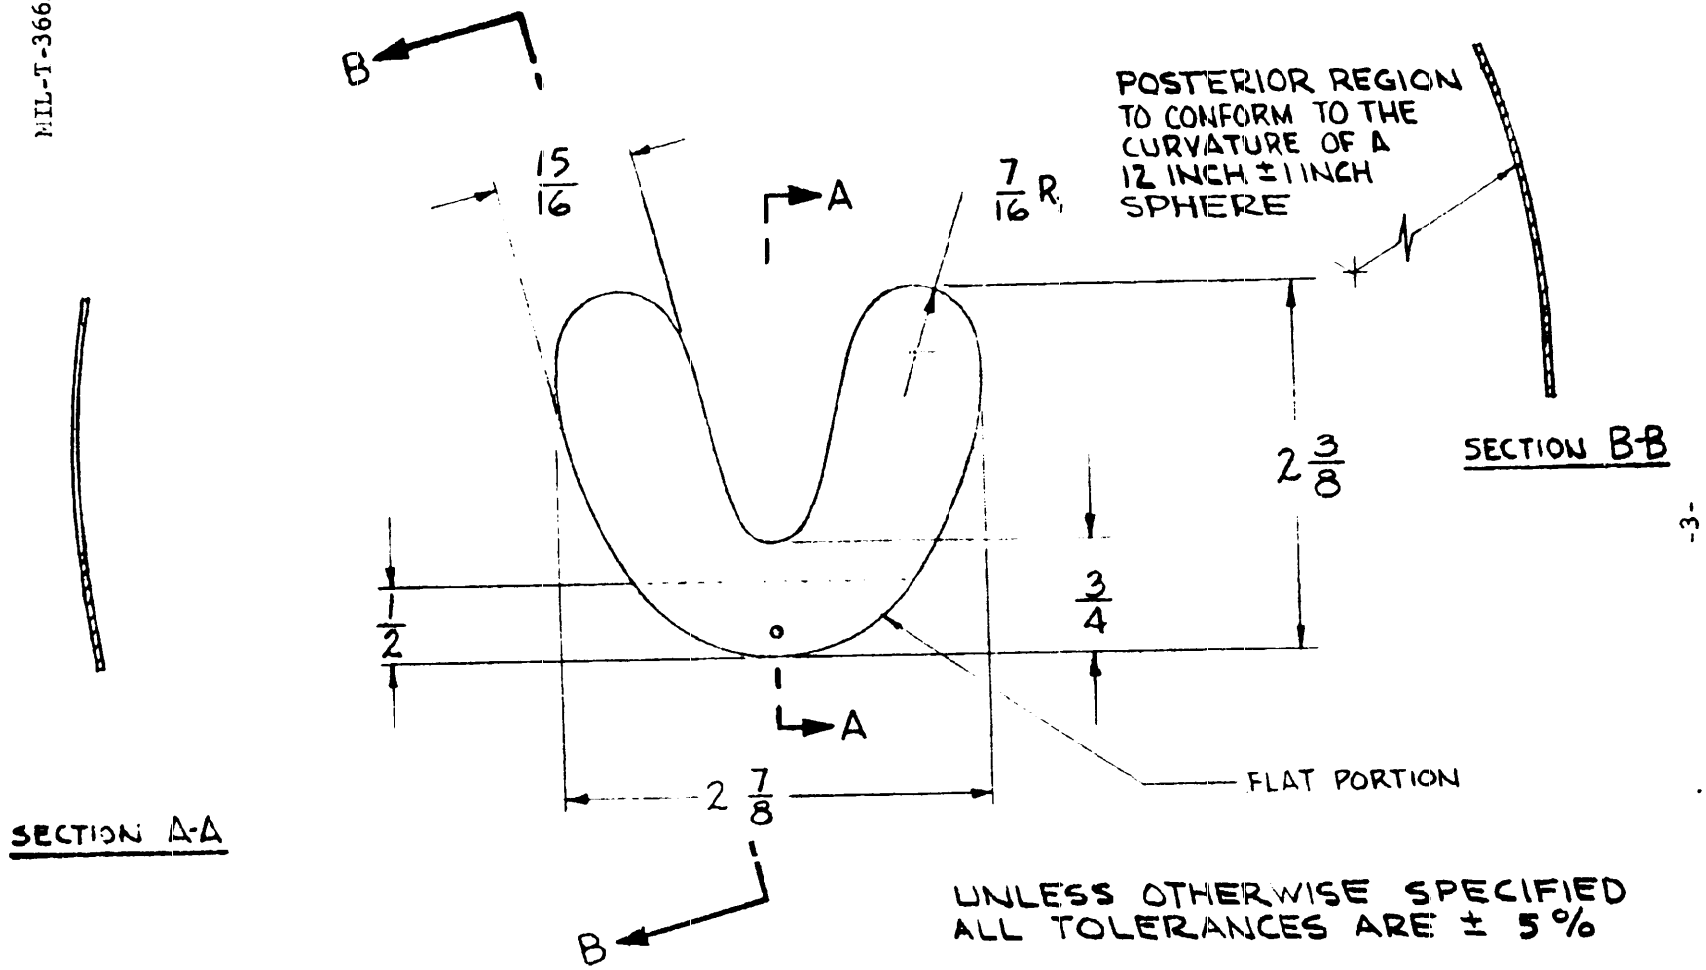


FIGURE 1

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.

4.1.1 Inspection. Inspection, as used in this specification, is defined as both examination (such as visual or auditory investigation without the use of special laboratory appliances or procedures) and testing (determination by technical means of physical and chemical properties).

4.1.2 Certificates of quality. Certificates of quality, supplied by the manufacturer of the material may be furnished in lieu of actual performance of such testing by the contractor, provided that lot identity has been maintained and can be demonstrated to the Government. The Certificate shall include the name of the contractor, the contract number, the name of the manufacturer or supplier, the FSN, the Item Identification, the name of the material, the date of testing, the test method, individual test results, and the specification requirements.

4.2 Quality conformance inspection. The examinations and tests required to assure conformance of those items or lots of items to be offered are classified as specified in tables I and II (see 4.2.1 and 4.3).

4.2.1 Sampling for examination. Sampling for examination shall be conducted in accordance with MIL-STD-105. The inspection levels and acceptable quality levels (AQL's) shall be as indicated in table I. Unit of product for examination purposes shall be one template.

Table I. Sampling for Examination

Type defect	Inspection level	AQL (percent defective
Major	II	1.0
Minor A	II	2.5
Minor B	S-2	4.0

4.2.2 Sampling for tests. Sampling for tests shall be conducted in accordance with MIL-STD-105. Unit of product for test purposes shall be one template.

4.3 Examination. The template shall be examined for the possible defects listed in table II. Examination shall not be restricted to the classified defects listed in the table.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.

Table II. Classification of Defects

Category	Defects
Major:	
101	Surface of template not free from corrosion, discoloration, or deep pits.
102	Instructions for use not as specified, or instructions missing.
103	Style and design not in accordance with figure 1.
104	Plating not firmly attached to brass so that it flakes off; or there is no plating at all.
Minor A:	
201	Finish not satin or bright.
202	Finish not free from coarse grind marks.
203	Template not free from dirt, oil, or other foreign matter.
204	Packaging and packing not as specified.
205	Marking on packaging and pack illegible, incomplete, improper, or missing altogether.
Minor B:	
251	Any dimension not as shown in figure 1.

4.4 Test procedure.

4.4.1 Presence of plating. The presence of nickel plating or chromium-over-nickel plating on the brass template shall be determined using a suitable spot test kit (see 6.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.

5. PREPARATION FOR DELIVERY

5.1 Packaging.

5.1.1 Unit of issue. One template, as specified, constitutes one unit of issue.

5.1.2 Packaging quantities. The number of units of issue indicated in table III shall be packaged in each unit, intermediate, and exterior container, as applicable, for the required level of protection specified in the procurement document.

Table III. Packaging Quantities

Unit package	Intermediate package	Exterior container
1 unit	12 units	576 units

5.1.2.1 Variation permitted. If the required number of units in the entire shipment is less than the number of units specified to be overpacked in an exterior container, such units may be packed in an exterior container of suitable size and design, acceptable to a common carrier, which shall insure safe delivery to destination.

5.1.3 Level A.

5.1.3.1 Unit package. Each unit shall be packaged in an envelope of suitable size and design. Closure shall be adequate to prevent accidental opening.

5.1.3.2 Intermediate package. Intermediate package shall be a box of appropriate size and design, constructed in accordance with PPP-B-566 or PPP-B-676, except that commercial colors will be acceptable; or PPP-B-636, type CF, class domestic. Closure shall be adequate to prevent accidental opening under normal handling.

5.1.4 Level C. Units shall be packaged in standard commercial containers, of the size and kind commonly used, which will afford the degree of protection required for shipment and use of the product for its intended purpose.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.

5.2 Packing.

5.2.1 Level A.

5.2.1.1 Exterior container. Exterior container shall be designed for a type 2 load and shall be constructed in accordance with PPP-B-585, class 3, style 3; PPP-B-601, overseas type; PPP-B-621, class 2; or PPP-B-636, class weather-resistant, grade V3. Closure and strapping shall be as specified in the appendix of the applicable box specification.

5.2.2 Level B.

5.2.2.1 Exterior container. Exterior container shall be designed for a type 2 load and shall be constructed in accordance with PPP-B-585, class 1, style 3; PPP-B-601, domestic type; PPP-B-621, class 1; or PPP-B-636, class domestic. Closure shall be as specified in the appendix of the applicable box specification.

5.2.3 Level C. The subject commodity shall be packed in substantial commercial containers, of the type, size, and kind commonly used for the purpose, so constructed as to insure acceptance and safe delivery by common or other carriers, at the lowest rate, to point of delivery called for in the contract or purchase order.

5.3 Marking.

5.3.1 Interior packages. Each unit package and each intermediate package shall be marked in accordance with MIL-STD-129. When labels are utilized, waterproofing shall be required only when applicable carton is fabricated of water-resistant material. Contract or purchase order number and name of contractor shall be shown.

5.3.2 Exterior container. Exterior container shall be marked in accordance with MIL-STD-129.

6. NOTES

6.1 Ordering data. Procurement documents should specify the following:

(a) Title, number, and date of this specification.
(b) Selection of applicable levels of packaging and packing (see 5.1 and 5.2).

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.

6.2 Spot test kit. A spot test outfit, suitable for determining the presence of nickel and chromium, is manufactured by British Drug Houses, Ltd., and is available from Arthur H. Thomas and Company, Philadelphia, Pa.

6.3 Specification coverage. This document covers the requirements for FSN 6520-561-3700, TEMPLATE, DENTAL.

6.4 Supersession data. This document supersedes Military Medical Purchase Description #3 dated 11 April 1968.

6.5 Limitations. This specification does not cover all types, classes, grades, styles, or sizes of the commodity indicated by the title of this specification, or those which are commercially available, but is intended to cover the dental template which is normally procured to meet Military requirements.

Custodians:
Army - MD
Navy - MS
Air Force - 03

Preparing activity:
Defense Supply Agency - DM

Review activities:
Army - MD
Navy - MS
Air Force - 03

Review information is current as of the date of this document. For future coordination of changes to this document, draft circulation should be based on the information in the current DODISS.

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.

SPECIFICATION ANALYSIS SHEET

Form Approved
Budget Bureau No. 22-R255

INSTRUCTIONS: This sheet is to be filled out by personnel, either Government or contractor, involved in the use of the specification in procurement of products for ultimate use by the Department of Defense. This sheet is provided for obtaining information on the use of this specification which will insure that suitable products can be procured with a minimum amount of delay and at the least cost. Comments and the return of this form will be appreciated. Fold on lines on reverse side, staple in corner, and send to preparing activity. Comments and suggestions submitted on this form do not constitute or imply authorization to waive any portion of the referenced document (s) or serve to amend contractual requirements.

SPECIFICATION: MIL-T-36631 FSN:

ORGANIZATION

CITY AND STATE | CONTRACT NUMBER

MATERIAL PROCURED UNDER A

☐ DIRECT GOVERNMENT CONTRACT ☐ SUBCONTRACT

1. HAS ANY PART OF THE SPECIFICATION CREATED PROBLEMS OR REQUIRED INTERPRETATION IN PROCUREMENT USE?

a. GIVE PARAGRAPH NUMBER AND WORDING.

b. RECOMMENDATIONS FOR CORRECTING THE DEFICIENCIES

2. COMMENTS ON ANY SPECIFICATION REQUIREMENT CONSIDERED TOO RIGID

3. IS THIS SPECIFICATION RESTRICTIVE?

☐ ☐ NO (If "yes", in what way?)

REMARKS (Attach any pertinent data which may be of use in improving this specification. If there are additional papers, attach to form and place both in an envelope addressed to preparing activity)

SUBMITTED BY (Printed or typed name and activity - Optional) | DATE

DD FORM 1426 REPLACES EDITION OF 1 OCT 64, WHICH MAY BE USED.

Source: https://assist.dla.mil -- Downloaded: 202640-21T08:56Z
Check the source to verify that this is the current version before use.

CAUTION

NOTICE TO BIDDERS/OFFERORS

DO NOT CONDITION OR BASE YOUR BID/OFFER ON ANY CURRENT PROCUREMENT ON THE **INFORMATION** SUBMITTED ON THIS FORM SINCE ANY CHANGES OR DELETIONS IN THE **SPECIFICATIONS** MAY RENDER YOUR BID/OFFER NON-RESPONSIVE IN WHICH CASE IT CAN-**NOT BE** CONSIDERED FOR AWARD.

DEFENSE PERSONNEL SUPPORT CENTER
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DEFENSE SUPPLY AGENCY
OFFICIAL BUSINESS

POSTAGE AND FEES PAID
DEFENSE SUPPLY AGENCY

HEADQUARTERS, DEFENSE PERSONNEL SUPPORT CENTER
ATTN: DIRECTORATE OF MEDICAL MATERIEL, CODE ATT
2800 SOUTH 20TH STREET
PHILADELPHIA, PA. 19101

DPSC FORM 2418 MAR 68

EDITION AUG 66, WILL BE USED UNTIL EXHAUSTED

Source: https://assist.dla.mil -- Downloaded: 2026-10-21T08:56Z
Check the source to verify that this is the current version before use.