
FED. SUP CLASS
6640

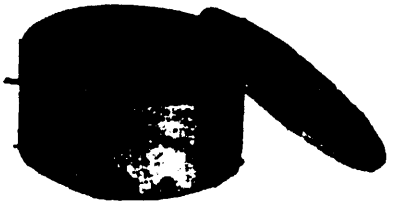

PART NUMBER	MINIMUM DIMENSIONS (MM)			OPERATING TEMPERATURE RANGE °C
	INNER CHAMBER		FLANGE WIDTH	
	DIAMETER	DEPTH		
MS36348-1	203	64	25	20 to 55 ± 1.5

MATERIAL: Interior and cover shall be 18 gauge porcelainized or enameled steel. Exterior shall be aluminum or steel. Insulated with fiberglass.

FINISH: Interior shall be finished in matte black color to insure high visibility of floating translucent tissues.

DESIGN: Water bath shall be designed for the purpose of preparing tissue specimens in histological processing and for spreading and water flotation of tissue ribbons preparatory to mounting.

Instruments and controls include on-off switch, red pilot light and thermo-regulator capable of controlling a pre-set temperature within ± 1.5°C.

A cover shall be included with the bath. The bath shall be fitted with a 3 wire power cord having a grounding type plug.

Bath shall be double-walled, suitably insulated to conserve heat and to permit comfortable handling.

The flange surface shall be horizontal to support micro-slides while drying.

Water bath shall be capable of operation on 115 volts, 50/60 Hz approximately 150 watts.

All electrical components shall conform to the standards of Underwriters Laboratories, Incorporated.

NOTES:
1. Items differing from this Military Standard by minor variations in design or dimensions are considered standard under this document, provided such variations do not affect performance and are not in conflict with the material requirements specified herein.
2. FSCM: 20512, 22527, 59728, and 95632.

(A) ENTIRE STANDARD REVISED

APPROVED 9 Sept 1963 REVISED (A) 16 JAN 1984

USER ACTIVITIES: ARMY - MD, DM
NAVY - MS

REVIEWER ACTIVITIES: ARMY - ME
AIR FORCE - 82

This military standard is approved for use by all Departments and Agencies of the Department of Defense. Selection for all new engineering and design applications and for repetitive use shall be made from this document.

P.A.	FA	INTERNATIONAL INTEREST	TITLE	MILITARY STANDARD
Other Cust	MS 99		WATER BATH, ELECTRIC, HISTOLOGICAL	MS36348
Procurement Specifications: NONE		SUPERSEDES:		SHEET 1 OF 1

DD FORM 672 (COORDINATED) PREVIOUS EDITIONS OF THIS FORM ARE OBSOLETE.

PROJECT NUMBER 6640-1210

Source: https://assist.dla.mil -- Downloaded: 2026-10-23T17:39Z
Check the source to verify that this is the current version before use.